

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
 Data File : VV006710.D
 Acq On : 26 Jul 2018 17:56
 Operator : SY/MD
 Sample : J4148-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW9

Quant Time: Jul 27 01:15:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 27 00:52:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	245281	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	228839	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	95767	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	92807	7.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	145.40%#
7) Chloroethane-d5	1.58	69	64702	6.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	129.20%
11) 1,1-Dichloroethene-d2	2.13	63	121266	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.80%
20) 2-Butanone-d5	3.97	46	208859	52.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.72%
24) Chloroform-d	4.41	84	144921	6.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.00%
26) 1,2-Dichloroethane-d4	5.09	65	74016	6.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.80%
32) Benzene-d6	5.10	84	313630	6.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	133.40%#
36) 1,2-Dichloropropane-d6	6.12	67	99187	6.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	124.80%
41) Toluene-d8	7.37	98	267165	6.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	129.80%
43) trans-1,3-Dichloropropene-	7.67	79	31294	6.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	120.60%
46) 2-Hexanone-d5	8.14	63	163849	49.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.82%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	68079	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	94235	6.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	132.00%#


Target Compounds					Ovalue
13) Acetone	2.21	43	7331	2.89 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072618\
Data File : VV006710.D
Acq On : 26 Jul 2018 17:56
Operator : SY/MD
Sample : J4148-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SW9

Quant Time: Jul 27 01:15:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 27 00:52:23 2018
Response via : Initial Calibration

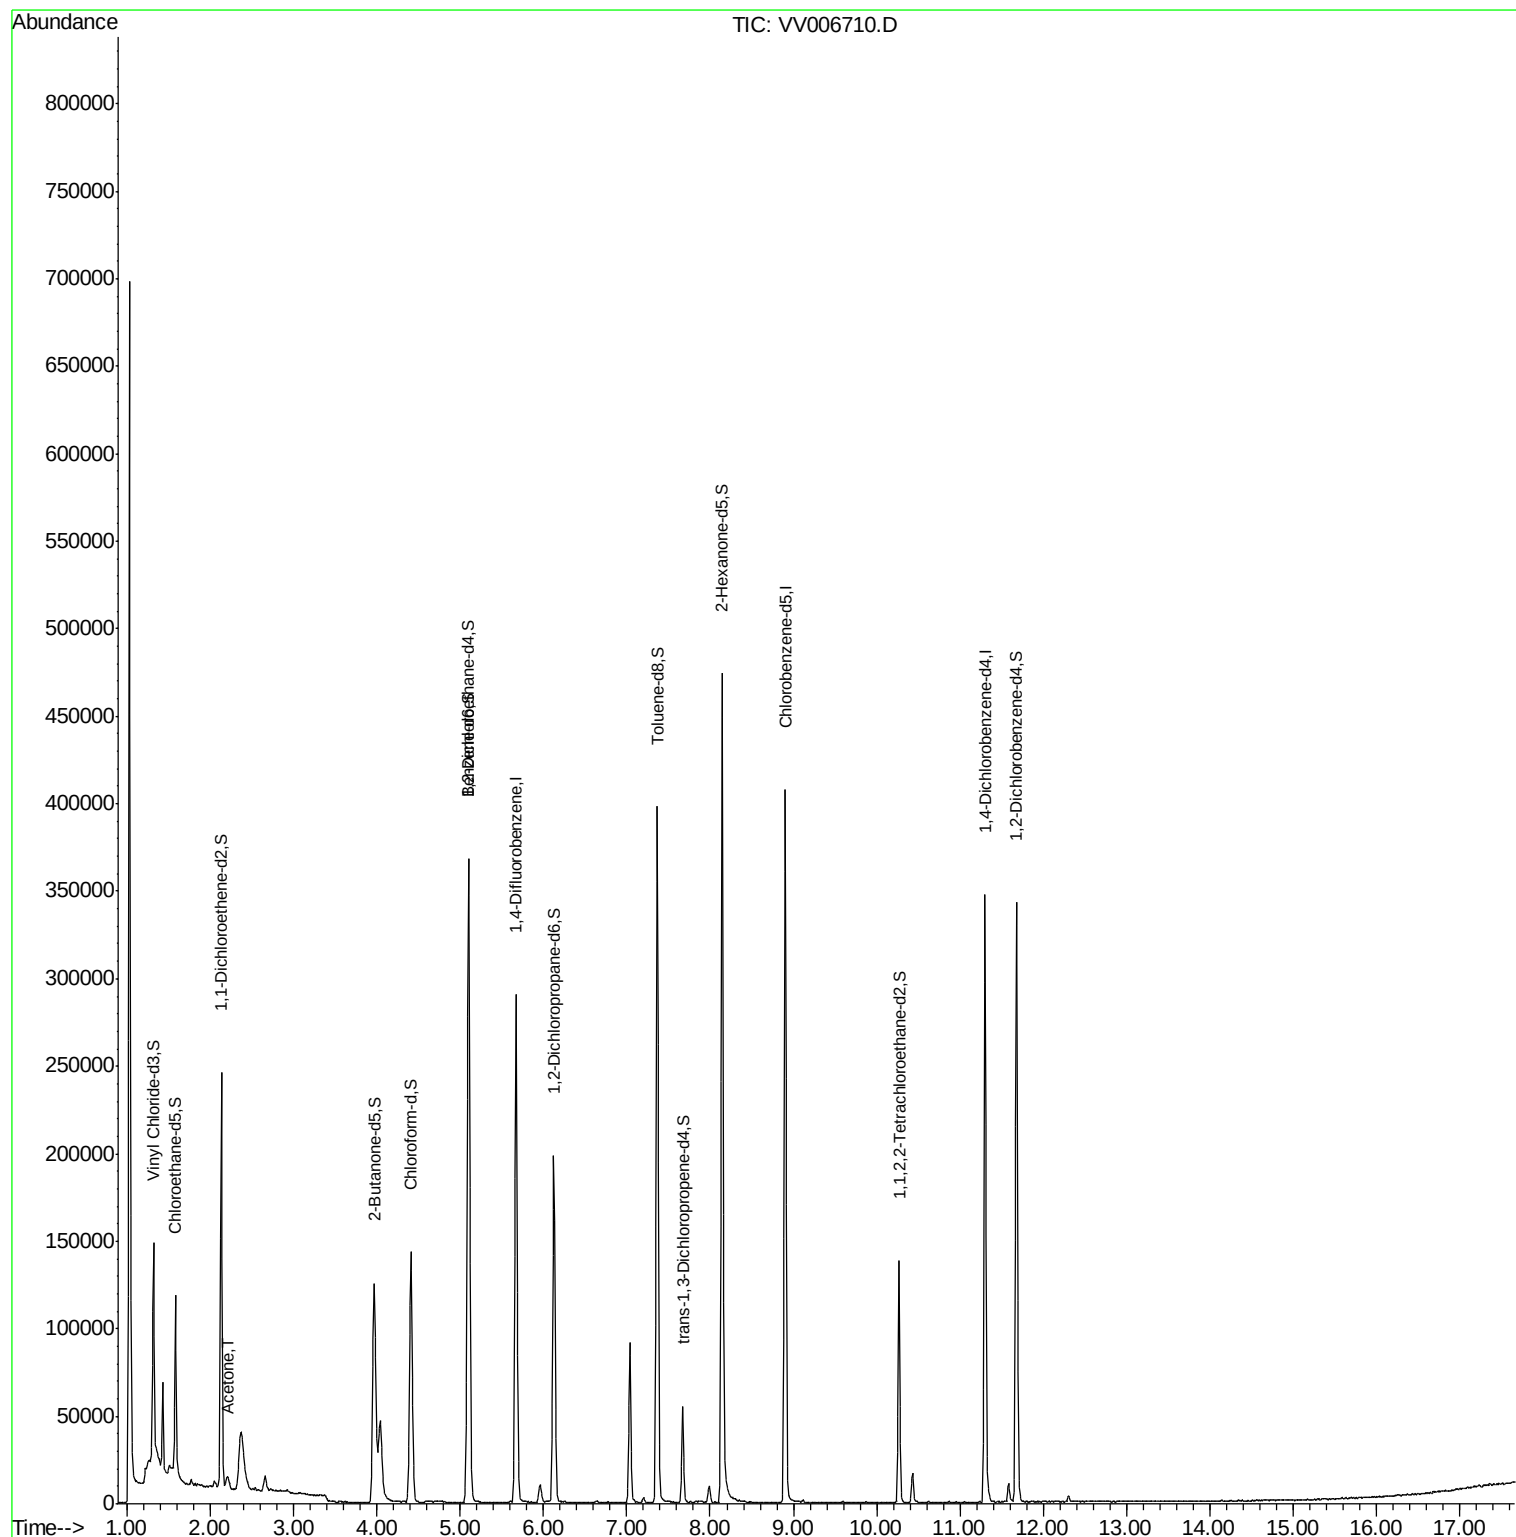

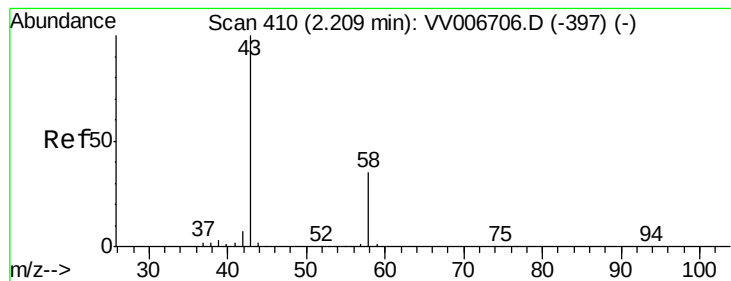

#13
 Acetone
 Concen: 2.89 ug/L
 RT: 2.21 min Scan# 410
 Delta R.T. 0.00 min
 Lab File: VV006710.D
 Acq: 26 Jul 2018 17:56

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SW9

Tot Ion: 43 Resp: 7331
 Ion Ratio Lower Upper
 43 100
 58 38.0 0.0 71.4

