

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
 Data File : VV006714.D
 Acq On : 26 Jul 2018 19:44
 Operator : SY/MD
 Sample : J4190-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE742

Quant Time: Jul 27 01:23:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 27 00:52:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	242816	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	224977	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	92550	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	84575	6.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	133.80%#
7) Chloroethane-d5	1.58	69	59940	6.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.80%
11) 1,1-Dichloroethene-d2	2.13	63	111490	4.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.00%
20) 2-Butanone-d5	3.96	46	199517	50.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.06%
24) Chloroform-d	4.41	84	136827	5.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.40%
26) 1,2-Dichloroethane-d4	5.09	65	69425	6.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.00%
32) Benzene-d6	5.10	84	292118	6.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	126.40%#
36) 1,2-Dichloropropane-d6	6.12	67	93481	5.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	119.60%
41) Toluene-d8	7.37	98	249241	6.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.20%
43) trans-1,3-Dichloropropene-	7.67	79	29276	5.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	114.80%
46) 2-Hexanone-d5	8.14	63	157958	48.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	66683	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	88837	6.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	128.80%#


Target Compounds					Ovalue
13) Acetone	2.21	43	5039	2.01 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072618\
Data File : VV006714.D
Acq On : 26 Jul 2018 19:44
Operator : SY/MD
Sample : J4190-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE742

Quant Time: Jul 27 01:23:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 27 00:52:23 2018
Response via : Initial Calibration

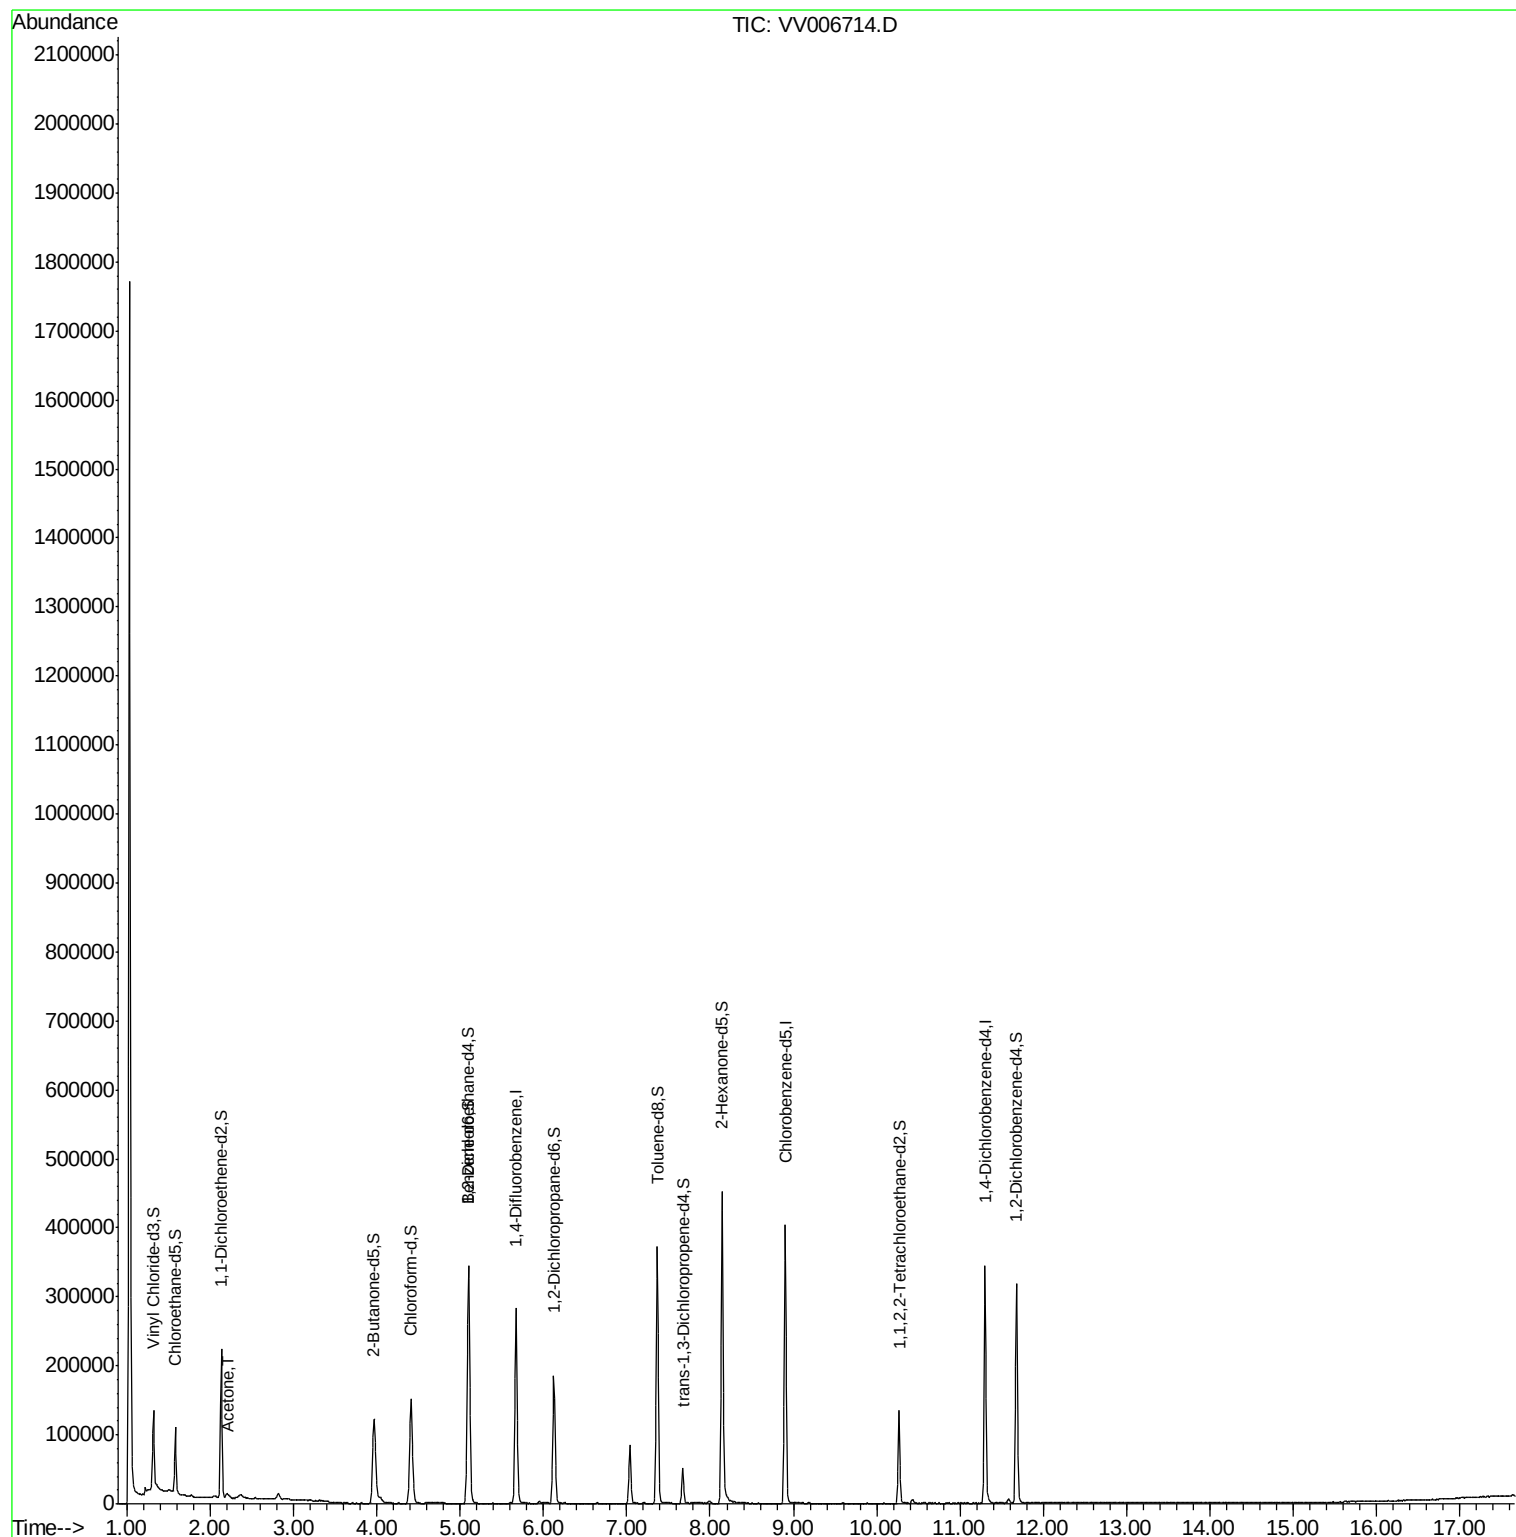

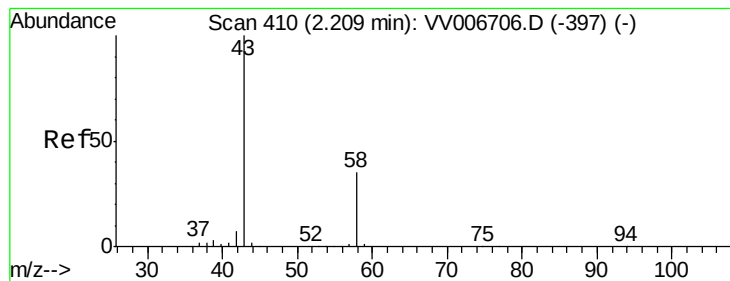

#13
 Acetone
 Concen: 2.01 ug/L
 RT: 2.21 min Scan# 409
 Delta R.T. -0.00 min
 Lab File: VV006714.D
 Acq: 26 Jul 2018 19:44

Instrument :
 MSVOA_V
 ClientSampleId :
 BE742

Tot Ion: 43 Resp: 5039
 Ion Ratio Lower Upper
 43 100
 58 38.3 0.0 71.4

