

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
 Data File : VV006715.D
 Acq On : 26 Jul 2018 20:11
 Operator : SY/MD
 Sample : J4190-03
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE743

Quant Time: Jul 27 01:27:24 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 27 00:52:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	247908	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	227646	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	92952	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	84686	6.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	131.20%#
7) Chloroethane-d5	1.58	69	62904	6.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	124.20%
11) 1,1-Dichloroethene-d2	2.13	63	112244	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.60%
20) 2-Butanone-d5	3.96	46	201474	49.98	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.96%
24) Chloroform-d	4.41	84	139351	5.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.20%
26) 1,2-Dichloroethane-d4	5.09	65	70872	6.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.00%
32) Benzene-d6	5.10	84	297848	6.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.40%#
36) 1,2-Dichloropropane-d6	6.12	67	94019	5.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	119.00%
41) Toluene-d8	7.37	98	251326	6.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.80%
43) trans-1,3-Dichloropropene-	7.67	79	30093	5.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	116.60%
46) 2-Hexanone-d5	8.14	63	159637	48.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	67317	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	89003	6.42	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	128.40%#


Target Compounds					Ovalue
13) Acetone	2.20	43	20058	7.82 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
Data File : VV006715.D
Acq On : 26 Jul 2018 20:11
Operator : SY/MD
Sample : J4190-03
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE743

Quant Time: Jul 27 01:27:24 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 27 00:52:23 2018
Response via : Initial Calibration

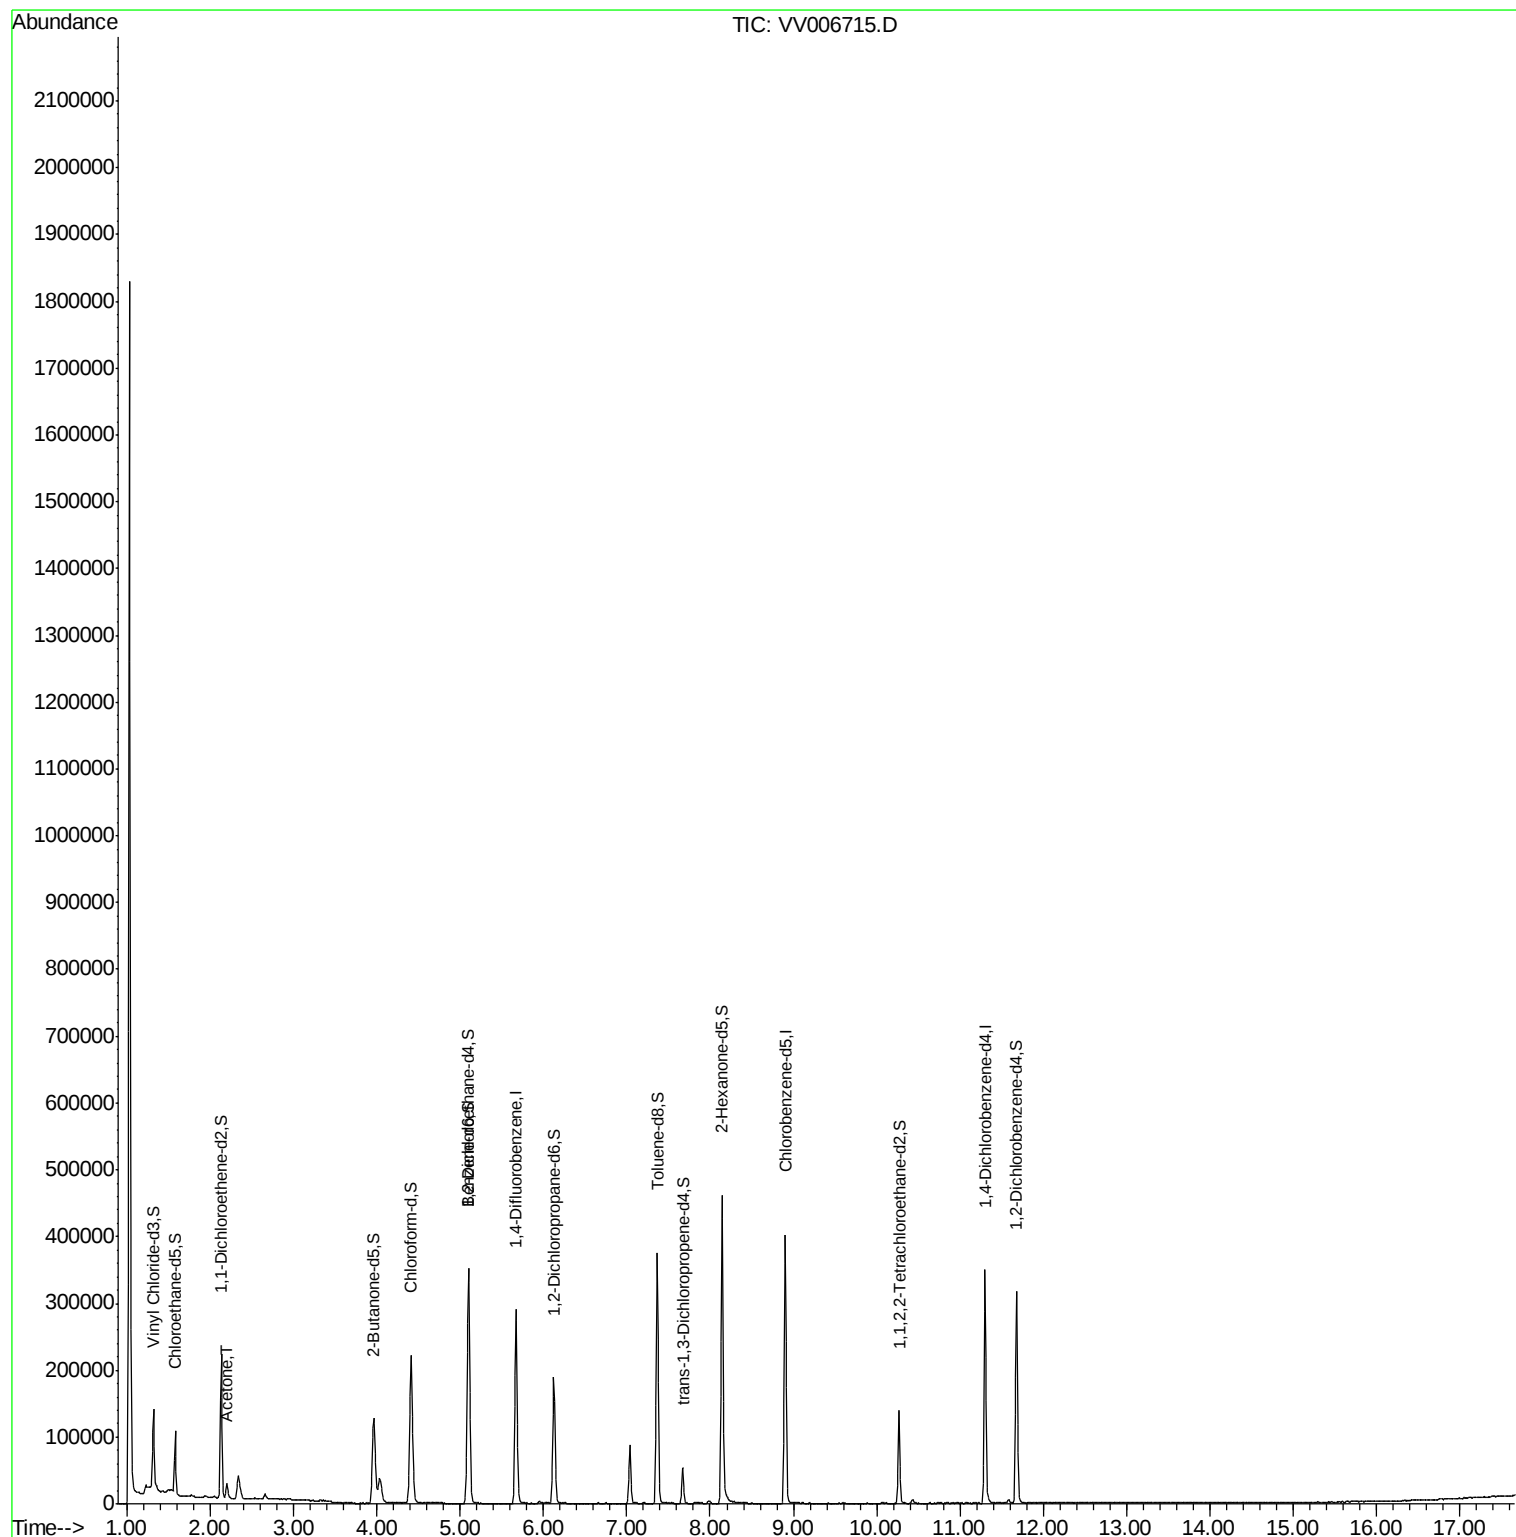

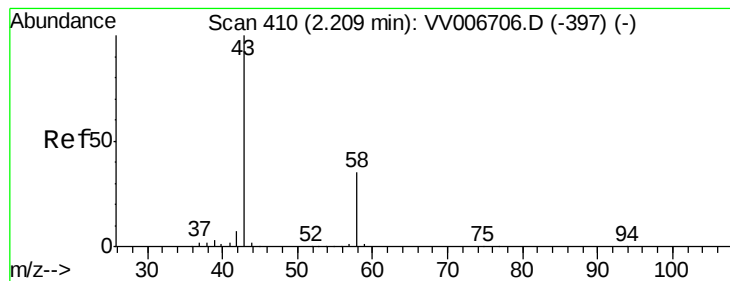

#13
 Acetone
 Concen: 7.82 ug/L
 RT: 2.20 min Scan# 407
 Delta R.T. -0.01 min
 Lab File: VV006715.D
 Acq: 26 Jul 2018 20:11

Instrument :
 MSVOA_V
 ClientSampleId :
 BE743

Tot Ion: 43 Resp: 20058
 Ion Ratio Lower Upper
 43 100
 58 36.7 0.0 71.4

