


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072618\
Data File : VV006705.D
Acq On : 26 Jul 2018 09:59
Operator : SY/MD
Sample : BFB71
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jul 30 14:38:46 2018

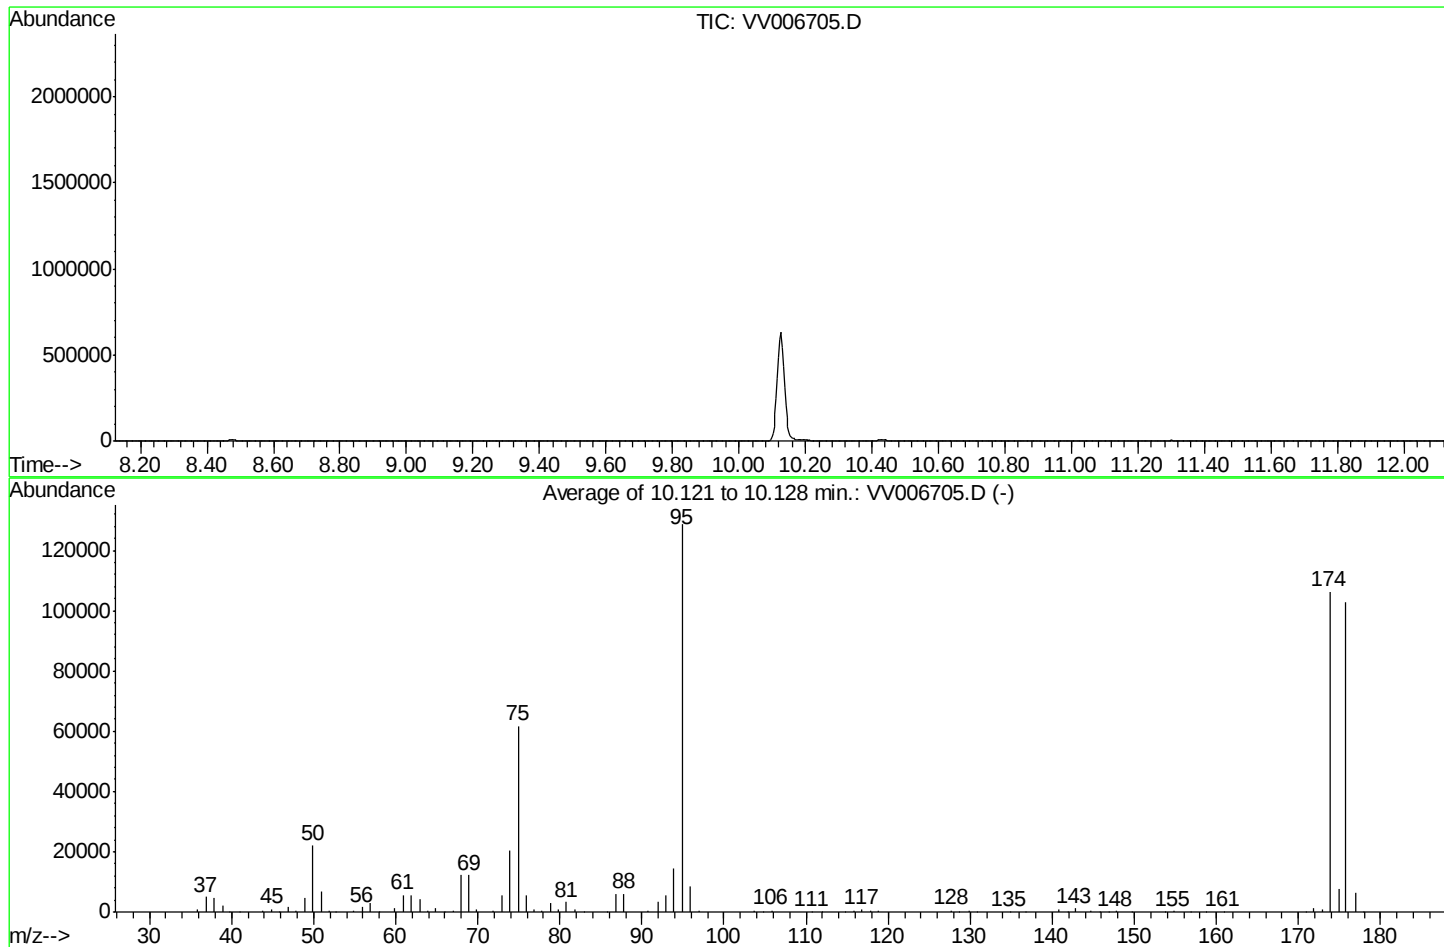

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	21952	PASS
75	95	30	80	48.1	61821	PASS
95	95	100	100	100.0	128648	PASS
96	95	5	9	6.8	8712	PASS
173	174	0.00	2	0.9	923	PASS
174	95	50	120	82.7	106368	PASS
175	174	5	9	7.1	7577	PASS
176	174	95	101	96.6	102760	PASS
177	176	5	9	6.3	6500	PASS

Scan 2857 (10.076 min): VV006705.D
BFB71

m/z	Abundance
39.80	231.0
43.80	563.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	876.0
36.90	4963.0
37.90	4528.0
38.90	2118.0
39.90	289.0
43.90	1040.0
44.90	963.0
46.80	1828.0
47.90	706.0
48.90	4492.0
49.90	21256.0
50.90	6781.0
52.00	254.0
54.90	330.0
55.90	1538.0
56.90	3017.0
57.90	154.0
59.90	1070.0
60.90	5460.0
61.90	5353.0
62.90	4228.0
63.90	650.0
64.90	1062.0
66.90	288.0
67.90	11716.0
68.90	11926.0
69.90	1031.0
71.90	587.0
72.90	5304.0
73.90	19976.0
74.90	60200.0
75.90	5410.0
76.90	825.0
77.80	565.0
78.80	3109.0
79.80	933.0
80.80	3294.0
81.80	715.0
85.80	197.0
86.80	5630.0
87.80	5681.0
90.80	412.0
91.90	3141.0
92.90	5245.0
93.90	13842.0
94.90	123832.0
96.00	8658.0
97.00	238.0
103.70	354.0
104.70	145.0
105.80	443.0
114.70	110.0
115.80	455.0
116.80	734.0
117.80	353.0
118.80	642.0
127.70	562.0
128.70	145.0
129.80	356.0
130.70	183.0
134.80	201.0
136.80	157.0
140.80	904.0
141.90	113.0
142.80	1164.0
144.70	209.0
145.70	155.0
147.80	259.0
149.70	122.0
154.80	300.0
156.80	227.0
158.80	149.0
160.90	117.0
170.90	105.0
171.80	1191.0
172.80	823.0
173.80	99056.0
174.90	7008.0
175.80	95824.0
176.90	6244.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	942.0
36.90	5156.0
37.90	4927.0
38.90	2206.0
39.80	329.0
40.90	105.0
43.90	1103.0
44.90	1016.0
46.90	1927.0
47.90	664.0
48.90	4732.0
49.90	22744.0
50.90	7199.0
52.00	239.0
52.60	111.0
54.90	380.0
55.90	1669.0
56.90	3274.0
57.90	210.0
59.90	1168.0
60.90	5860.0
61.90	5788.0
62.90	4432.0
63.90	632.0
64.90	1167.0
65.90	111.0
67.00	322.0
67.90	12693.0
68.90	12686.0
69.90	1038.0
71.90	635.0
72.90	5768.0
73.90	21152.0
74.90	64224.0
75.90	5743.0
76.90	926.0
77.70	610.0
78.80	3267.0
79.80	963.0
80.80	3322.0
81.80	779.0
85.70	218.0
86.80	5979.0
87.80	6263.0
90.80	423.0
91.90	3425.0
92.90	5602.0
93.90	15006.0
94.90	133184.0
96.00	8965.0
96.90	232.0
103.80	419.0
104.80	179.0
105.90	467.0
110.70	108.0
114.70	126.0
115.80	494.0
116.80	826.0
117.80	374.0
118.90	676.0
127.70	568.0
128.70	159.0
129.80	392.0
130.70	202.0
134.80	206.0
136.80	169.0
140.80	1059.0
141.80	128.0
142.80	1229.0
144.70	248.0
145.70	150.0
147.80	275.0
149.70	125.0
154.80	310.0
156.80	223.0
158.70	147.0
160.90	130.0
170.90	112.0
171.80	1382.0
172.80	946.0
173.90	110232.0
174.90	7877.0
175.80	106568.0
176.90	6736.0
177.90	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	895.0
36.90	4861.0
37.90	4746.0
38.90	2017.0
39.80	349.0
43.90	1157.0
44.90	947.0
45.80	109.0
46.90	1846.0
47.80	588.0
48.90	4506.0
49.90	21856.0
50.90	6946.0
51.90	222.0
52.60	121.0
54.90	409.0
55.90	1605.0
56.90	3144.0
57.90	203.0
59.90	1142.0
60.90	5779.0
61.90	5610.0
62.90	4286.0
63.80	562.0
64.90	1099.0
65.90	120.0
66.90	293.0
67.90	12192.0
68.90	12313.0
69.90	950.0
71.90	608.0
72.90	5453.0
73.90	20136.0
74.90	61040.0
75.90	5518.0
76.90	940.0
77.70	622.0
78.90	3152.0
79.80	901.0
80.80	3064.0
81.80	794.0
83.00	121.0
85.70	230.0
86.90	5780.0
87.80	5963.0
90.80	394.0
91.90	3404.0
92.90	5315.0
93.90	14762.0
94.90	128928.0
95.90	8514.0
96.90	227.0
103.80	452.0
104.80	194.0
105.80	432.0
110.70	109.0
111.90	116.0
114.80	134.0
115.80	451.0
116.80	810.0
117.80	366.0
118.90	641.0
127.70	521.0
128.70	162.0
129.80	399.0
130.80	200.0
134.80	201.0
136.70	161.0
140.80	1143.0
141.80	152.0
142.80	1207.0
144.70	246.0
145.80	140.0
146.80	134.0
147.70	267.0
149.80	128.0
153.70	102.0
154.80	286.0
156.80	204.0
158.70	131.0
160.90	133.0
171.80	1405.0
172.90	1001.0
173.90	109816.0
174.90	7848.0
175.80	105888.0
176.90	6520.0
177.90	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71