


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072619\  
 Data File : VV012040.D  
 Acq On : 26 Jul 2019 08:47  
 Operator : SY/MD  
 Sample : BFB39  
 Misc : 25ML/MSVOA V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR072219WMA.M  
 Title : TRACE VOA SOM01.0  
 Last Update : Fri Jul 26 23:19:45 2019

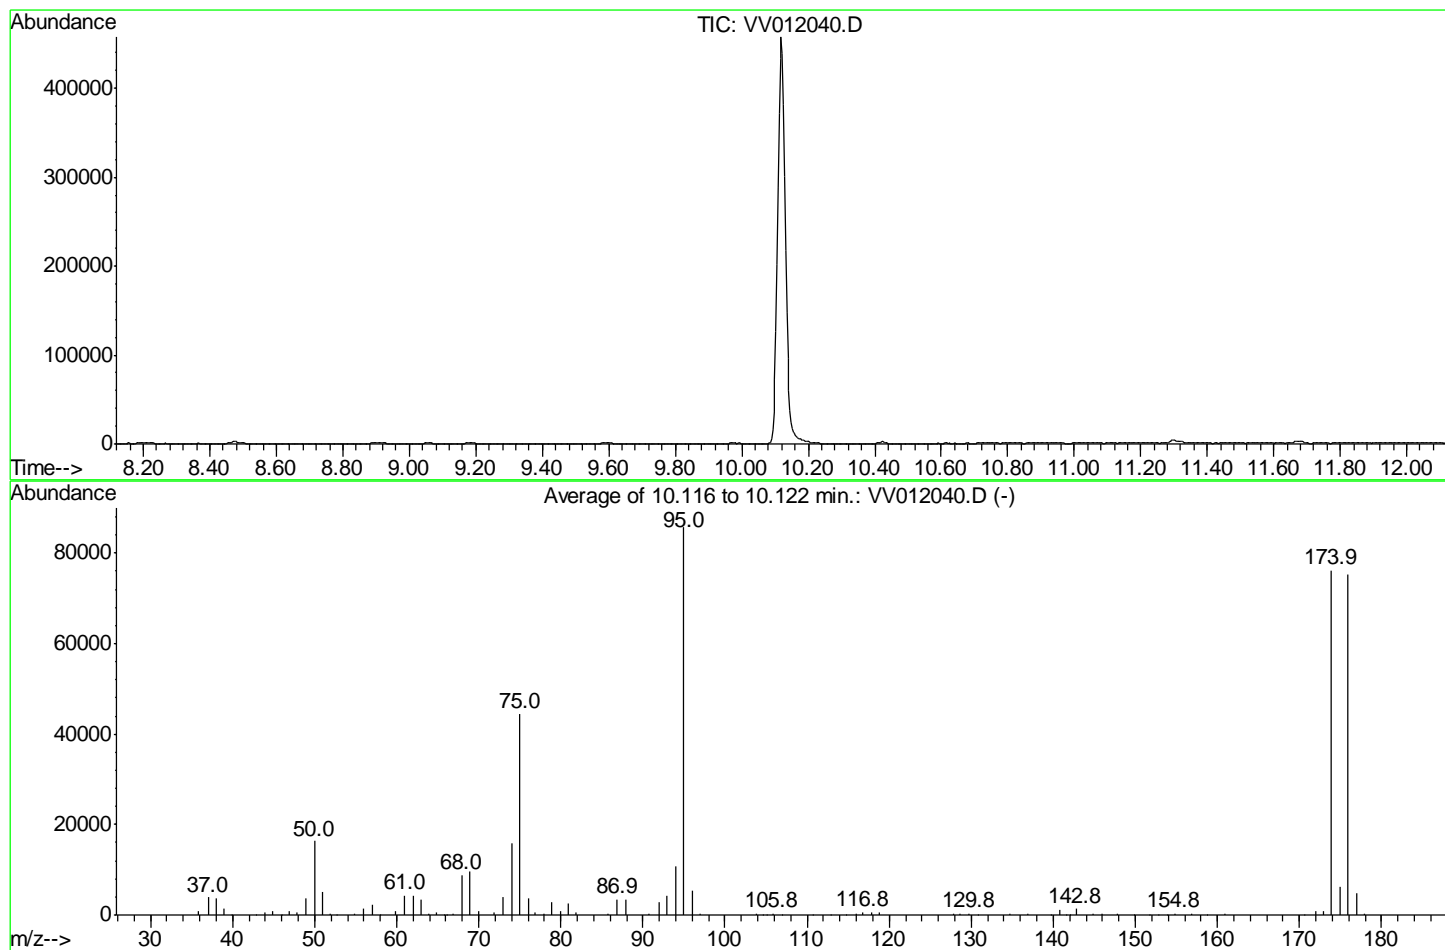

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	16326	PASS
75	95	30	80	51.9	44498	PASS
95	95	100	100	100.0	85685	PASS
96	95	5	9	6.4	5441	PASS
173	174	0.00	2	1.0	779	PASS
174	95	50	120	88.9	76160	PASS
175	174	5	9	8.1	6164	PASS
176	174	95	101	98.6	75130	PASS
177	176	5	9	6.5	4858	PASS

Scan 2794 (10.074 min): VV012040.D  
BFB39

m/z	Abundance
39.90	172.0
43.90	240.0

**Instrument :**  
MSVOA\_V  
**ClientSampleId :**  
BFB39

m/z	Abundance
35.90	885.0
37.00	4030.0
38.00	3693.0
38.90	1486.0
40.00	214.0
42.80	124.0
43.90	681.0
44.90	773.0
46.10	132.0
46.90	971.0
47.90	687.0
49.00	3547.0
50.00	16202.0
50.90	5173.0
51.90	243.0
55.00	253.0
55.90	1457.0
57.00	2282.0
57.90	106.0
60.00	729.0
61.00	4305.0
62.00	4158.0
63.00	3562.0
63.90	459.0
64.80	566.0
65.80	138.0
66.90	256.0
67.90	8814.0
69.00	9550.0
70.00	789.0
71.90	600.0
72.90	4115.0
74.00	15455.0
75.00	44128.0
76.00	3909.0
76.90	578.0
78.00	384.0
78.90	2775.0
79.90	873.0
80.90	2725.0
81.80	644.0
85.80	216.0
86.90	3331.0
87.80	3362.0
90.80	352.0
91.90	2628.0
92.90	4181.0
94.00	10546.0
95.00	83496.0
96.00	5535.0
97.00	205.0
103.80	430.0
104.70	114.0
105.00	107.0
105.80	470.0
107.00	122.0
110.80	101.0
112.80	134.0
114.80	128.0
116.00	321.0
116.80	680.0
117.90	464.0
118.90	559.0
127.80	343.0
128.70	159.0
129.70	329.0
130.80	117.0
134.70	288.0
136.90	167.0
139.70	117.0
140.90	984.0
142.80	1235.0
144.80	299.0
145.90	188.0
147.80	237.0
154.80	276.0
156.90	197.0
160.90	209.0
170.60	141.0
171.90	839.0
173.00	1226.0
173.90	72664.0
174.90	6173.0
175.90	71848.0
176.90	4899.0
177.90	165.0

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB39

m/z	Abundance
35.90	910.0
37.00	3958.0
38.00	3830.0
39.00	1538.0
40.00	209.0
43.90	769.0
45.00	892.0
45.90	141.0
47.00	926.0
47.80	692.0
49.00	3756.0
50.00	16856.0
50.90	5280.0
51.90	245.0
52.70	110.0
54.90	203.0
55.90	1472.0
57.00	2366.0
57.90	122.0
59.80	798.0
61.00	4390.0
62.00	4427.0
63.00	3599.0
64.00	436.0
64.90	541.0
65.70	113.0
66.90	281.0
67.90	9147.0
68.90	9909.0
70.00	802.0
71.90	631.0
72.90	4206.0
74.00	16367.0
75.00	45704.0
76.00	3909.0
76.90	619.0
78.00	401.0
78.90	3021.0
79.90	897.0
80.90	2750.0
81.80	690.0
85.80	262.0
86.90	3710.0
87.90	3531.0
90.80	393.0
91.90	2787.0
92.90	4274.0
94.00	11140.0
95.00	88496.0
96.00	5557.0
97.00	200.0
103.90	423.0
104.60	118.0
105.80	428.0
106.90	132.0
110.70	103.0
112.80	140.0
116.00	349.0
116.90	681.0
117.90	470.0
118.80	554.0
127.90	327.0
128.70	177.0
129.80	345.0
130.90	115.0
134.80	284.0
136.90	228.0
139.80	127.0
140.80	1046.0
142.80	1482.0
144.90	325.0
145.90	212.0
147.80	221.0
151.70	106.0
152.80	118.0
153.90	120.0
154.80	314.0
156.90	225.0
158.70	116.0
160.90	197.0
170.50	155.0
172.00	949.0
173.00	1112.0
173.90	78592.0
174.90	6373.0
175.90	77824.0
176.90	5009.0
177.90	156.0

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB39

m/z	Abundance
35.90	789.0
37.00	3731.0
38.00	3580.0
39.00	1471.0
40.00	222.0
43.90	796.0
45.00	890.0
45.90	141.0
47.00	847.0
47.80	609.0
49.00	3611.0
50.00	15920.0
51.00	4924.0
51.90	223.0
52.70	114.0
54.80	188.0
55.90	1305.0
57.00	2325.0
57.90	122.0
59.80	838.0
60.90	4118.0
62.00	4328.0
63.00	3323.0
64.00	378.0
65.00	534.0
66.10	100.0
66.90	243.0
68.00	8572.0
68.90	9302.0
70.00	737.0
71.90	601.0
73.00	4006.0
74.00	15543.0
75.00	43664.0
76.00	3610.0
76.90	612.0
78.00	420.0
78.90	2863.0
79.90	857.0
80.90	2622.0
81.80	713.0
85.80	245.0
86.90	3597.0
87.90	3238.0
90.80	422.0
91.90	2834.0
92.90	3906.0
94.00	10463.0
95.00	85064.0
96.00	5233.0
97.00	201.0
103.90	391.0
104.70	107.0
105.90	357.0
106.90	138.0
112.80	132.0
115.80	340.0
116.90	647.0
117.90	424.0
118.80	590.0
127.90	294.0
128.70	195.0
129.80	380.0
130.80	130.0
134.80	233.0
136.90	262.0
139.80	122.0
140.80	1051.0
141.60	136.0
142.00	164.0
142.80	1479.0
144.90	305.0
145.90	184.0
147.70	205.0
149.90	122.0
151.60	104.0
152.80	130.0
153.90	110.0
154.80	344.0
156.90	216.0
158.80	132.0
160.80	134.0
170.50	127.0
172.00	924.0
173.90	77224.0
174.90	5948.0
175.90	75720.0
176.90	4666.0
177.90	149.0

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB39