

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026957.D
 Acq On : 26 Jul 2022 17:33
 Operator : SY/MD
 Sample : N3841-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC9

Quant Time: Jul 27 01:42:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	537715	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	536390	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	223942	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	178063	39.483	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.960%		
7) Chloroethane-d5	1.564	69	152674	41.846	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.700%		
11) 1,1-Dichloroethene-d2	2.101	63	247385	30.490	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.980%		
21) 2-Butanone-d5	3.883	46	276607	90.994	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.990%		
24) Chloroform-d	4.342	84	375140	42.266	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.540%		
26) 1,2-Dichloroethane-d4	5.027	65	223326	43.988	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.980%		
32) Benzene-d6	5.047	84	733640	45.248	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.500%		
36) 1,2-Dichloropropane-d6	6.066	67	240433	46.015	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.020%		
41) Toluene-d8	7.313	98	585942	41.303	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.600%		
43) trans-1,3-Dichloroprop...	7.622	79	93362	42.643	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.280%		
47) 2-Hexanone-d5	8.088	63	190532	83.746	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.750%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	356343	44.892	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.780%		
66) 1,2-Dichlorobenzene-d4	11.622	152	223166	53.118	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.240%		
Target Compounds					Qvalue	
13) Acetone	2.175	43	9287	4.351	ug/L	96
39) cis-1,3-Dichloropropene	6.982	75	5047	0.810	ug/L #	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026957.D
Acq On : 26 Jul 2022 17:33
Operator : SY/MD
Sample : N3841-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC9

Quant Time: Jul 27 01:42:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

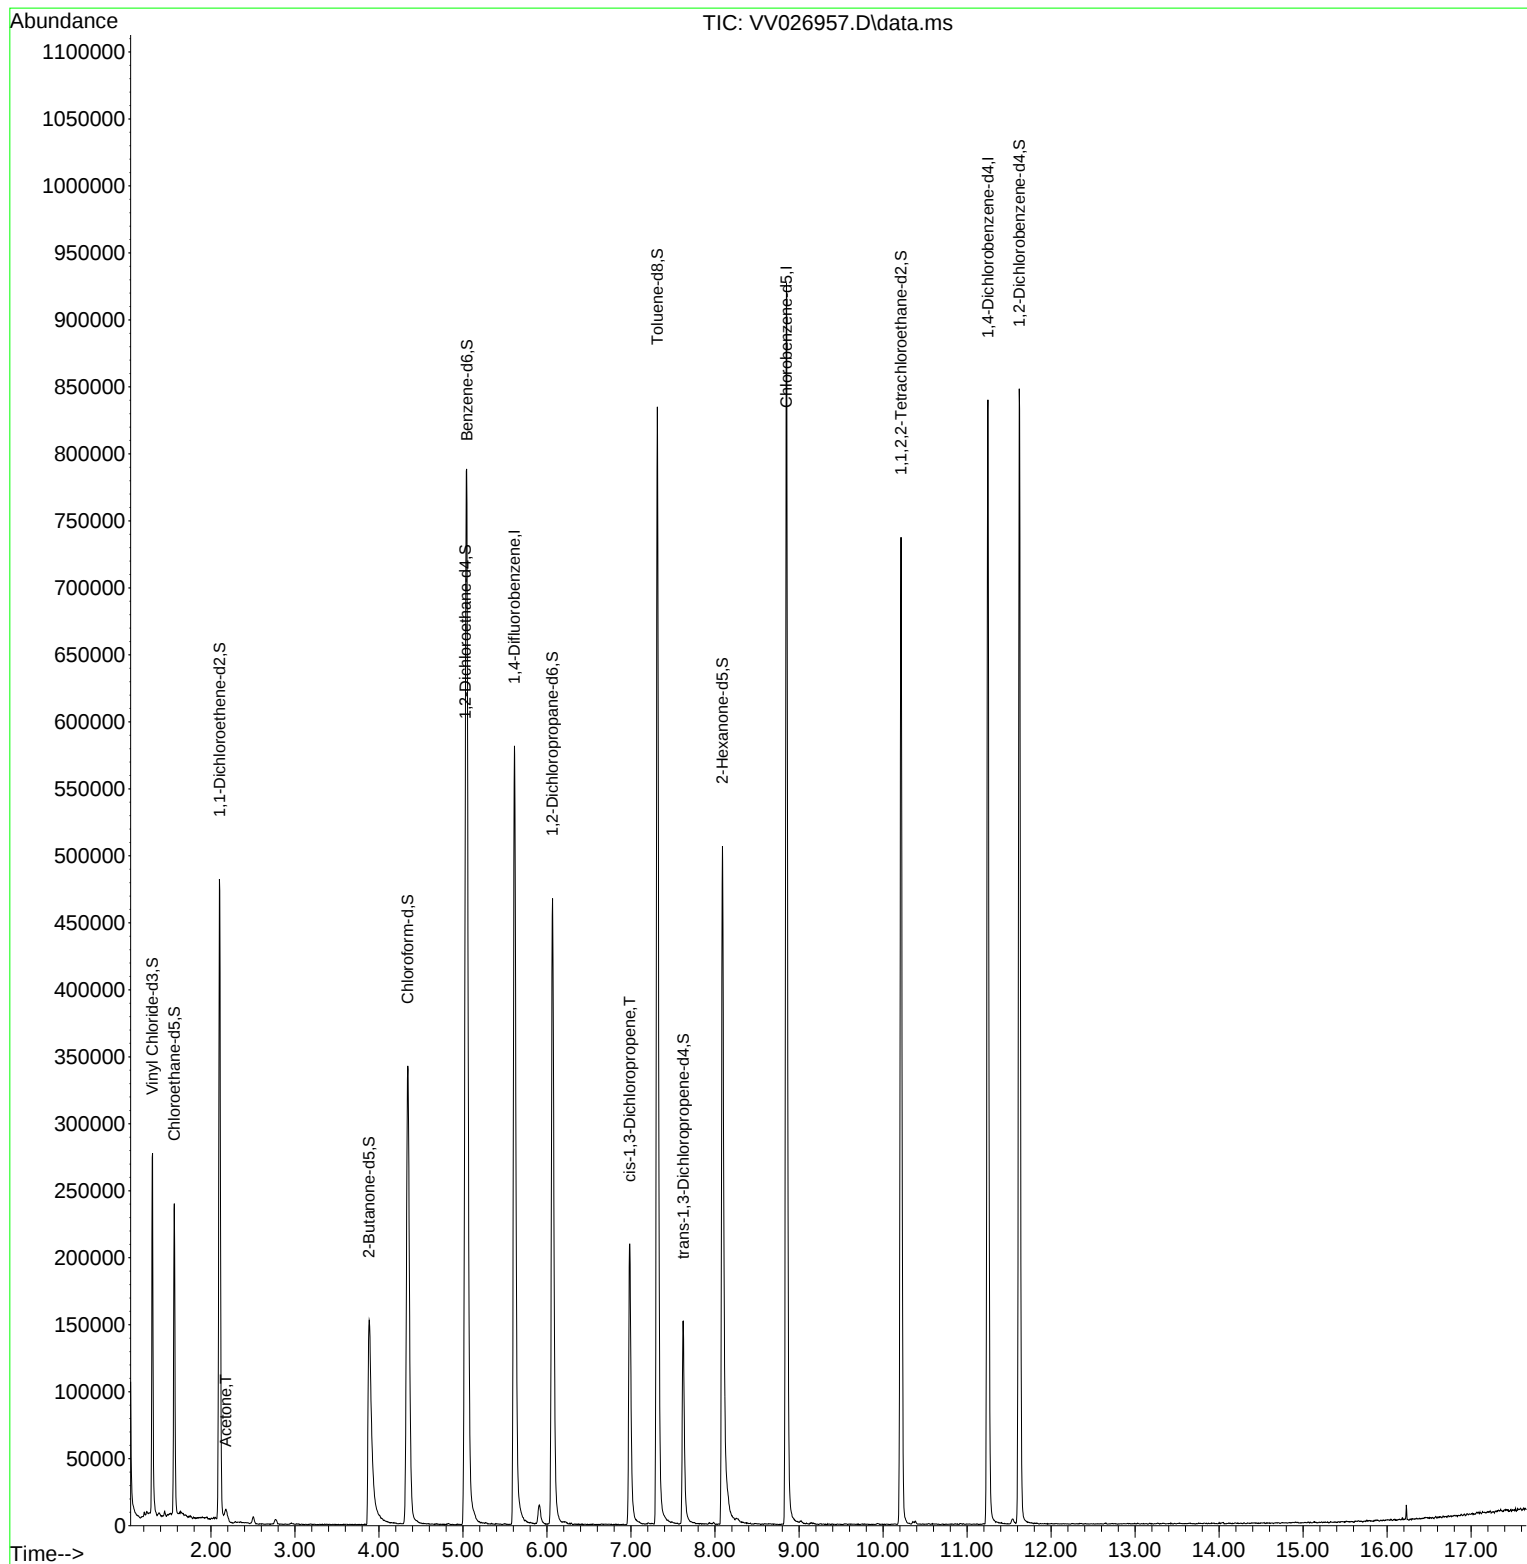

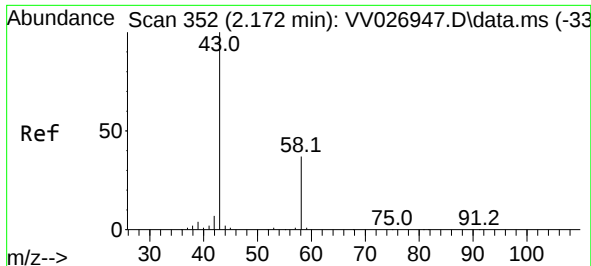

#13

Acetone

Concen: 4.351 ug/L

RT: 2.175 min Scan# 3

Delta R.T. 0.003 min

Lab File: VV026957.D

Acq: 26 Jul 2022 17:33

Instrument :

MSVOA_V

ClientSampleId :





DBUC9

Tgt Ion: 43 Resp: 9287

Ion Ratio Lower Upper

43 100

58 33.7 0.0 72.6

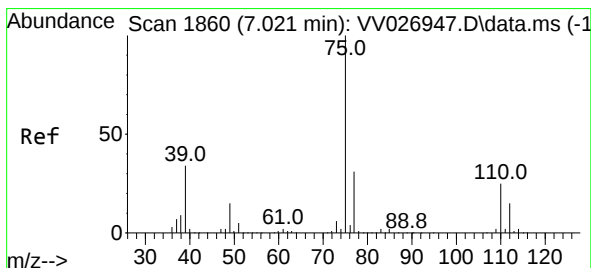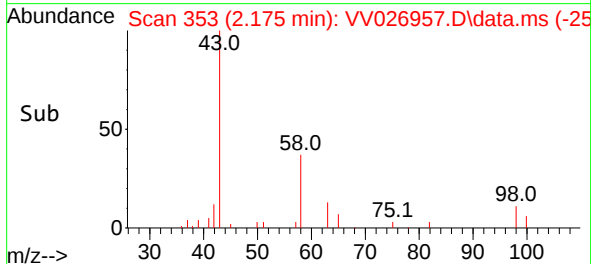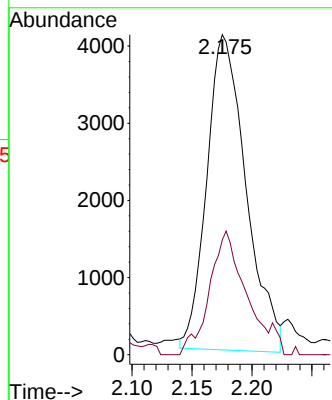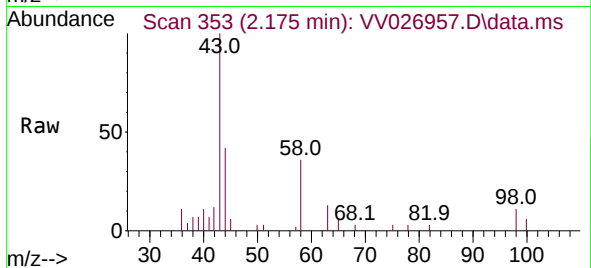

#39

cis-1,3-Dichloropropene

Concen: 0.810 ug/L

RT: 6.982 min Scan# 1848

Delta R.T. -0.039 min

Lab File: VV026957.D

Acq: 26 Jul 2022 17:33

Tgt Ion: 75 Resp: 5047

Ion Ratio Lower Upper

75 100

77 55.5 22.4 41.6#

