

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026959.D
 Acq On : 26 Jul 2022 18:22
 Operator : SY/MD
 Sample : N3841-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD1

Quant Time: Jul 27 01:43:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	500715	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	512927	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	217037	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	179830	42.821	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.640%		
7) Chloroethane-d5	1.564	69	158056	46.522	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.040%		
11) 1,1-Dichloroethene-d2	2.101	63	247468	32.754	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.500%		
21) 2-Butanone-d5	3.886	46	278409	98.354	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.350%		
24) Chloroform-d	4.342	84	382813	46.318	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.640%		
26) 1,2-Dichloroethane-d4	5.027	65	227609	48.144	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.280%		
32) Benzene-d6	5.047	84	725840	46.814	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.620%		
36) 1,2-Dichloropropane-d6	6.066	67	244224	48.878	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.760%		
41) Toluene-d8	7.313	98	582894	42.967	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.940%		
43) trans-1,3-Dichloroprop...	7.619	79	95086	45.417	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.840%		
47) 2-Hexanone-d5	8.088	63	188433	86.612	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.610%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	357155	47.053	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.100%		
66) 1,2-Dichlorobenzene-d4	11.625	152	225979	55.499	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.000%		
Target Compounds					Qvalue	
13) Acetone	2.179	43	8365	4.209	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026959.D
Acq On : 26 Jul 2022 18:22
Operator : SY/MD
Sample : N3841-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD1

Quant Time: Jul 27 01:43:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

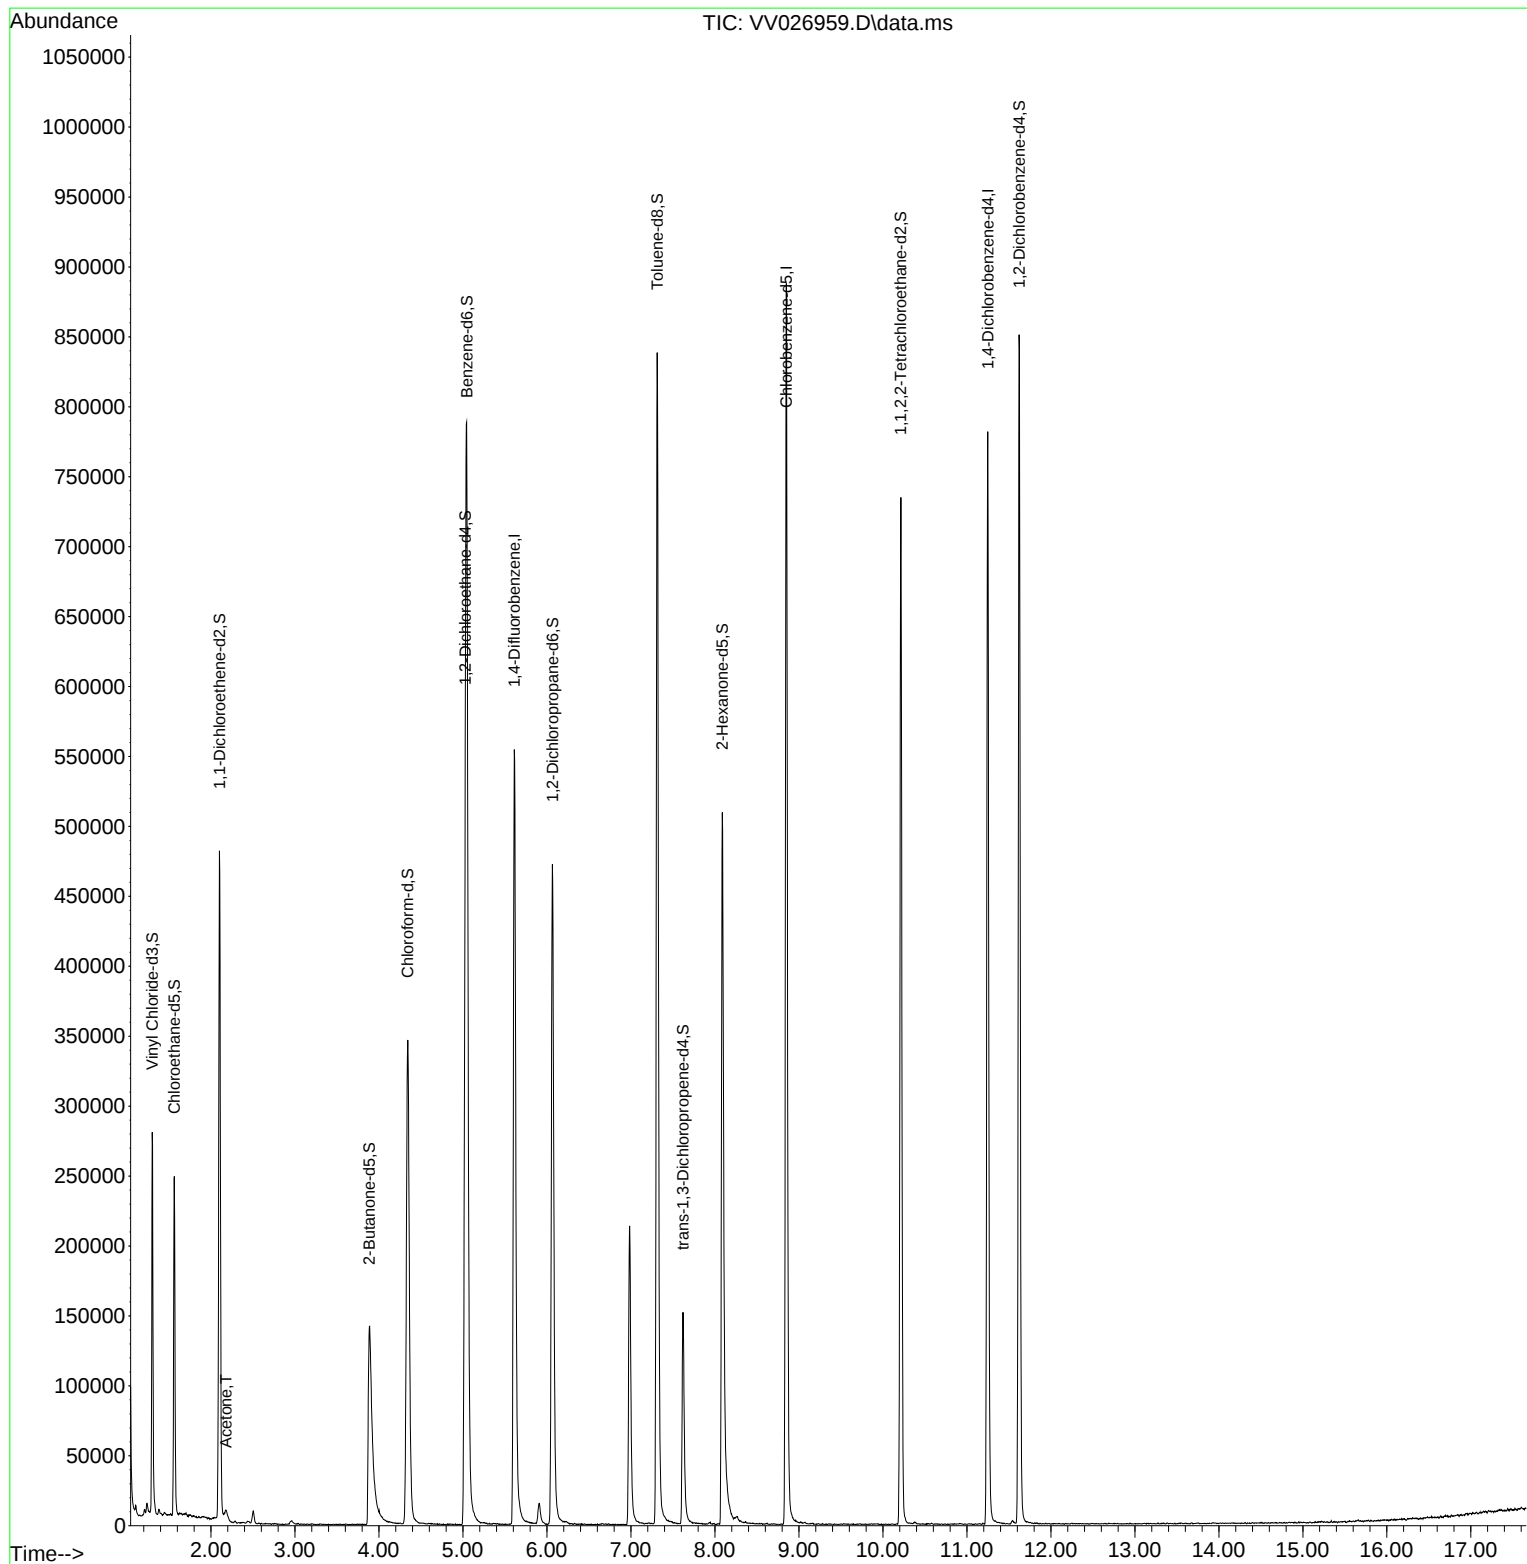

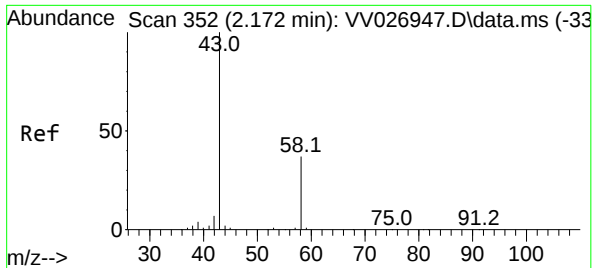

#13
 Acetone
 Concen: 4.209 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV026959.D
 Acq: 26 Jul 2022 18:22

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD1

Tgt Ion: 43 Resp: 8365
 Ion Ratio Lower Upper
 43 100
 58 36.0 0.0 72.6

