

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026964.D
 Acq On : 26 Jul 2022 20:25
 Operator : SY/MD
 Sample : N3843-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE4

Quant Time: Jul 27 01:44:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	496416	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	499519	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	205496	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	170153	40.868	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.740%
7) Chloroethane-d5	1.564	69	148318	44.034	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.060%
11) 1,1-Dichloroethene-d2	2.101	63	241697	32.267	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.540%
21) 2-Butanone-d5	3.886	46	291808	103.980	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.980%
24) Chloroform-d	4.342	84	378013	46.133	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.260%
26) 1,2-Dichloroethane-d4	5.027	65	224174	47.828	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.660%
32) Benzene-d6	5.047	84	723675	47.927	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.860%
36) 1,2-Dichloropropane-d6	6.066	67	241965	49.726	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.460%
41) Toluene-d8	7.313	98	573102	43.379	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.760%
43) trans-1,3-Dichloroprop...	7.619	79	91885	45.066	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.140%
47) 2-Hexanone-d5	8.088	63	197669	93.296	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.300%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	364621	49.326	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.660%
66) 1,2-Dichlorobenzene-d4	11.622	152	224005	58.104	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.200%
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	23388	5.672	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026964.D
Acq On : 26 Jul 2022 20:25
Operator : SY/MD
Sample : N3843-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE4

Quant Time: Jul 27 01:44:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

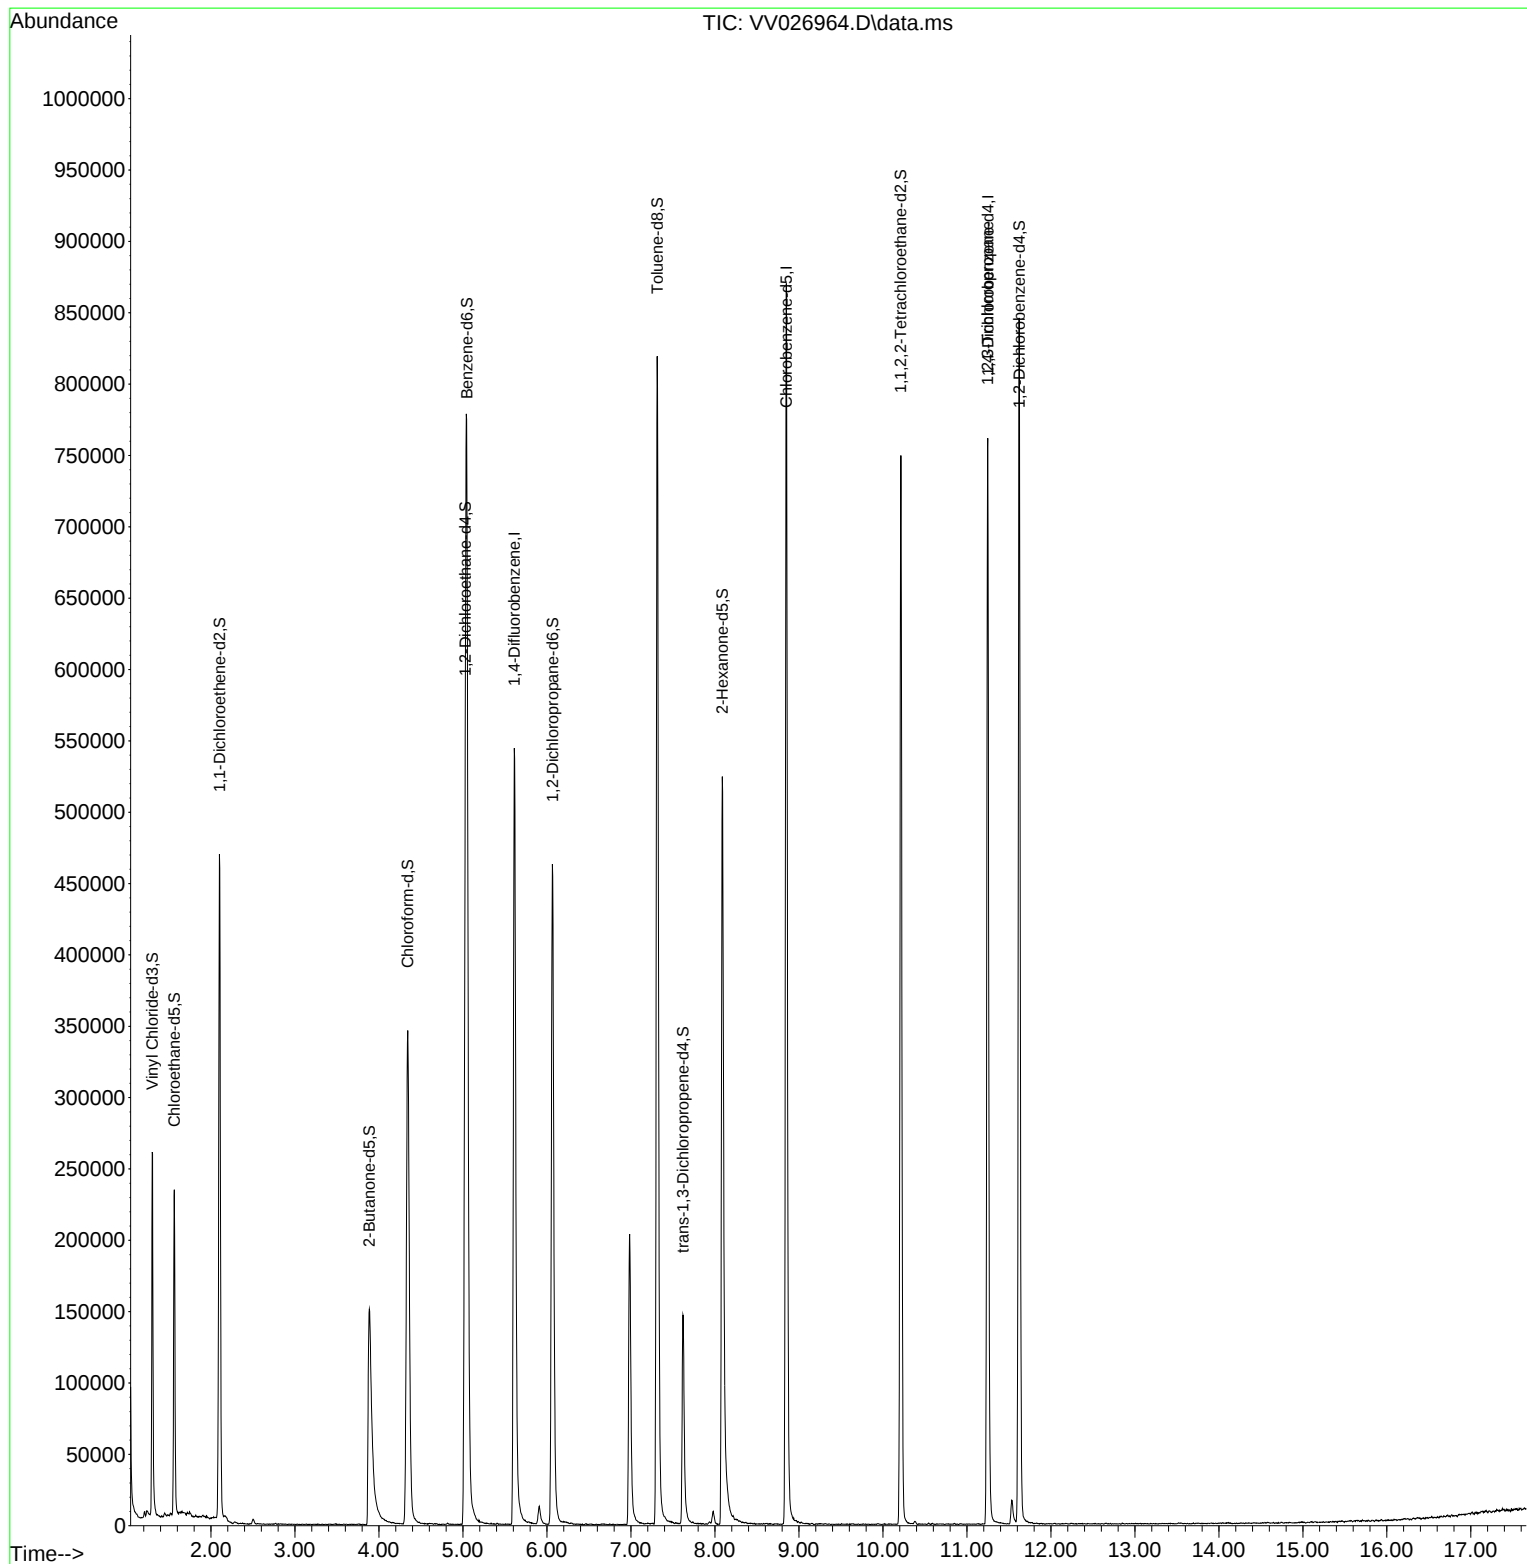

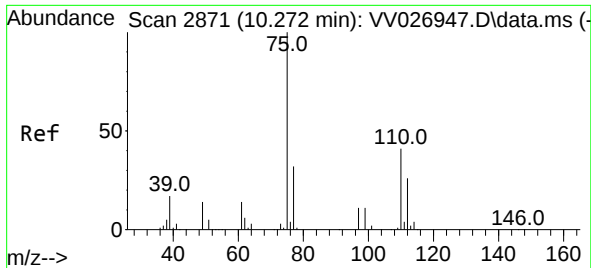

#61
 1,2,3-Trichloropropane
 Concen: 5.672 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV026964.D
 Acq: 26 Jul 2022 20:25

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE4

Tgt Ion: 75 Resp: 23388
 Ion Ratio Lower Upper
 75 100
 77 31.3 25.6 38.4
 110 2.5 31.7 47.5#

