

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026967.D
 Acq On : 26 Jul 2022 21:39
 Operator : SY/MD
 Sample : N3843-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE8

Quant Time: Jul 27 01:44:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	489471	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	498266	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	207283	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	166191	40.483	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.960%
7) Chloroethane-d5	1.565	69	150080	45.190	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.380%
11) 1,1-Dichloroethene-d2	2.101	63	238610	32.307	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.620%
21) 2-Butanone-d5	3.883	46	267868	96.804	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.800%
24) Chloroform-d	4.343	84	378424	46.838	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.680%
26) 1,2-Dichloroethane-d4	5.027	65	226580	49.027	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.060%
32) Benzene-d6	5.043	84	721144	47.880	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.760%
36) 1,2-Dichloropropane-d6	6.066	67	239926	49.431	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.860%
41) Toluene-d8	7.313	98	571793	43.389	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.780%
43) trans-1,3-Dichloroprop...	7.619	79	91032	44.760	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.520%
47) 2-Hexanone-d5	8.088	63	187141	88.549	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.550%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	362843	49.209	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.420%
66) 1,2-Dichlorobenzene-d4	11.625	152	225349	57.949	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.900%
Target Compounds						
39) cis-1,3-Dichloropropene	6.982	75	5413	0.935	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026967.D
Acq On : 26 Jul 2022 21:39
Operator : SY/MD
Sample : N3843-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE8

Quant Time: Jul 27 01:44:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

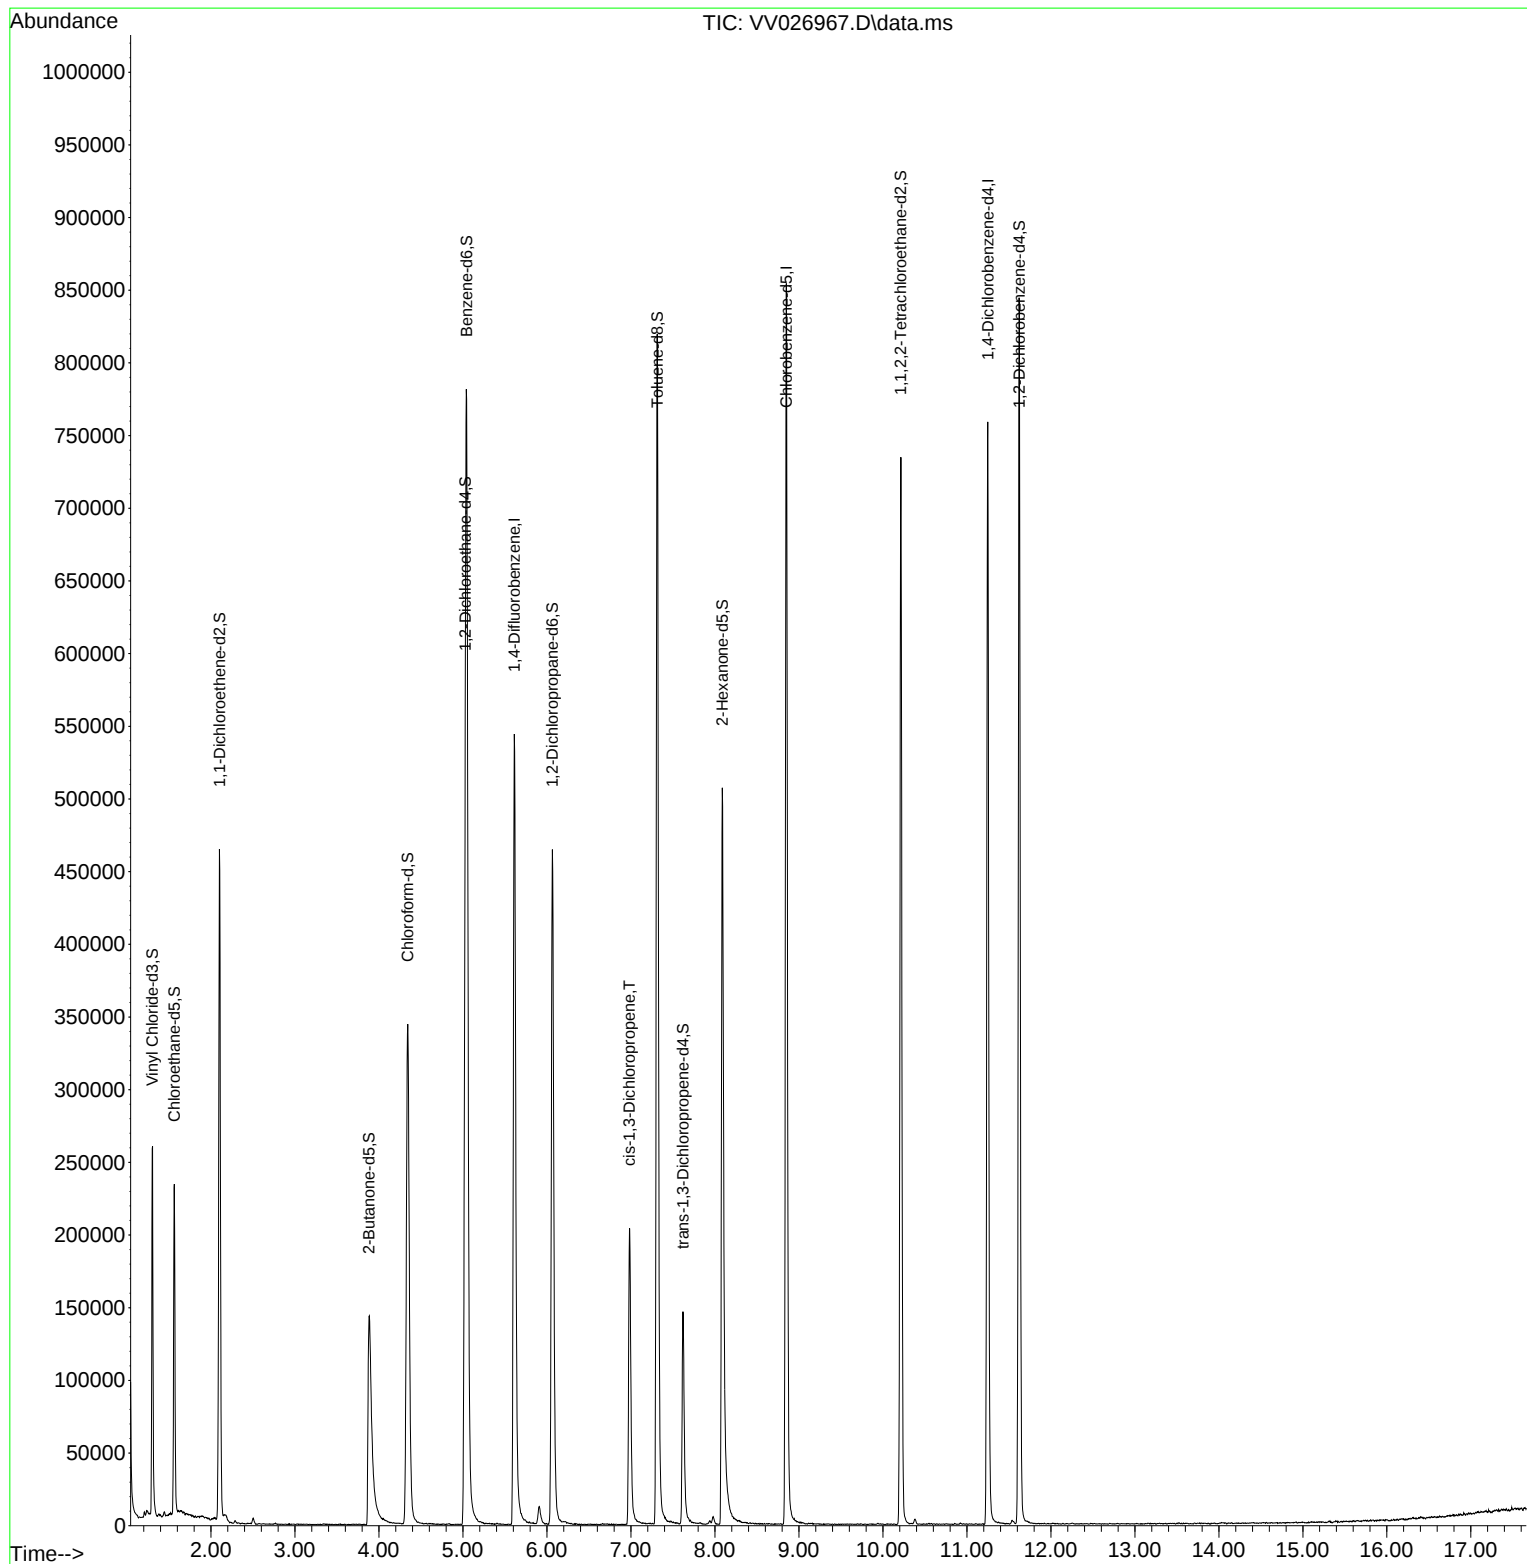

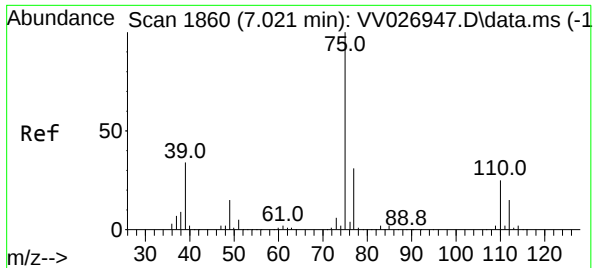

#39

cis-1,3-Dichloropropene

Concen: 0.935 ug/L

RT: 6.982 min Scan# 11

Delta R.T. -0.039 min

Lab File: VV026967.D

Acq: 26 Jul 2022 21:39

Instrument :

MSVOA_V

ClientSampleId :

DBUE8

Tgt Ion: 75 Resp: 5413

Ion Ratio Lower Upper

75 100

77 51.5 22.4 41.6#

