

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026976.D
 Acq On : 27 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3843-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP2

Quant Time: Jul 27 07:02:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 02:43:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	505135	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	502004	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	213415	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	171660	40.518	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.040%
7) Chloroethane-d5	1.564	69	156013	45.519	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.040%
11) 1,1-Dichloroethene-d2	2.105	63	242658	31.837	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.680%
21) 2-Butanone-d5	3.886	46	283498	99.276	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.280%
24) Chloroform-d	4.342	84	380765	45.667	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.340%
26) 1,2-Dichloroethane-d4	5.027	65	232692	48.788	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.580%
32) Benzene-d6	5.047	84	744275	49.048	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.100%
36) 1,2-Dichloropropane-d6	6.066	67	247463	50.604	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.200%
41) Toluene-d8	7.313	98	601454	45.300	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	7.622	79	93715	45.736	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.480%
47) 2-Hexanone-d5	8.088	63	195997	92.049	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.050%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	366182	49.292	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.580%
66) 1,2-Dichlorobenzene-d4	11.622	152	235789	58.891	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	117.780%
Target Compounds						
39) cis-1,3-Dichloropropene	6.985	75	5305	0.910	ug/L	Qvalue # 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026976.D
Acq On : 27 Jul 2022 01:43
Operator : SY/MD
Sample : N3843-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP2

Quant Time: Jul 27 07:02:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 02:43:35 2022
Response via : Initial Calibration

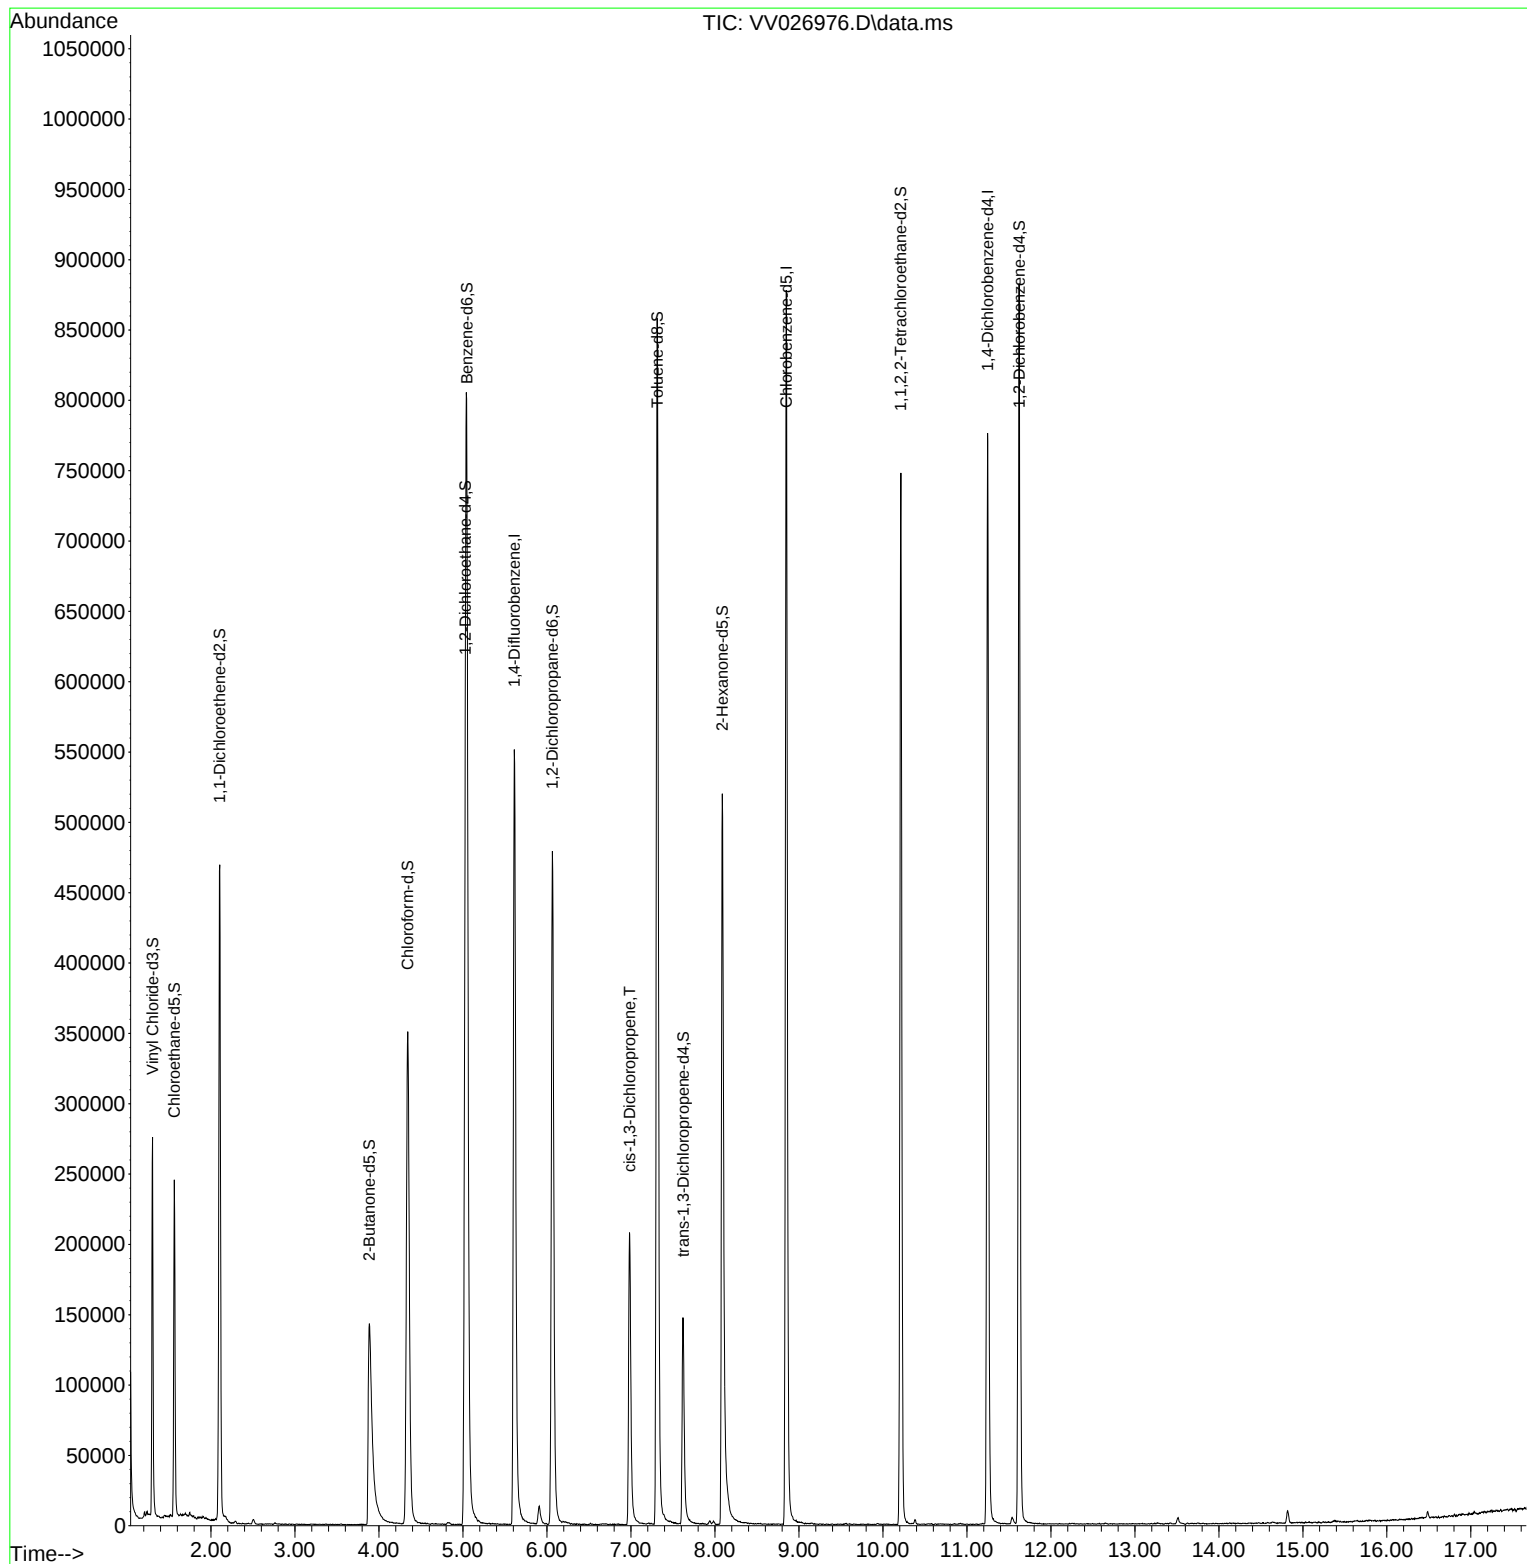

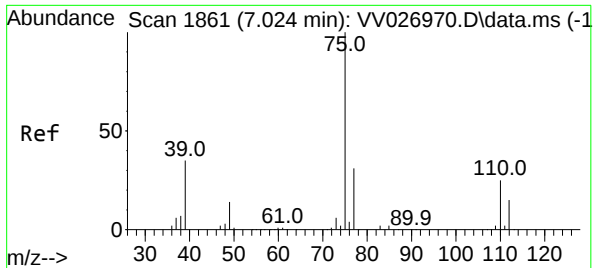

#39
 cis-1,3-Dichloropropene
 Concen: 0.910 ug/L
 RT: 6.985 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV026976.D
 Acq: 27 Jul 2022 01:43

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP2

Tgt Ion: 75 Resp: 5305
 Ion Ratio Lower Upper
 75 100
 77 45.9 22.4 41.6#

