




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 27 01:42:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

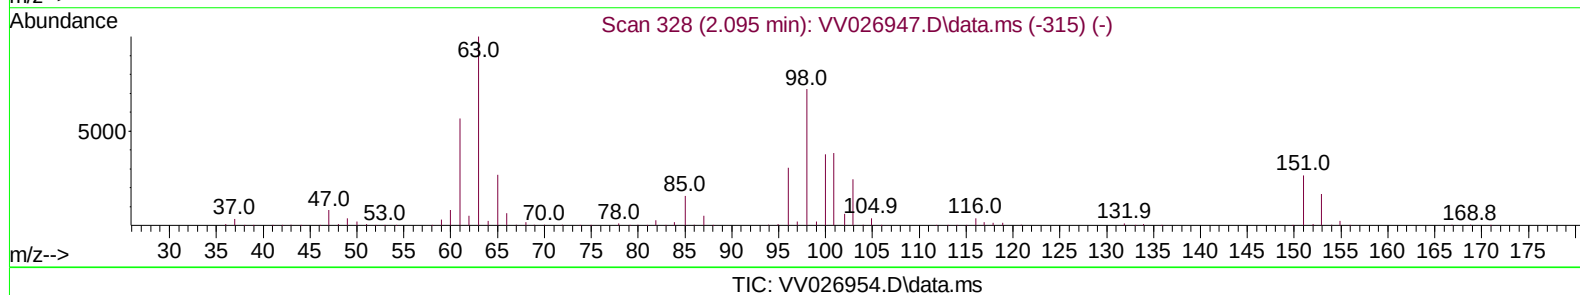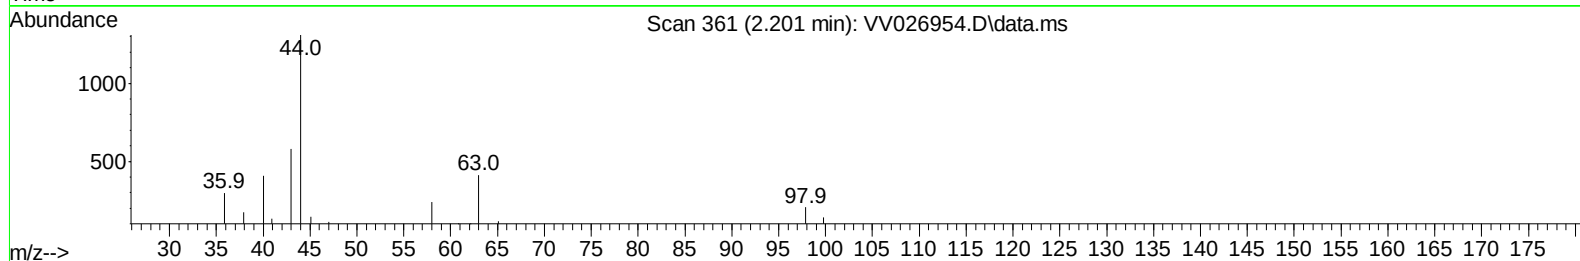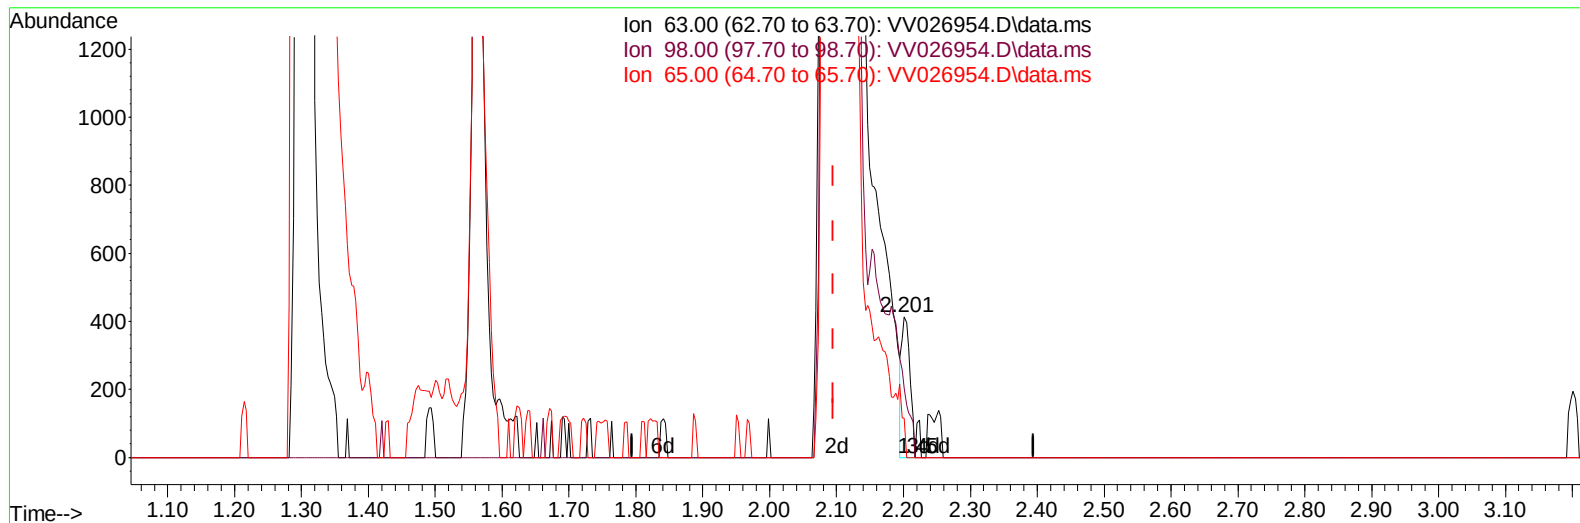

(11) 1,1-Dichloroethene-d2 (S)

2.201min (+ 0.106) 0.06 ug/L

response 351

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.00	73.50
65.00	24.00	24.50
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 27 01:42:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

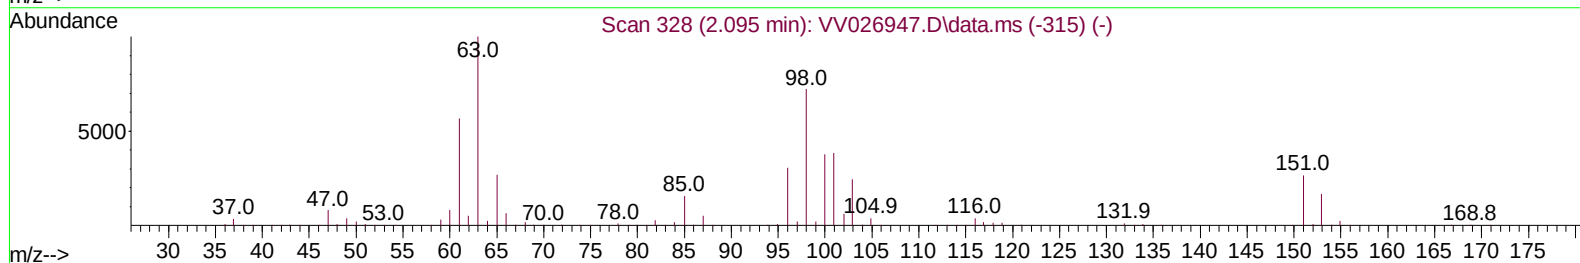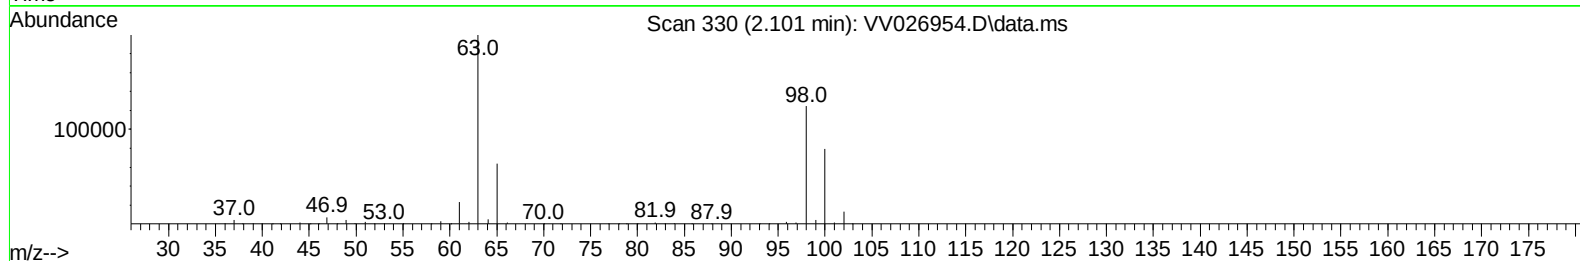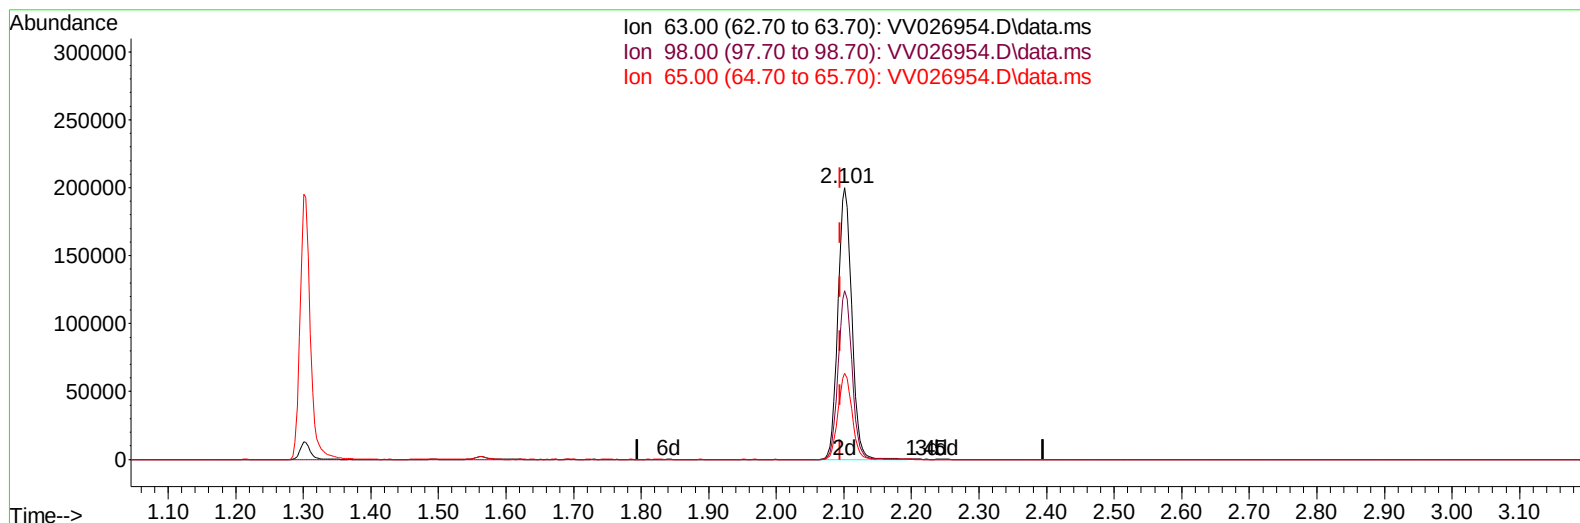

TIC: VV026954.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (+ 0.006) 52.04 ug/L m

response 283793

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.00	0.09#
65.00	24.00	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 27 01:42:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	361431	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	369713	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	156403	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	206136	68.001	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	136.000%#	
7) Chloroethane-d5	1.564	69	179952	73.379	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	146.760%#	
11) 1,1-Dichloroethene-d2	2.101	63	283793m	52.037	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	104.080%	
21) 2-Butanone-d5	3.883	46	298922	146.296	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	146.300%#	
24) Chloroform-d	4.339	84	416846	69.872	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	139.740%#	
26) 1,2-Dichloroethane-d4	5.024	65	246824	72.328	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	144.660%#	
32) Benzene-d6	5.043	84	817252	73.128	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	146.260%#	
36) 1,2-Dichloropropane-d6	6.063	67	262269	72.822	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	145.640%#	
41) Toluene-d8	7.310	98	654898	66.975	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	133.960%#	
43) trans-1,3-Dichloroprop...	7.619	79	104223	69.064	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	138.120%#	
47) 2-Hexanone-d5	8.088	63	198224	126.406	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	126.410%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	382497	69.912	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	139.820%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	248733	84.770	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	169.540%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026954.D
Acq On : 26 Jul 2022 16:20
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 27 01:42:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

