




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 27 01:44:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

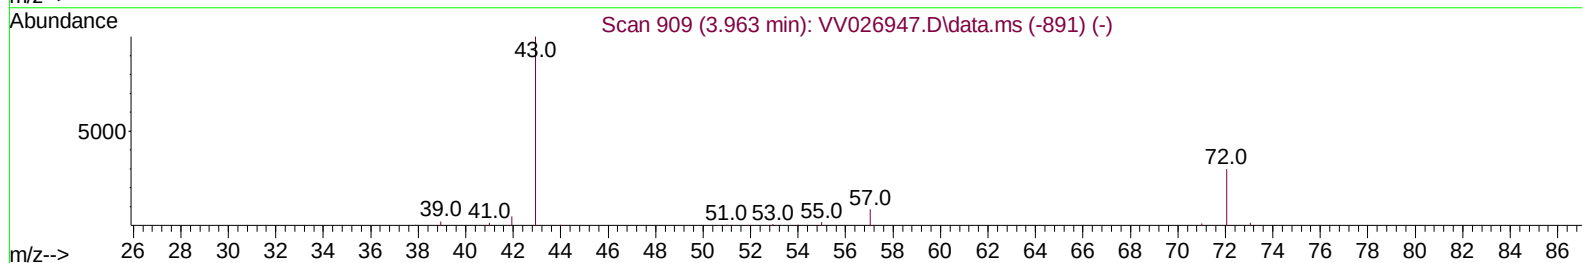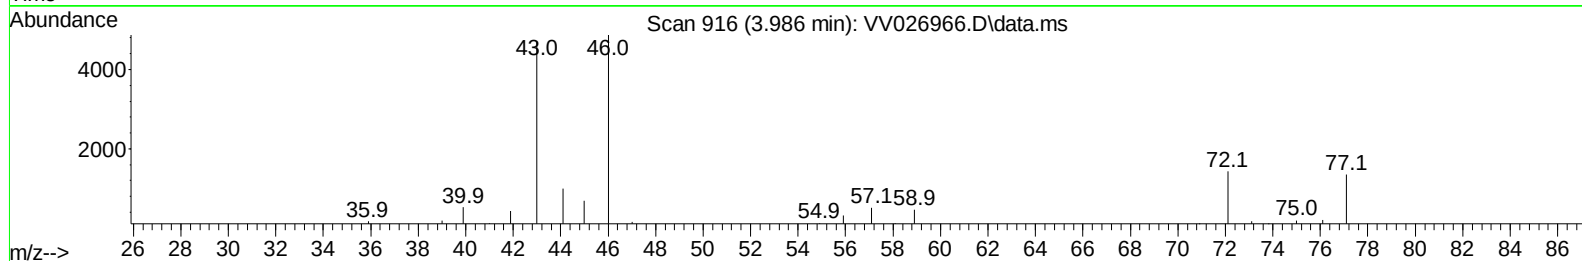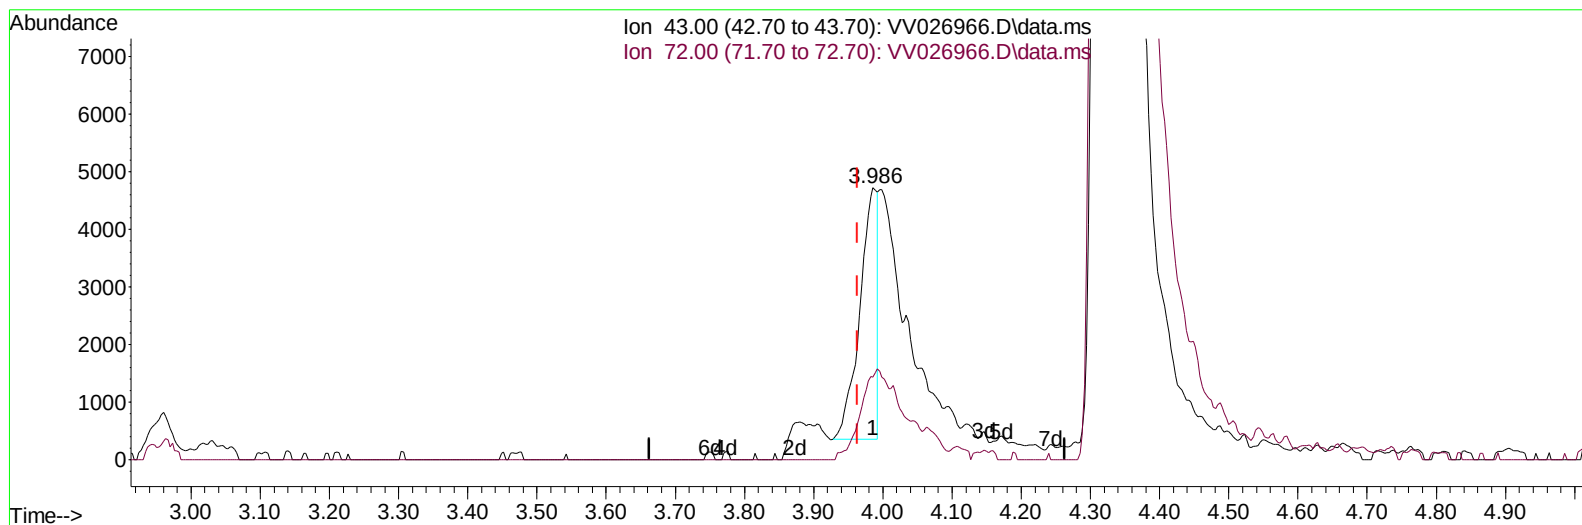

TIC: VV026966.D\data.ms

(22) 2-Butanone (T)

3.986min (+ 0.022) 2.93 ug/L

response 7774

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	45.45#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Manual IntegrationsAPPROVED

Quant Time: Jul 27 01:44:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

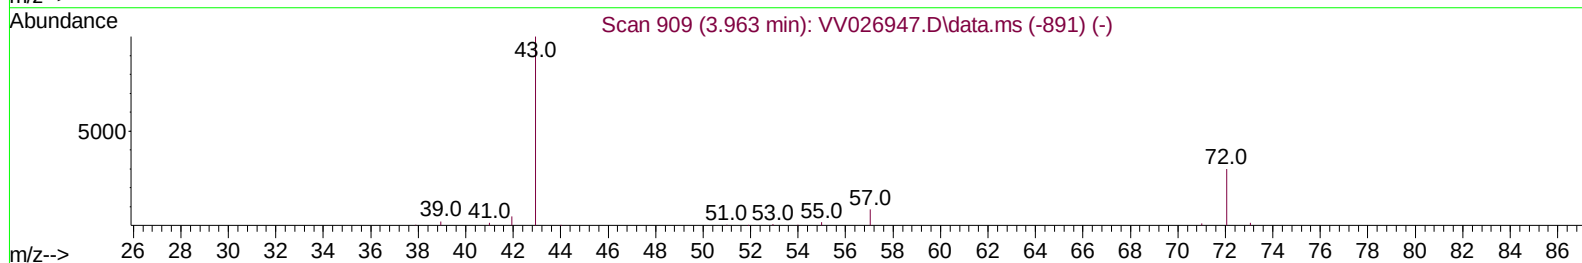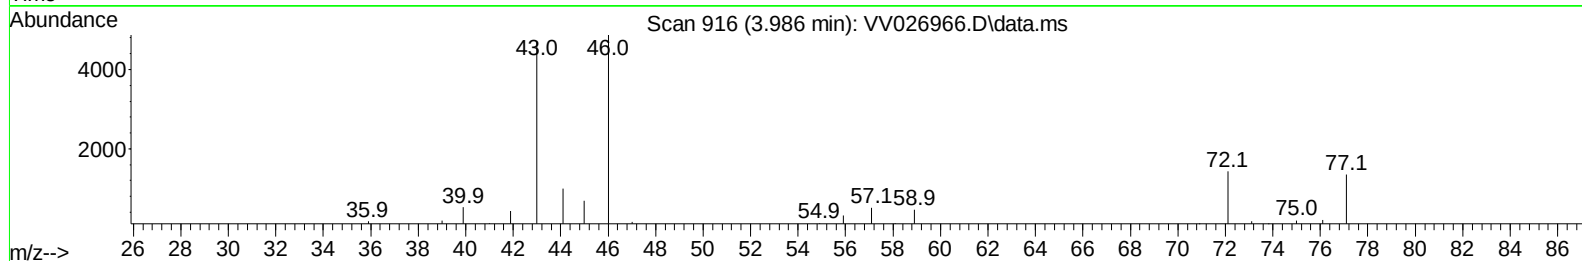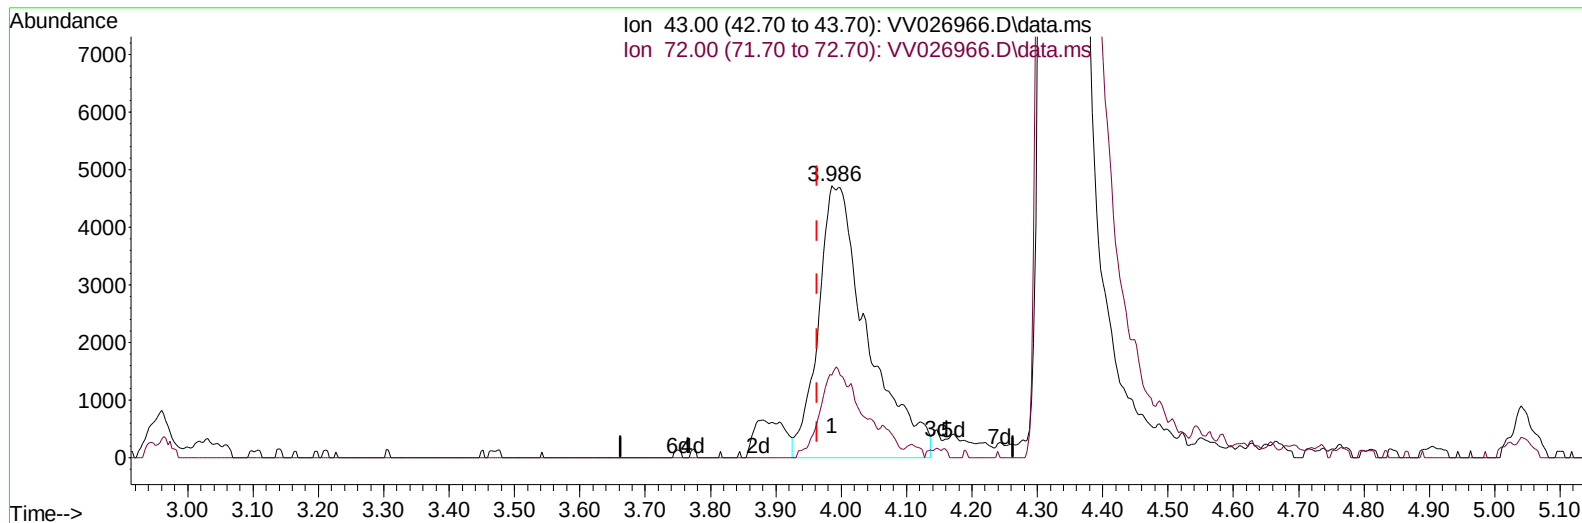

TIC: VV026966.D\data.ms

(22) 2-Butanone (T)

3.986min (+ 0.022) 9.26 ug/L m

response 24593

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	14.37#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Manual IntegrationsAPPROVED

Quant Time: Jul 27 01:44:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	490754	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	489490	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	206085	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	166131	40.362	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	80.720%	
7) Chloroethane-d5	1.565	69	149021	44.753	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	89.500%	
11) 1,1-Dichloroethene-d2	2.101	63	238584	32.219	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	64.440%	
21) 2-Butanone-d5	3.883	46	279824	100.861	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	100.860%	
24) Chloroform-d	4.343	84	382589	47.230	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.460%	
26) 1,2-Dichloroethane-d4	5.027	65	227005	48.991	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.980%	
32) Benzene-d6	5.043	84	738305	49.898	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.800%	
36) 1,2-Dichloropropane-d6	6.066	67	239360	50.198	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	100.400%	
41) Toluene-d8	7.314	98	569991	44.028	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.060%	
43) trans-1,3-Dichloroprop...	7.619	79	92089	46.091	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	92.180%	
47) 2-Hexanone-d5	8.088	63	187037	90.087	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	90.090%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	360570	49.777	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.560%	
66) 1,2-Dichlorobenzene-d4	11.622	152	223764	57.876	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	115.760%	
Target Compounds						
13) Acetone	2.175	43	573202	294.248	ug/L	98
22) 2-Butanone	3.986	43	24593m	9.256	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026966.D
Acq On : 26 Jul 2022 21:14
Operator : SY/MD
Sample : N3843-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 27 01:44:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

