




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026972.D
 Acq On : 27 Jul 2022 00:05
 Operator : SY/MD
 Sample : N3843-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF0

Manual IntegrationsAPPROVED

Quant Time: Jul 27 07:01:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 02:43:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

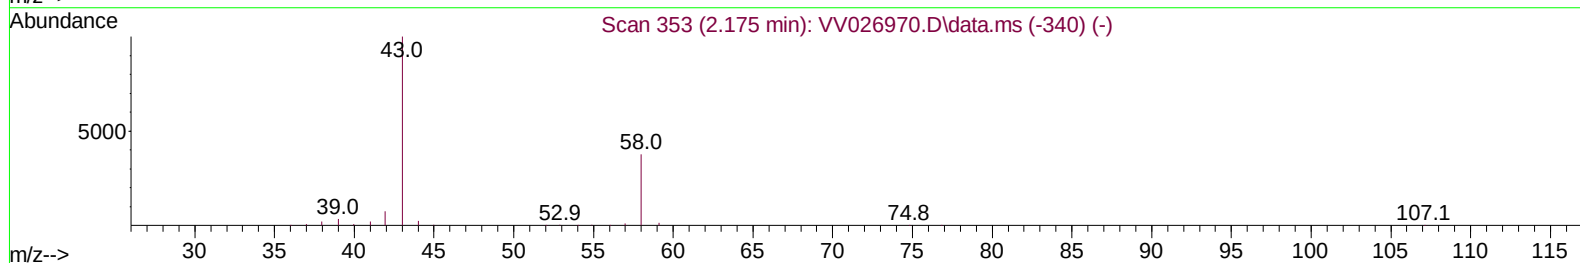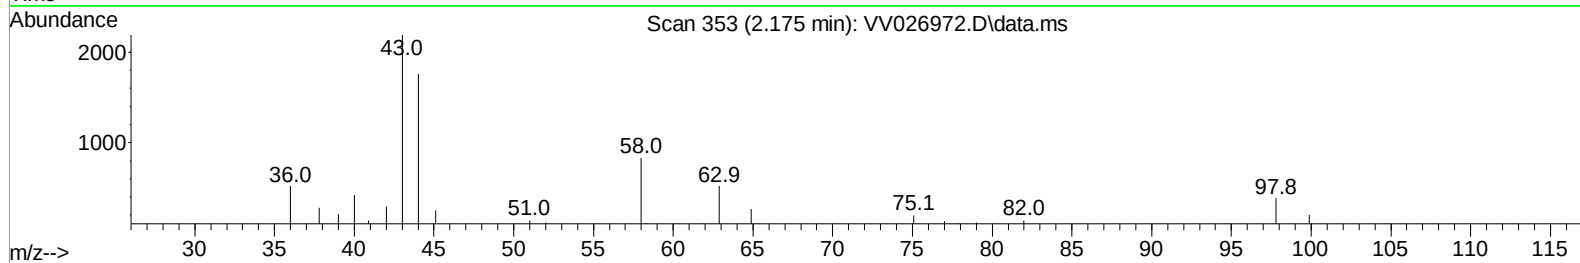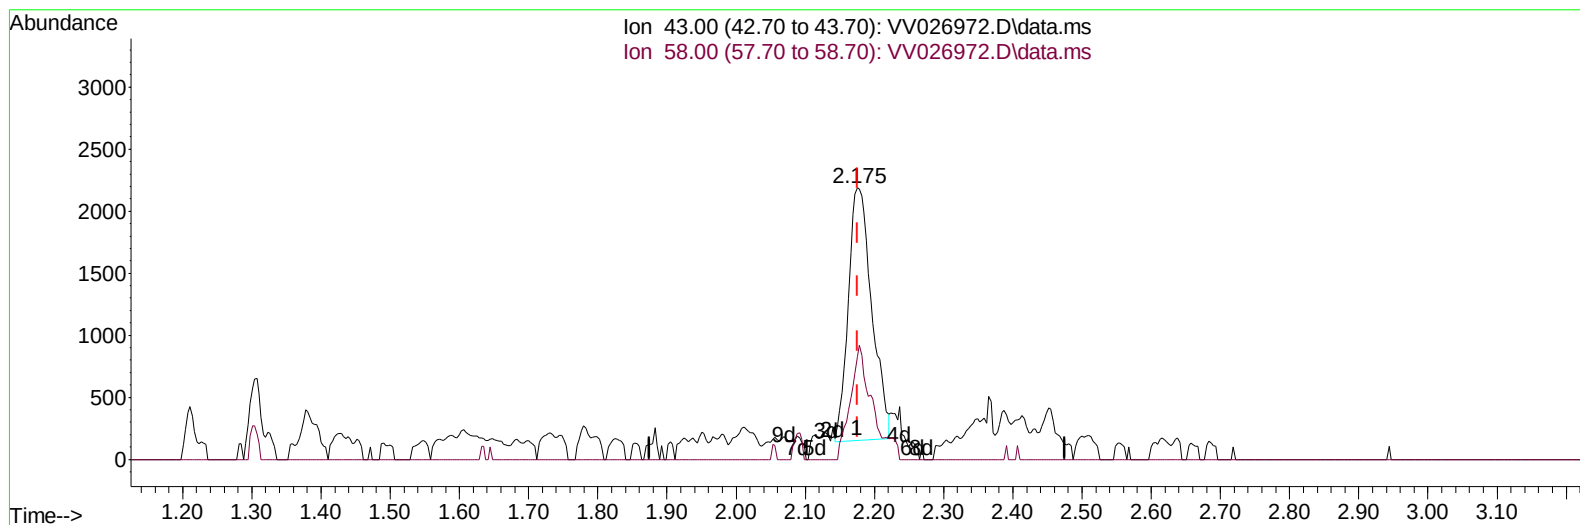

TIC: VV026972.D\data.ms

(13) Acetone (T)

2.175min (-0.000) 2.41 ug/L

response 4807

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	29.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026972.D
 Acq On : 27 Jul 2022 00:05
 Operator : SY/MD
 Sample : N3843-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF0

Manual IntegrationsAPPROVED

Quant Time: Jul 27 07:01:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 02:43:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

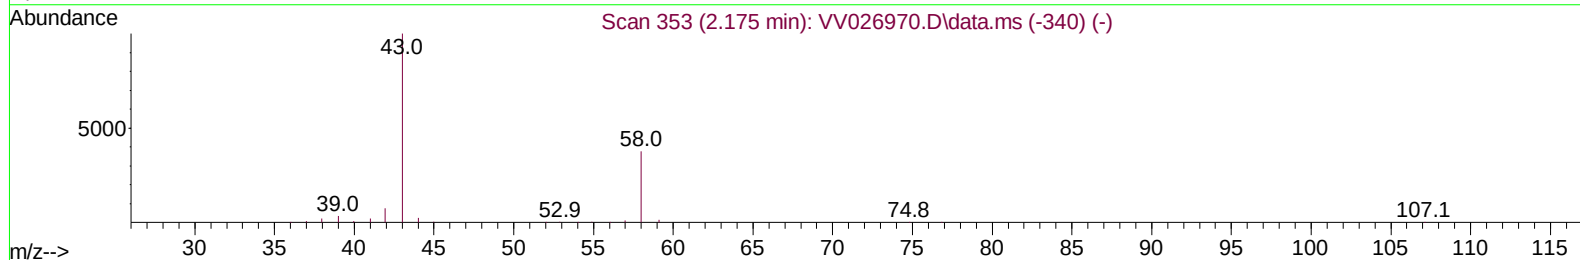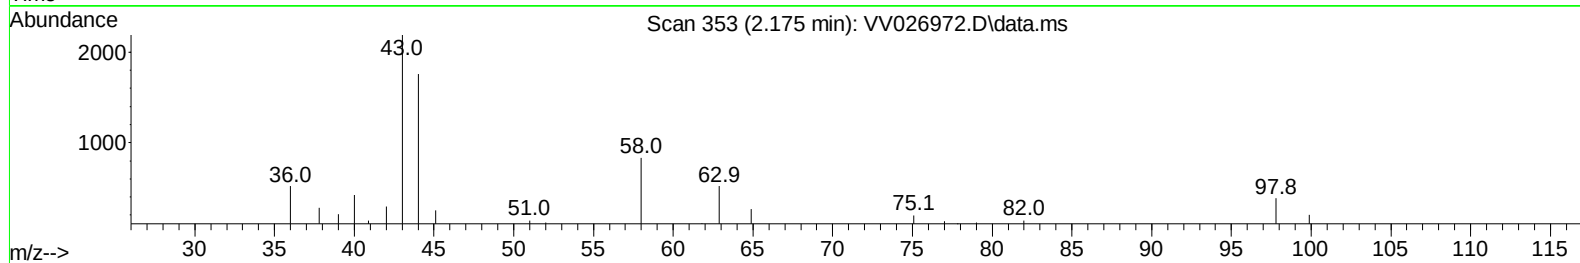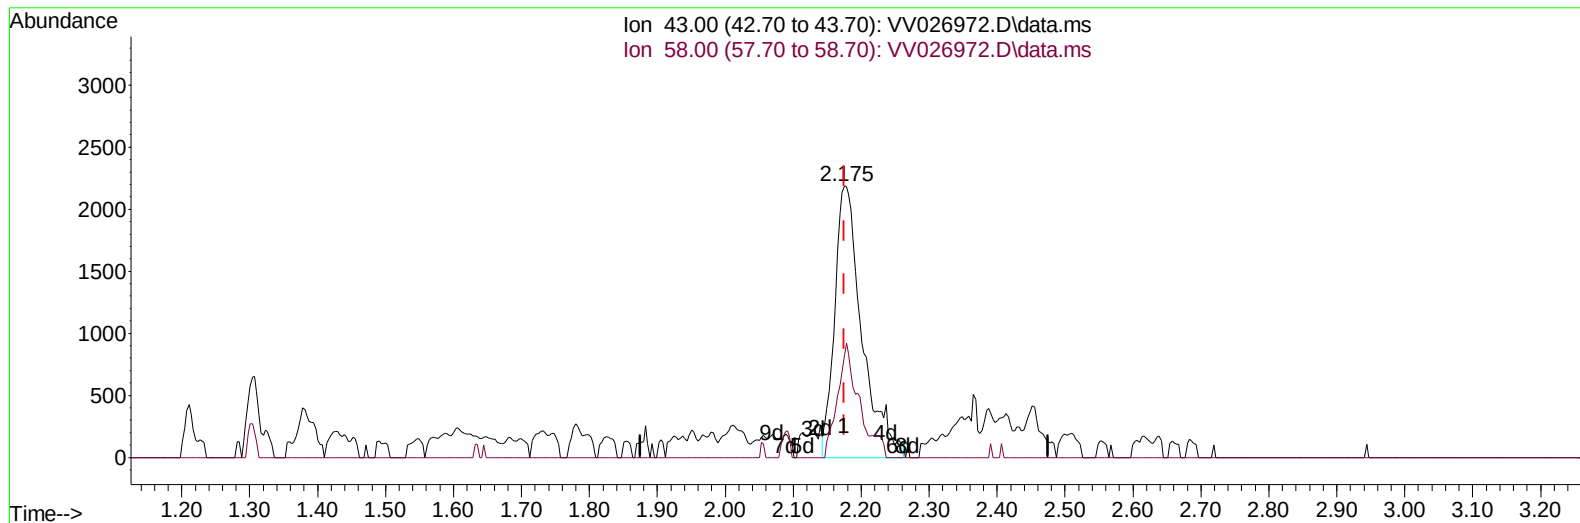

TIC: VV026972.D\data.ms

(13) Acetone (T)

2.175min (-0.000) 3.05 ug/L m

response 6099

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	23.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026972.D
 Acq On : 27 Jul 2022 00:05
 Operator : SY/MD
 Sample : N3843-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF0

Manual IntegrationsAPPROVED

Quant Time: Jul 27 07:01:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 02:43:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		503196	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		515351	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		216224	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		164409	38.956	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	77.920%	
7) Chloroethane-d5	1.564	69		150848	44.182	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	88.360%	
11) 1,1-Dichloroethene-d2	2.101	63		233883	30.804	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	61.600%	
21) 2-Butanone-d5	3.883	46		292661	102.879	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	102.880%	
24) Chloroform-d	4.342	84		382950	46.106	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	92.220%	
26) 1,2-Dichloroethane-d4	5.027	65		229389	48.281	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	96.560%	
32) Benzene-d6	5.043	84		731443	46.954	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	93.900%	
36) 1,2-Dichloropropane-d6	6.066	67		244885	48.780	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	97.560%	
41) Toluene-d8	7.313	98		584442	42.879	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	85.760%	
43) trans-1,3-Dichloroprop...	7.619	79		92337	43.896	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	87.800%	
47) 2-Hexanone-d5	8.088	63		201267	92.076	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	92.080%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		372189	48.803	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152		230545	56.833	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	113.660%	
Target Compounds							
13) Acetone	2.175	43		6099m	3.053	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026972.D
Acq On : 27 Jul 2022 00:05
Operator : SY/MD
Sample : N3843-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF0

Manual IntegrationsAPPROVED

Quant Time: Jul 27 07:01:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 02:43:35 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

