

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026965.D
 Acq On : 26 Jul 2022 20:50
 Operator : SY/MD
 Sample : N3843-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE5

Quant Time: Jul 27 01:44:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 01:39:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	467187	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	476562	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	194522	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	163212	41.653	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.300%
7) Chloroethane-d5	1.564	69	148750	46.925	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.860%
11) 1,1-Dichloroethene-d2	2.101	63	228288	32.384	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.760%
21) 2-Butanone-d5	3.883	46	274721	104.016	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.020%
24) Chloroform-d	4.342	84	368574	47.795	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.027	65	223973	50.775	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.540%
32) Benzene-d6	5.047	84	700406	48.621	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.240%
36) 1,2-Dichloropropane-d6	6.066	67	238402	51.354	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.700%
41) Toluene-d8	7.313	98	548724	43.535	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.080%
43) trans-1,3-Dichloroprop...	7.622	79	90855	46.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.420%
47) 2-Hexanone-d5	8.088	63	189897	93.945	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.950%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	360167	51.071	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.140%
66) 1,2-Dichlorobenzene-d4	11.622	152	213100	58.394	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.780%
Target Compounds						
					Qvalue	
13) Acetone	2.179	43	13257	7.149	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026965.D
Acq On : 26 Jul 2022 20:50
Operator : SY/MD
Sample : N3843-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE5

Quant Time: Jul 27 01:44:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 01:39:23 2022
Response via : Initial Calibration

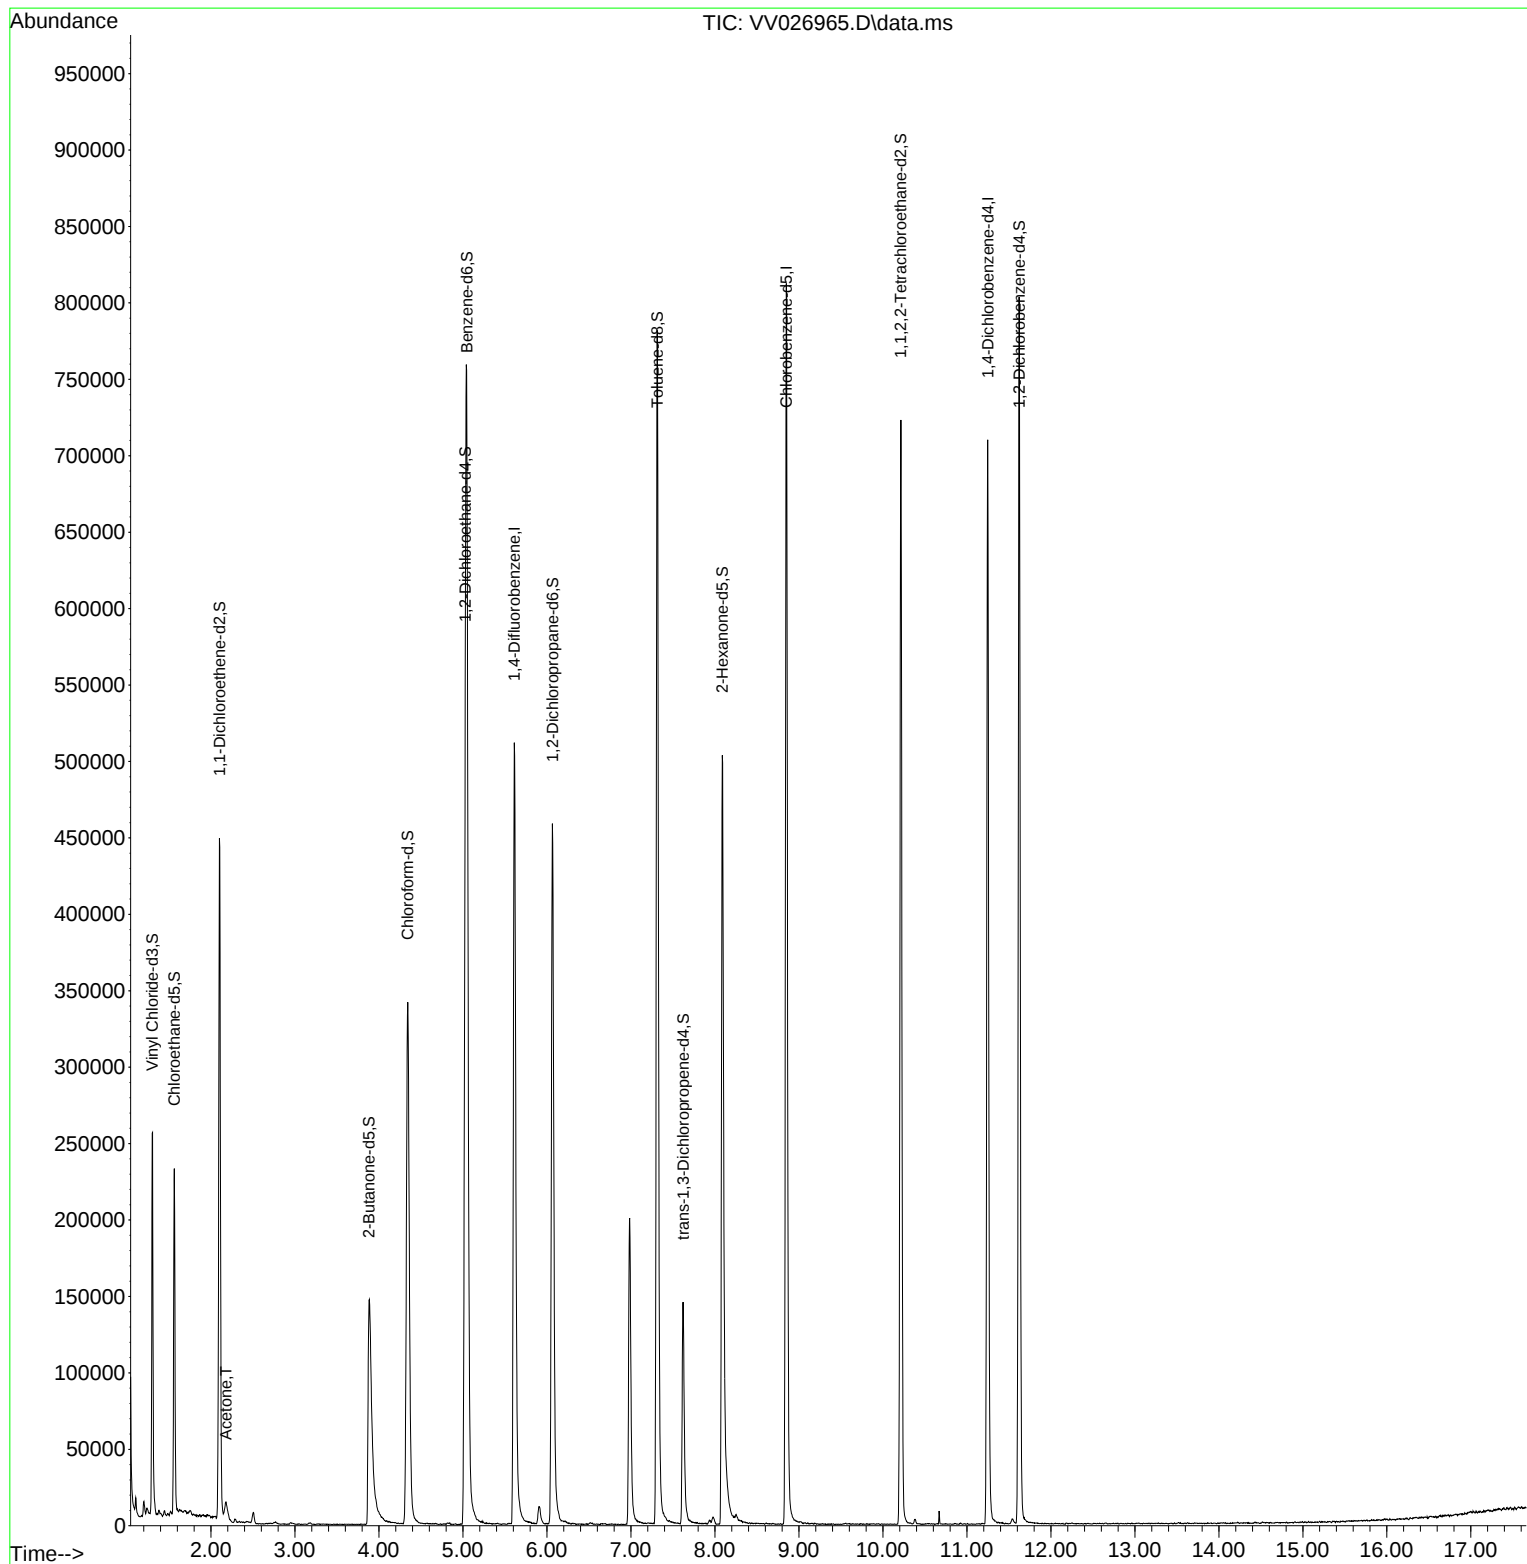

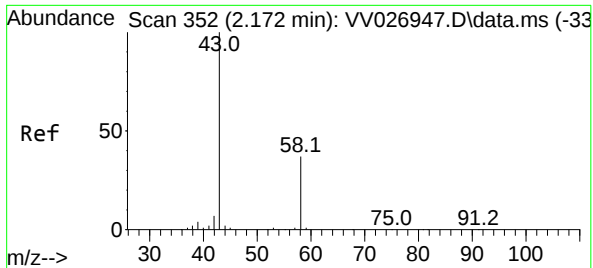

#13
 Acetone
 Concen: 7.149 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV026965.D
 Acq: 26 Jul 2022 20:50

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE5

Tgt Ion: 43 Resp: 13257
 Ion Ratio Lower Upper
 43 100
 58 39.9 0.0 72.6

