

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026972.D
 Acq On : 27 Jul 2022 00:05
 Operator : SY/MD
 Sample : N3843-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 27 07:01:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 27 02:43:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	503196	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	515351	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	216224	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	164409	38.956	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.920%		
7) Chloroethane-d5	1.564	69	150848	44.182	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.360%		
11) 1,1-Dichloroethene-d2	2.101	63	233883	30.804	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.600%		
21) 2-Butanone-d5	3.883	46	292661	102.879	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.880%		
24) Chloroform-d	4.342	84	382950	46.106	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.220%		
26) 1,2-Dichloroethane-d4	5.027	65	229389	48.281	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.560%		
32) Benzene-d6	5.043	84	731443	46.954	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.900%		
36) 1,2-Dichloropropane-d6	6.066	67	244885	48.780	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.560%		
41) Toluene-d8	7.313	98	584442	42.879	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.760%		
43) trans-1,3-Dichloroprop...	7.619	79	92337	43.896	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.800%		
47) 2-Hexanone-d5	8.088	63	201267	92.076	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.080%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	372189	48.803	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	230545	56.833	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	113.660%		
Target Compounds					Qvalue	
13) Acetone	2.175	43	6099m	3.053	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026972.D
Acq On : 27 Jul 2022 00:05
Operator : SY/MD
Sample : N3843-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBUF0

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Quant Time: Jul 27 07:01:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 27 02:43:35 2022
Response via : Initial Calibration

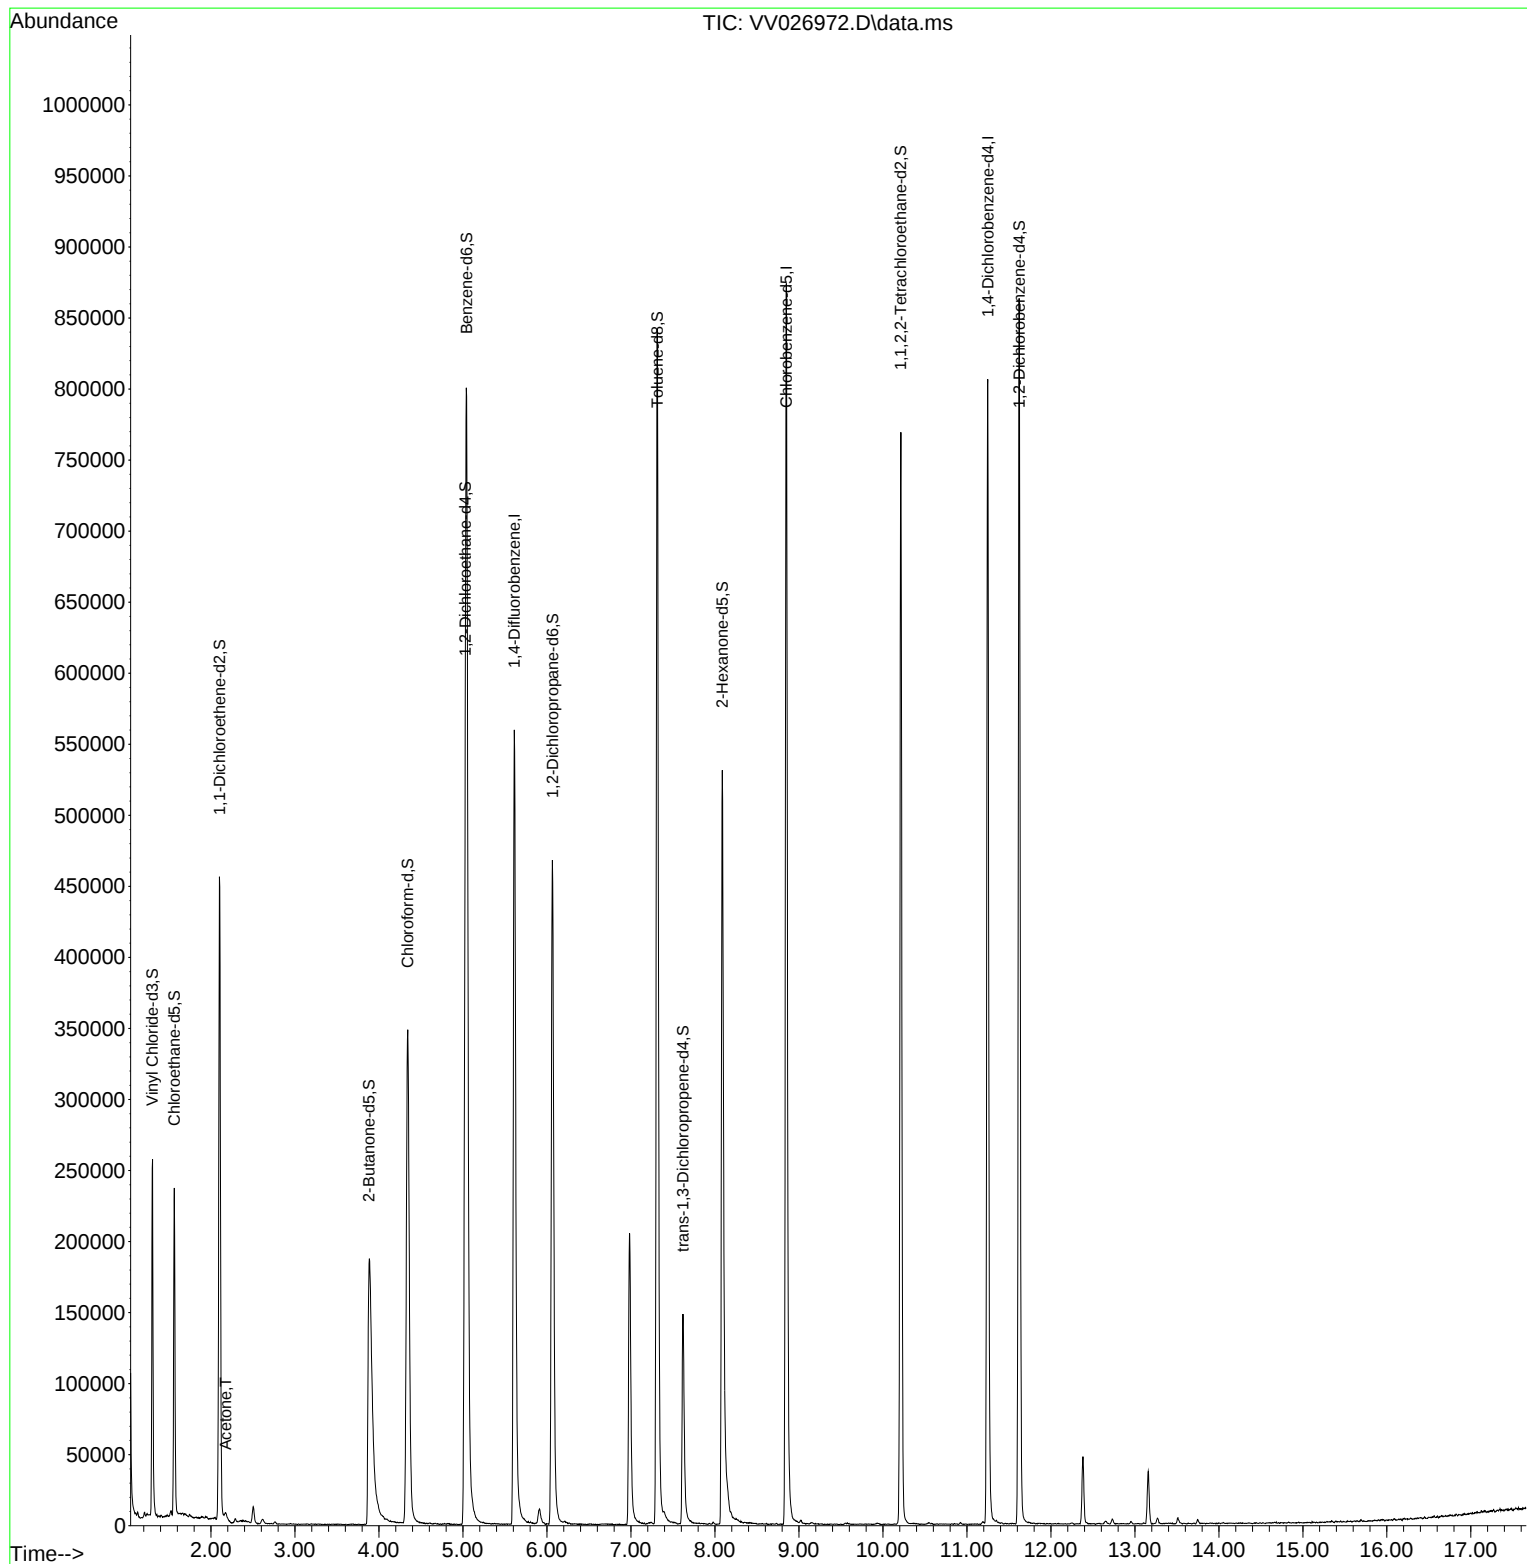

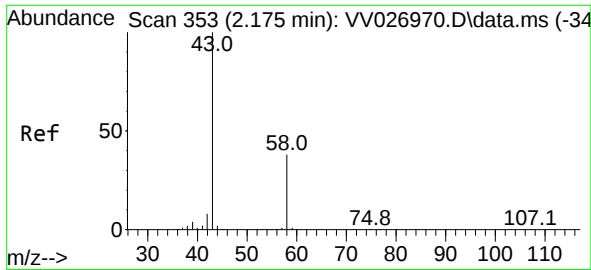

#13
 Acetone
 Concen: 3.053 ug/L m
 RT: 2.175 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV026972.D
 Acq: 27 Jul 2022 00:05

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF0

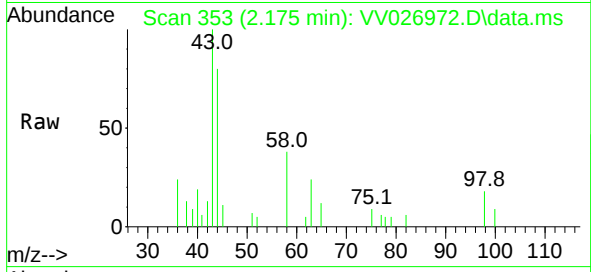

Tgt Ion: 43 Resp: 6099
 Ion Ratio Lower Upper
 43 100
 58 23.4 0.0 72.6

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

