

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026949.D
 Acq On : 26 Jul 2022 13:51
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	99	rVB	299544	315649	14.14%	1.950%
2	1.564	155	163	178	rBV	261253	300688	13.47%	1.858%
3	2.101	319	330	346	rBV	537960	771298	34.56%	4.765%
4	2.503	445	455	465	rBV	17692	28088	1.26%	0.174%
5	2.613	479	489	497	rVV4	1584	2762	0.12%	0.017%
6	2.754	531	533	540	rVB5	825	757	0.03%	0.005%
7	2.809	548	550	558	rVB3	456	349	0.02%	0.002%
8	2.905	576	580	583	rVB3	340	324	0.01%	0.002%
9	2.931	583	588	593	rBV3	436	549	0.02%	0.003%
10	3.037	618	621	624	rVB2	404	250	0.01%	0.002%
11	3.053	624	626	629	rBV2	412	269	0.01%	0.002%
12	3.156	655	658	663	rBV	396	341	0.02%	0.002%
13	3.191	667	669	673	rVV2	400	296	0.01%	0.002%
14	3.259	684	690	692	rBV2	393	442	0.02%	0.003%
15	3.326	708	711	718	rBV3	406	394	0.02%	0.002%
16	3.394	725	732	733	rBV	513	318	0.01%	0.002%
17	3.468	752	755	758	rBV2	403	262	0.01%	0.002%
18	3.497	758	764	767	rVB2	348	314	0.01%	0.002%
19	3.651	809	812	816	rVB2	616	458	0.02%	0.003%
20	3.767	845	848	853	rBV	322	251	0.01%	0.002%
21	3.802	854	859	863	rBV2	263	313	0.01%	0.002%
22	3.886	873	885	928	rBV2	158797	577268	25.86%	3.567%
23	4.339	1009	1026	1057	rBV2	367145	916433	41.06%	5.662%
24	4.519	1079	1082	1088	rBV4	448	508	0.02%	0.003%
25	4.629	1113	1116	1119	rVB3	664	408	0.02%	0.003%
26	4.699	1135	1138	1142	rVB3	390	303	0.01%	0.002%
27	4.969	1219	1222	1225	rVB3	429	304	0.01%	0.002%
28	5.040	1225	1244	1270	rBV2	865526	2232084	100.00%	13.791%
29	5.394	1348	1354	1356	rBV4	364	399	0.02%	0.002%
30	5.481	1379	1381	1385	rVB4	447	265	0.01%	0.002%
31	5.506	1385	1389	1394	rBV2	650	685	0.03%	0.004%
32	5.612	1410	1422	1449	rBV	549370	1130192	50.63%	6.983%
33	5.825	1486	1488	1492	rVB4	642	390	0.02%	0.002%
34	5.857	1496	1498	1502	rVB3	366	260	0.01%	0.002%
35	5.905	1502	1513	1537	rVB2	16099	36011	1.61%	0.222%
36	6.063	1548	1562	1595	rBV	498570	1036304	46.43%	6.403%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026949.D
 Acq On : 26 Jul 2022 13:51
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.307	1634	1638	1640	rVB4	661	501	0.02%	0.003%
38	6.378	1658	1660	1663	rBV	434	259	0.01%	0.002%
39	6.423	1672	1674	1677	rBV2	442	262	0.01%	0.002%
40	6.513	1698	1702	1705	rVB2	666	411	0.02%	0.003%
41	6.538	1705	1710	1711	rBV2	411	271	0.01%	0.002%
42	6.583	1721	1724	1731	rBV3	360	353	0.02%	0.002%
43	6.654	1742	1746	1748	rBV2	582	462	0.02%	0.003%
44	6.696	1756	1759	1762	rVB3	719	492	0.02%	0.003%
45	6.773	1781	1783	1792	rVB4	451	497	0.02%	0.003%
46	6.879	1812	1816	1820	rBV2	351	285	0.01%	0.002%
47	6.982	1837	1848	1876	rBV	230192	437807	19.61%	2.705%
48	7.217	1918	1921	1925	rVB3	846	625	0.03%	0.004%
49	7.313	1937	1951	1982	rBV	931193	1647781	73.82%	10.181%
50	7.619	2036	2046	2076	rBV	168600	306964	13.75%	1.897%
51	7.931	2138	2143	2145	rBV2	885	685	0.03%	0.004%
52	8.088	2181	2192	2228	rBV	519513	1026596	45.99%	6.343%
53	8.423	2288	2296	2305	rBV7	2055	3840	0.17%	0.024%
54	8.567	2337	2341	2342	rBV3	520	442	0.02%	0.003%
55	8.622	2356	2358	2363	rVB4	482	315	0.01%	0.002%
56	8.664	2363	2371	2374	rBV4	633	750	0.03%	0.005%
57	8.850	2417	2429	2462	rBV	888079	1453327	65.11%	8.979%
58	9.114	2508	2511	2513	rBV2	348	260	0.01%	0.002%
59	9.143	2518	2520	2529	rVB5	664	681	0.03%	0.004%
60	9.220	2541	2544	2547	rVB2	445	285	0.01%	0.002%
61	9.249	2547	2553	2555	rBV3	552	588	0.03%	0.004%
62	9.265	2556	2558	2564	rVB3	282	270	0.01%	0.002%
63	9.484	2623	2626	2631	rVB2	429	326	0.01%	0.002%
64	9.525	2636	2639	2642	rBV2	324	263	0.01%	0.002%
65	9.590	2656	2659	2663	rVB3	331	253	0.01%	0.002%
66	9.654	2675	2679	2683	rBV2	319	301	0.01%	0.002%
67	9.718	2696	2699	2702	rVB	479	345	0.02%	0.002%
68	9.738	2702	2705	2708	rBV2	415	270	0.01%	0.002%
69	9.882	2746	2750	2754	rBV2	331	385	0.02%	0.002%
70	9.908	2756	2758	2763	rVB	354	293	0.01%	0.002%
71	9.937	2763	2767	2769	rBV	481	377	0.02%	0.002%
72	10.214	2841	2853	2872	rBV	770271	1199322	53.73%	7.410%
73	10.538	2951	2954	2959	rVB2	459	427	0.02%	0.003%
74	10.580	2960	2967	2969	rBV5	658	653	0.03%	0.004%
75	10.857	3050	3053	3059	rVB4	754	599	0.03%	0.004%
76	10.889	3059	3063	3067	rVB	385	357	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026949.D
 Acq On : 26 Jul 2022 13:51
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.927	3067	3075	3079	rBV3	546	696	0.03%	0.004%
78	11.056	3111	3115	3121	rBV2	316	396	0.02%	0.002%
79	11.188	3153	3156	3162	rVB3	853	788	0.04%	0.005%
80	11.246	3162	3174	3199	rBV	807858	1268202	56.82%	7.836%
81	11.622	3278	3291	3318	rBV	939329	1459717	65.40%	9.019%
82	11.831	3349	3356	3360	rBV4	744	976	0.04%	0.006%
83	11.886	3370	3373	3376	rVV3	581	407	0.02%	0.003%
84	11.914	3380	3382	3388	rVB3	575	526	0.02%	0.003%
85	12.056	3422	3426	3430	rBV2	357	347	0.02%	0.002%
86	12.522	3567	3571	3573	rBV	617	473	0.02%	0.003%
87	12.564	3579	3584	3588	rBV2	511	561	0.03%	0.003%
88	12.603	3593	3596	3598	rBV2	465	274	0.01%	0.002%
89	12.805	3656	3659	3667	rBV2	507	676	0.03%	0.004%
90	13.117	3753	3756	3760	rBV2	377	331	0.01%	0.002%
91	13.159	3766	3769	3772	rBV3	491	318	0.01%	0.002%
92	13.178	3772	3775	3780	rBV3	576	510	0.02%	0.003%
93	13.271	3800	3804	3806	rBV3	489	477	0.02%	0.003%
94	13.403	3842	3845	3847	rBV2	347	247	0.01%	0.002%
95	13.512	3874	3879	3883	rBV3	1569	1598	0.07%	0.010%
96	14.033	4038	4041	4044	rBV	490	380	0.02%	0.002%
97	14.107	4060	4064	4071	rBV4	599	603	0.03%	0.004%
98	14.181	4084	4087	4089	rBV2	551	277	0.01%	0.002%
99	15.361	4451	4454	4456	rBV2	816	487	0.02%	0.003%
100	16.027	4659	4661	4663	rBV2	1046	641	0.03%	0.004%


Sum of corrected areas: 16185274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026949.D
Acq On : 26 Jul 2022 13:51
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

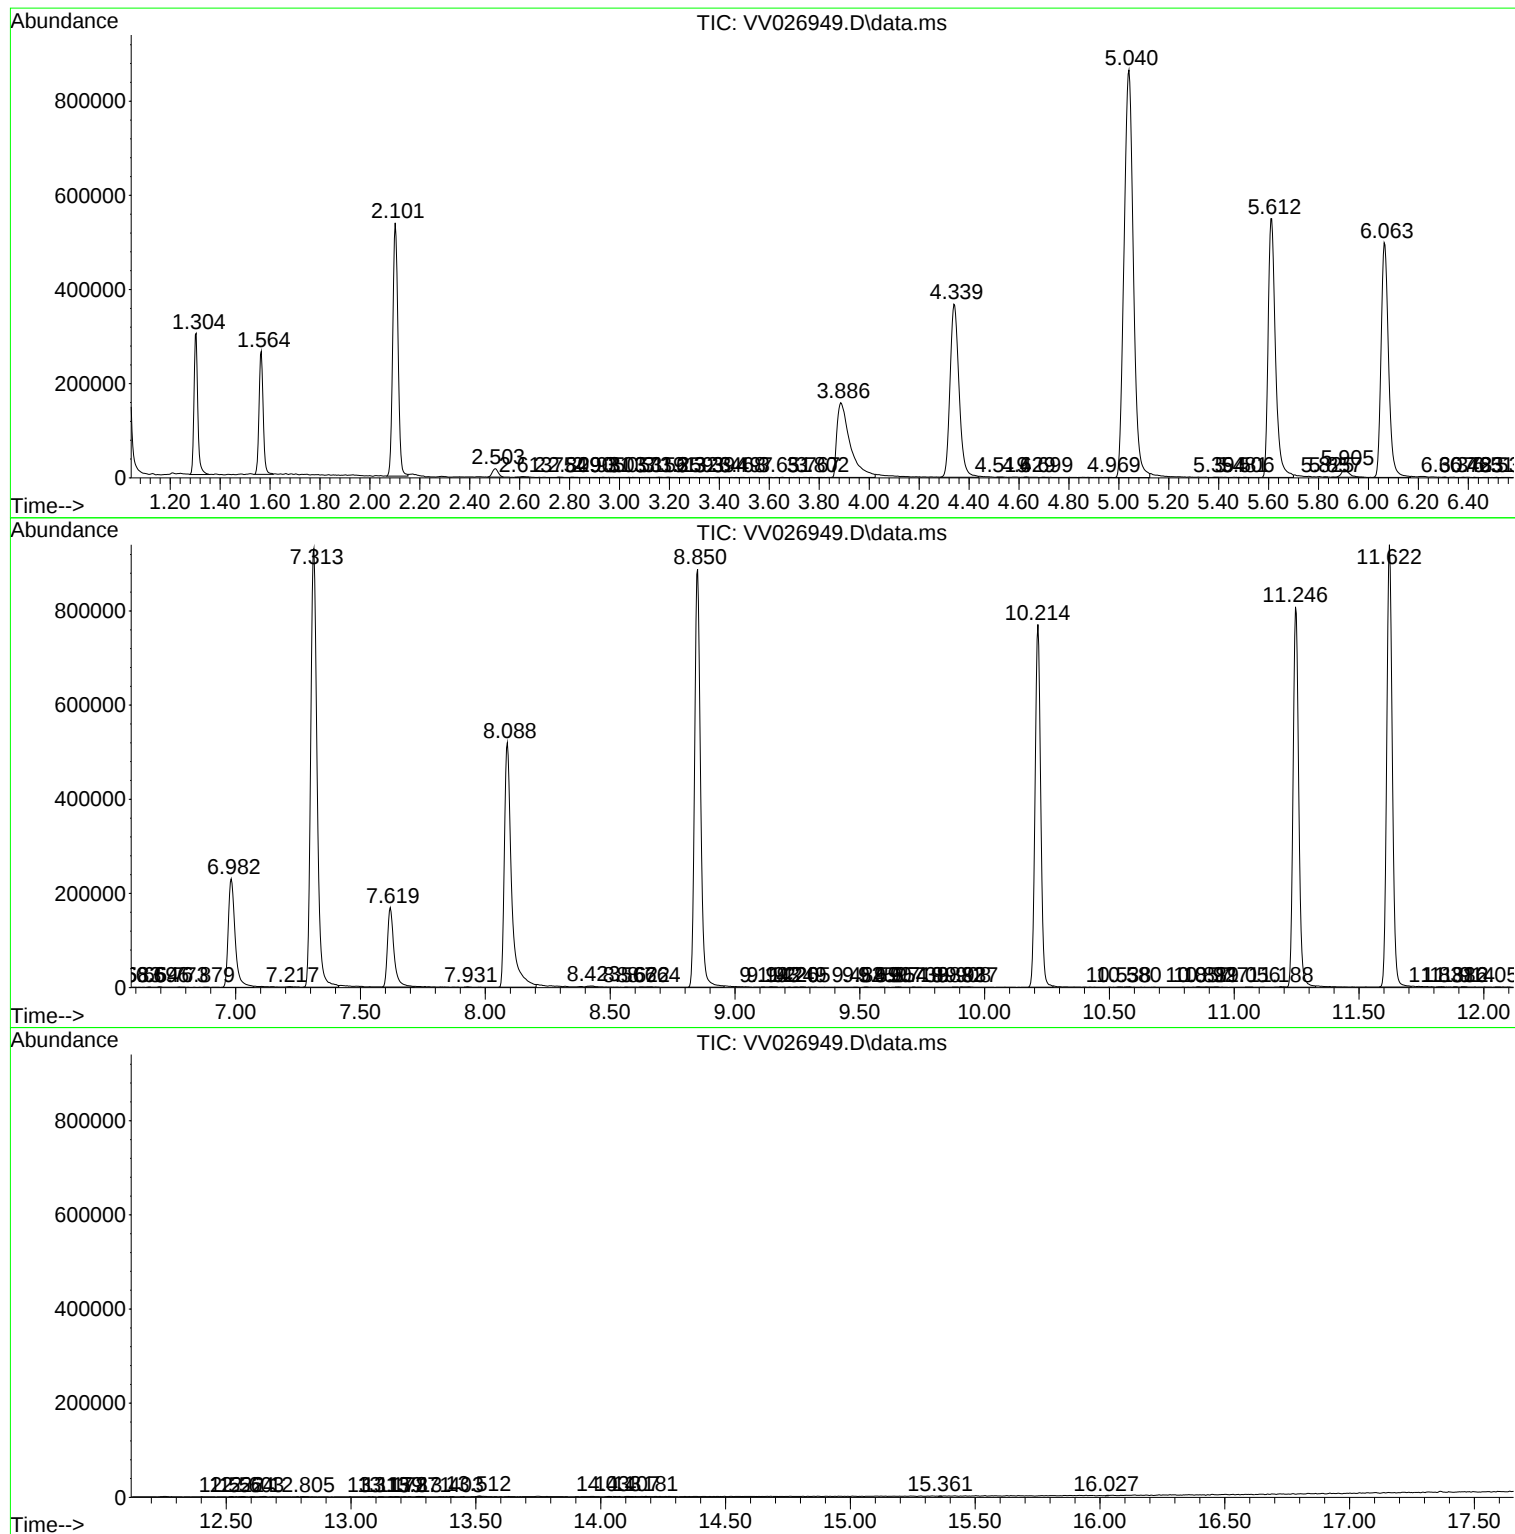

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026949.D
Acq On : 26 Jul 2022 13:51
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026949.D
Acq On : 26 Jul 2022 13:51
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc