

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	308298	324384	14.32%	2.132%
2	1.561	155	162	175	rBV	269527	308475	13.61%	2.027%
3	2.101	320	330	347	rBV	548139	778598	34.36%	5.117%
4	2.433	430	433	435	rBV2	558	390	0.02%	0.003%
5	2.500	444	454	467	rVB	13352	22638	1.00%	0.149%
6	2.603	480	486	488	rBV4	820	929	0.04%	0.006%
7	2.703	514	517	521	rVB2	636	520	0.02%	0.003%
8	2.764	533	536	539	rBV2	614	447	0.02%	0.003%
9	2.815	550	552	556	rVB2	497	277	0.01%	0.002%
10	2.873	566	570	575	rBV2	390	371	0.02%	0.002%
11	3.201	669	672	676	rVB2	580	426	0.02%	0.003%
12	3.886	873	885	929	rBV	157685	563184	24.85%	3.701%
13	4.339	1010	1026	1056	rBV	376756	939538	41.46%	6.174%
14	4.548	1087	1091	1092	rBV3	402	291	0.01%	0.002%
15	4.622	1111	1114	1120	rBV3	441	482	0.02%	0.003%
16	4.654	1122	1124	1128	rVV2	441	350	0.02%	0.002%
17	4.677	1128	1131	1133	rVV2	712	453	0.02%	0.003%
18	4.709	1137	1141	1143	rVB	511	382	0.02%	0.003%
19	5.040	1227	1244	1279	rBV2	879299	2265947	100.00%	14.891%
20	5.227	1301	1302	1304	rBV2	597	285	0.01%	0.002%
21	5.449	1368	1371	1376	rVB4	587	534	0.02%	0.004%
22	5.494	1380	1385	1391	rBV3	641	685	0.03%	0.005%
23	5.551	1399	1403	1407	rBV2	285	280	0.01%	0.002%
24	5.613	1409	1422	1454	rBV	391271	818047	36.10%	5.376%
25	5.825	1486	1488	1492	rVB4	638	424	0.02%	0.003%
26	5.905	1502	1513	1526	rBV2	15142	32968	1.45%	0.217%
27	6.063	1547	1562	1593	rBV	506167	1045882	46.16%	6.873%
28	6.256	1619	1622	1626	rVB4	756	533	0.02%	0.004%
29	6.320	1640	1642	1649	rVB3	559	516	0.02%	0.003%
30	6.407	1664	1669	1672	rBV3	333	314	0.01%	0.002%
31	6.439	1676	1679	1681	rBV	419	311	0.01%	0.002%
32	6.606	1729	1731	1738	rVB2	300	291	0.01%	0.002%
33	6.645	1738	1743	1747	rBV3	503	486	0.02%	0.003%
34	6.674	1747	1752	1754	rBV2	459	407	0.02%	0.003%
35	6.709	1760	1763	1765	rVV3	522	305	0.01%	0.002%
36	6.760	1777	1779	1786	rVB4	392	435	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.899	1816	1822	1826	rBV3	281	286	0.01%	0.002%
38	6.982	1836	1848	1874	rBV	239517	440028	19.42%	2.892%
39	7.198	1907	1915	1917	rBV5	659	859	0.04%	0.006%
40	7.214	1917	1920	1925	rVB4	674	550	0.02%	0.004%
41	7.310	1936	1950	1981	rBV	936893	1658465	73.19%	10.899%
42	7.619	2036	2046	2071	rBV	165615	304484	13.44%	2.001%
43	7.937	2142	2145	2147	rBV2	491	312	0.01%	0.002%
44	7.973	2152	2156	2164	rVB4	740	940	0.04%	0.006%
45	8.008	2164	2167	2171	rBV2	571	340	0.02%	0.002%
46	8.088	2180	2192	2223	rBV	538897	1041690	45.97%	6.845%
47	8.426	2290	2297	2299	rBV4	1235	1585	0.07%	0.010%
48	8.500	2313	2320	2327	rBV6	587	849	0.04%	0.006%
49	8.609	2351	2354	2356	rBV3	666	345	0.02%	0.002%
50	8.641	2361	2364	2367	rBV4	405	286	0.01%	0.002%
51	8.702	2378	2383	2386	rBV3	596	417	0.02%	0.003%
52	8.805	2410	2415	2417	rBV2	399	375	0.02%	0.002%
53	8.850	2417	2429	2463	rBV	636125	1047460	46.23%	6.883%
54	9.001	2473	2476	2478	rBV2	531	290	0.01%	0.002%
55	9.018	2479	2481	2488	rVB5	1128	889	0.04%	0.006%
56	9.149	2520	2522	2525	rVB4	527	275	0.01%	0.002%
57	9.194	2533	2536	2539	rVB	635	389	0.02%	0.003%
58	9.217	2539	2543	2549	rVB3	455	353	0.02%	0.002%
59	9.265	2554	2558	2561	rBV3	523	402	0.02%	0.003%
60	9.358	2583	2587	2590	rBV	355	364	0.02%	0.002%
61	9.413	2602	2604	2609	rVB	563	304	0.01%	0.002%
62	9.510	2631	2634	2639	rBV2	546	691	0.03%	0.005%
63	9.542	2639	2644	2646	rVV4	937	1002	0.04%	0.007%
64	9.555	2646	2648	2655	rVB3	1046	1114	0.05%	0.007%
65	9.635	2668	2673	2680	rBV2	483	647	0.03%	0.004%
66	9.744	2702	2707	2711	rBV2	465	480	0.02%	0.003%
67	9.940	2765	2768	2780	rVB4	617	922	0.04%	0.006%
68	9.998	2780	2786	2790	rBV3	286	338	0.01%	0.002%
69	10.214	2840	2853	2881	rBV	793001	1222979	53.97%	8.037%
70	10.429	2915	2920	2928	rVB4	1292	1698	0.07%	0.011%
71	10.545	2950	2956	2961	rVV3	685	635	0.03%	0.004%
72	10.583	2964	2968	2972	rBV	735	496	0.02%	0.003%
73	10.622	2975	2980	2983	rBV2	459	433	0.02%	0.003%
74	10.841	3044	3048	3050	rBV2	501	291	0.01%	0.002%
75	10.857	3050	3053	3059	rVB3	701	708	0.03%	0.005%
76	10.979	3088	3091	3094	rBV	468	325	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026954.D
 Acq On : 26 Jul 2022 16:20
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.172	3148	3151	3154	rBV3	380	290	0.01%	0.002%
78	11.198	3154	3159	3162	rVB4	713	519	0.02%	0.003%
79	11.246	3162	3174	3196	rBV	572466	896892	39.58%	5.894%
80	11.622	3279	3291	3315	rVV	933480	1463392	64.58%	9.617%
81	11.799	3342	3346	3351	rBV4	468	569	0.03%	0.004%
82	11.921	3380	3384	3386	rBV3	397	301	0.01%	0.002%
83	11.979	3397	3402	3405	rBV2	500	501	0.02%	0.003%
84	12.124	3443	3447	3453	rBV3	375	480	0.02%	0.003%
85	12.432	3537	3543	3549	rBV4	1160	1366	0.06%	0.009%
86	12.654	3609	3612	3617	rBV4	562	512	0.02%	0.003%
87	12.760	3643	3645	3648	rBV3	415	314	0.01%	0.002%
88	13.027	3723	3728	3729	rBV2	378	339	0.01%	0.002%
89	13.233	3790	3792	3795	rVV3	401	273	0.01%	0.002%
90	13.275	3802	3805	3810	rVB2	540	410	0.02%	0.003%
91	13.336	3822	3824	3828	rBV2	493	318	0.01%	0.002%
92	13.435	3852	3855	3861	rVB3	595	451	0.02%	0.003%
93	13.484	3866	3870	3871	rBV2	457	318	0.01%	0.002%
94	13.612	3907	3910	3912	rBV	572	383	0.02%	0.003%
95	13.747	3949	3952	3954	rBV3	664	383	0.02%	0.003%
96	13.799	3964	3968	3970	rBV3	455	378	0.02%	0.002%
97	13.818	3970	3974	3976	rBV3	681	428	0.02%	0.003%
98	14.731	4256	4258	4264	rBV3	564	524	0.02%	0.003%
99	14.979	4333	4335	4338	rBV3	720	513	0.02%	0.003%
100	15.281	4424	4429	4433	rBV3	1179	1233	0.05%	0.008%




Sum of corrected areas: 15217168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026954.D
Acq On : 26 Jul 2022 16:20
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

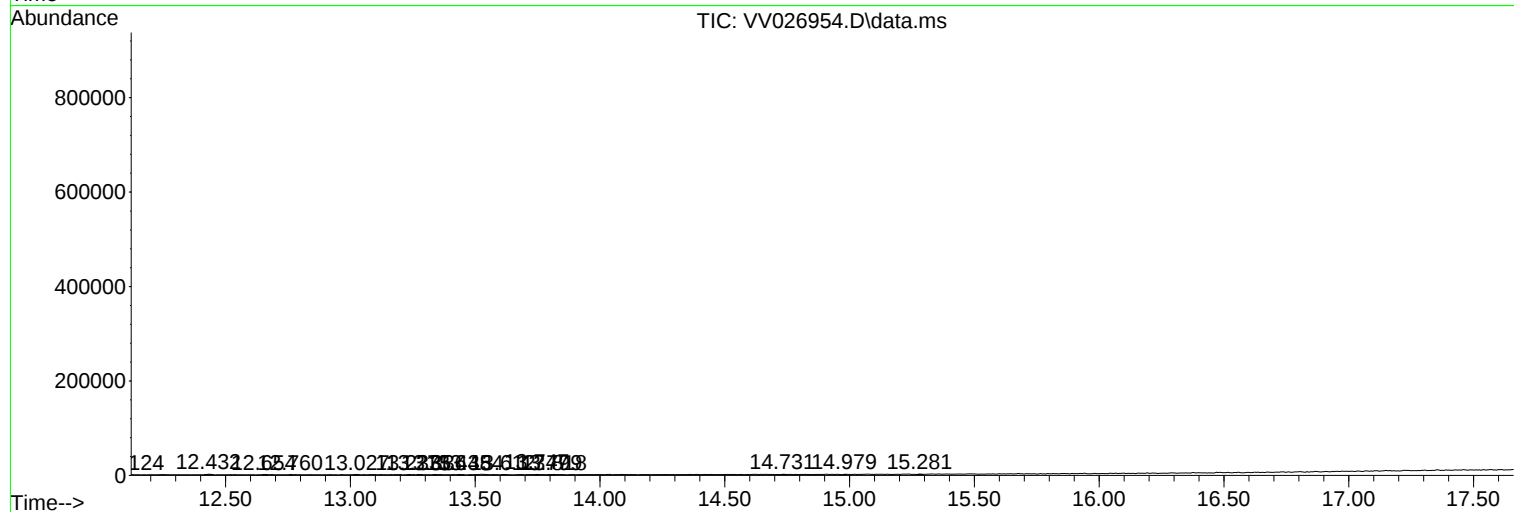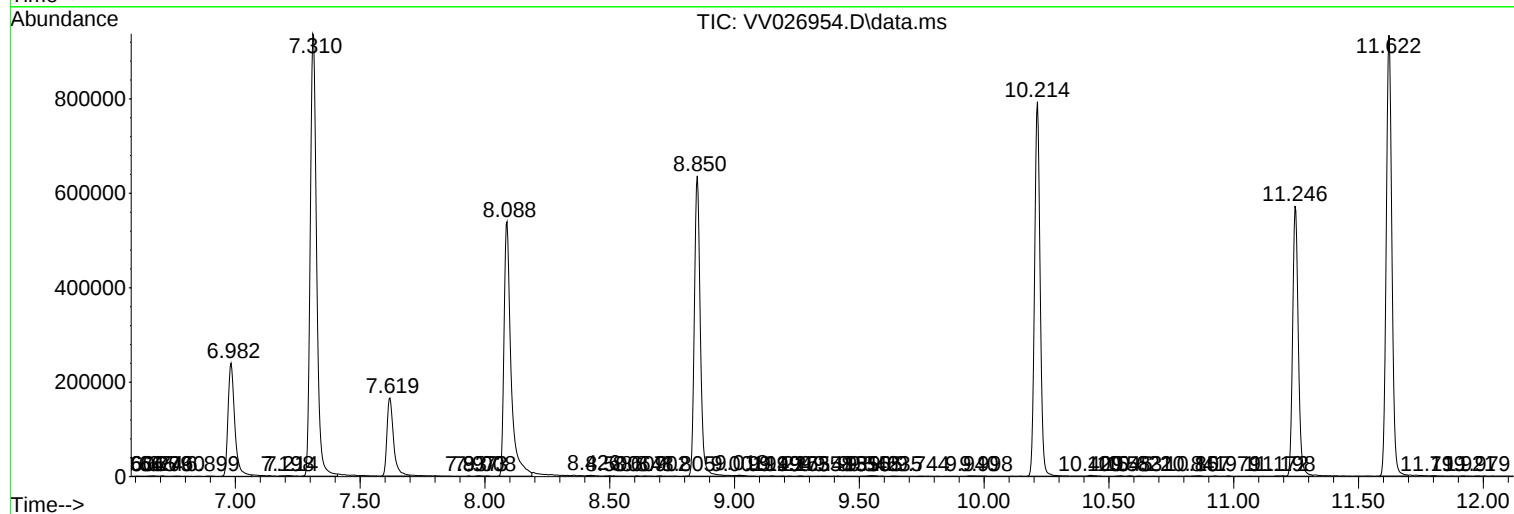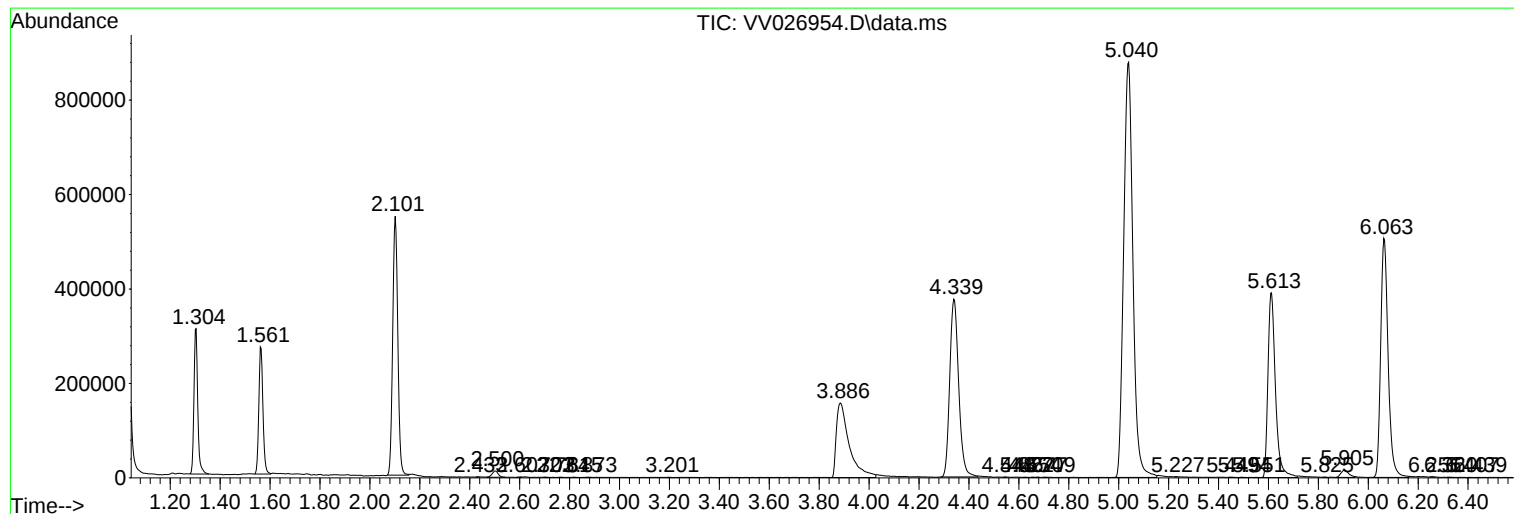

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026954.D
Acq On : 26 Jul 2022 16:20
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026954.D
Acq On : 26 Jul 2022 16:20
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------