

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026956.D
 Acq On : 26 Jul 2022 17:09
 Operator : SY/MD
 Sample : N3841-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	289979	305037	14.21%	1.908%
2	1.564	156	163	174	rVB	251480	282690	13.17%	1.768%
3	2.101	321	330	345	rVB	500499	711245	33.14%	4.449%
4	2.503	448	455	466	rVB2	5369	8074	0.38%	0.051%
5	2.883	571	573	574	rBV2	240	95	0.00%	0.001%
6	2.995	604	608	611	rBV3	346	274	0.01%	0.002%
7	3.018	612	615	617	rVV	277	154	0.01%	0.001%
8	3.034	617	620	625	rVV2	474	411	0.02%	0.003%
9	3.069	629	631	635	rVV2	290	175	0.01%	0.001%
10	3.111	642	644	648	rVB2	356	159	0.01%	0.001%
11	3.133	648	651	654	rBV2	229	196	0.01%	0.001%
12	3.240	682	684	687	rVB2	272	122	0.01%	0.001%
13	3.256	687	689	695	rBV	353	348	0.02%	0.002%
14	3.323	706	710	712	rBV2	224	148	0.01%	0.001%
15	3.336	712	714	717	rVB	352	211	0.01%	0.001%
16	3.362	717	722	724	rBV	396	277	0.01%	0.002%
17	3.416	736	739	743	rBV2	183	176	0.01%	0.001%
18	3.474	754	757	759	rBV2	206	139	0.01%	0.001%
19	3.494	760	763	767	rVV3	283	222	0.01%	0.001%
20	3.526	771	773	777	rVB2	306	185	0.01%	0.001%
21	3.725	833	835	839	rVB2	236	135	0.01%	0.001%
22	3.757	843	845	849	rVB3	194	130	0.01%	0.001%
23	3.780	849	852	855	rBV	202	140	0.01%	0.001%
24	3.886	875	885	929	rBV	153076	515564	24.02%	3.225%
25	4.342	1011	1027	1065	rBV	358834	895334	41.72%	5.601%
26	4.606	1106	1109	1110	rBV2	462	228	0.01%	0.001%
27	4.670	1126	1129	1134	rBV2	482	536	0.02%	0.003%
28	4.699	1137	1138	1139	rBV	337	115	0.01%	0.001%
29	4.780	1162	1163	1164	rVB	535	103	0.00%	0.001%
30	4.809	1164	1172	1173	rBV3	715	574	0.03%	0.004%
31	4.841	1180	1182	1186	rVB4	534	308	0.01%	0.002%
32	4.908	1201	1203	1205	rBV	236	115	0.01%	0.001%
33	4.947	1212	1215	1218	rBV2	302	183	0.01%	0.001%
34	5.043	1225	1245	1277	rBV2	829405	2145991	100.00%	13.424%
35	5.371	1345	1347	1349	rVB3	352	92	0.00%	0.001%
36	5.416	1359	1361	1364	rBV3	358	203	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026956.D
 Acq On : 26 Jul 2022 17:09
 Operator : SY/MD
 Sample : N3841-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	5.612	1409	1422	1454	rBV	597335	1235464	57.57%	7.728%
38	5.908	1502	1514	1527	rBV2	15276	33318	1.55%	0.208%
39	6.066	1549	1563	1598	rBV	487905	1007319	46.94%	6.301%
40	6.346	1648	1650	1654	rVB4	280	185	0.01%	0.001%
41	6.381	1658	1661	1665	rVB2	651	469	0.02%	0.003%
42	6.410	1665	1670	1672	rBV2	488	341	0.02%	0.002%
43	6.468	1684	1688	1689	rBV	291	197	0.01%	0.001%
44	6.519	1697	1704	1708	rBV2	464	519	0.02%	0.003%
45	6.574	1718	1721	1724	rBV2	234	183	0.01%	0.001%
46	6.612	1728	1733	1735	rBV3	223	226	0.01%	0.001%
47	6.625	1735	1737	1739	rBV	186	104	0.00%	0.001%
48	6.725	1764	1768	1771	rVB3	480	377	0.02%	0.002%
49	6.744	1771	1774	1779	rVB3	295	267	0.01%	0.002%
50	6.767	1779	1781	1783	rBV	227	151	0.01%	0.001%
51	6.796	1788	1790	1792	rVV2	284	100	0.00%	0.001%
52	6.812	1792	1795	1799	rVB2	372	276	0.01%	0.002%
53	6.886	1816	1818	1822	rVB3	297	195	0.01%	0.001%
54	6.911	1823	1826	1828	rBV	194	100	0.00%	0.001%
55	6.928	1829	1831	1835	rVB2	284	184	0.01%	0.001%
56	6.985	1835	1849	1876	rBV	218702	420798	19.61%	2.632%
57	7.313	1939	1951	1975	rBV	892945	1551835	72.31%	9.707%
58	7.619	2037	2046	2074	rBV	157861	286407	13.35%	1.792%
59	8.088	2182	2192	2225	rBV	551786	1069402	49.83%	6.689%
60	8.564	2337	2340	2342	rBV2	598	337	0.02%	0.002%
61	8.664	2369	2371	2372	rVB	443	120	0.01%	0.001%
62	8.709	2384	2385	2388	rBV	201	111	0.01%	0.001%
63	8.744	2392	2396	2397	rBV	417	257	0.01%	0.002%
64	8.805	2412	2415	2417	rBV	267	180	0.01%	0.001%
65	8.850	2417	2429	2460	rBV	942961	1544266	71.96%	9.660%
66	9.220	2541	2544	2547	rVB2	733	512	0.02%	0.003%
67	9.265	2556	2558	2561	rVB2	264	117	0.01%	0.001%
68	9.342	2578	2582	2585	rBV2	381	336	0.02%	0.002%
69	9.522	2635	2638	2639	rBV	368	197	0.01%	0.001%
70	9.606	2662	2664	2670	rBV3	530	320	0.01%	0.002%
71	9.632	2670	2672	2675	rVB2	424	213	0.01%	0.001%
72	9.664	2680	2682	2685	rBV	271	146	0.01%	0.001%
73	9.786	2718	2720	2727	rVB3	274	191	0.01%	0.001%
74	9.815	2727	2729	2731	rVB2	345	158	0.01%	0.001%
75	9.831	2731	2734	2736	rBV	334	203	0.01%	0.001%
76	9.905	2754	2757	2759	rBV	273	163	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026956.D
 Acq On : 26 Jul 2022 17:09
 Operator : SY/MD
 Sample : N3841-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.943	2763	2769	2772	rBV2	843	745	0.03%	0.005%
78	9.972	2776	2778	2782	rVB2	384	275	0.01%	0.002%
79	10.005	2786	2788	2790	rBV2	248	134	0.01%	0.001%
80	10.133	2824	2828	2831	rBV2	253	250	0.01%	0.002%
81	10.214	2841	2853	2877	rBV	768161	1195361	55.70%	7.477%
82	10.358	2891	2898	2910	rVB2	7607	11945	0.56%	0.075%
83	10.542	2952	2955	2959	rBV2	483	374	0.02%	0.002%
84	10.641	2983	2986	2987	rBV	201	91	0.00%	0.001%
85	10.693	2998	3002	3004	rBV2	272	236	0.01%	0.001%
86	10.754	3018	3021	3024	rBV	457	292	0.01%	0.002%
87	10.767	3024	3025	3026	rBV	331	106	0.00%	0.001%
88	10.853	3049	3052	3053	rBV2	678	437	0.02%	0.003%
89	10.927	3068	3075	3081	rBV2	768	1274	0.06%	0.008%
90	11.030	3104	3107	3109	rBV	363	194	0.01%	0.001%
91	11.053	3109	3114	3116	rBV	409	302	0.01%	0.002%
92	11.127	3135	3137	3140	rBV2	311	212	0.01%	0.001%
93	11.249	3163	3175	3199	rBV	858255	1325123	61.75%	8.289%
94	11.535	3256	3264	3279	rBV3	10456	20234	0.94%	0.127%
95	11.622	3280	3291	3314	rVV	889528	1399479	65.21%	8.754%
96	12.619	3598	3601	3607	rVB2	670	648	0.03%	0.004%
97	12.648	3607	3610	3612	rBV2	639	365	0.02%	0.002%
98	12.664	3612	3615	3618	rBV3	606	443	0.02%	0.003%
99	12.895	3681	3687	3689	rBV2	465	535	0.02%	0.003%
100	13.673	3924	3929	3935	rBV4	834	1226	0.06%	0.008%




Sum of corrected areas: 15986614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026956.D
Acq On : 26 Jul 2022 17:09
Operator : SY/MD
Sample : N3841-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

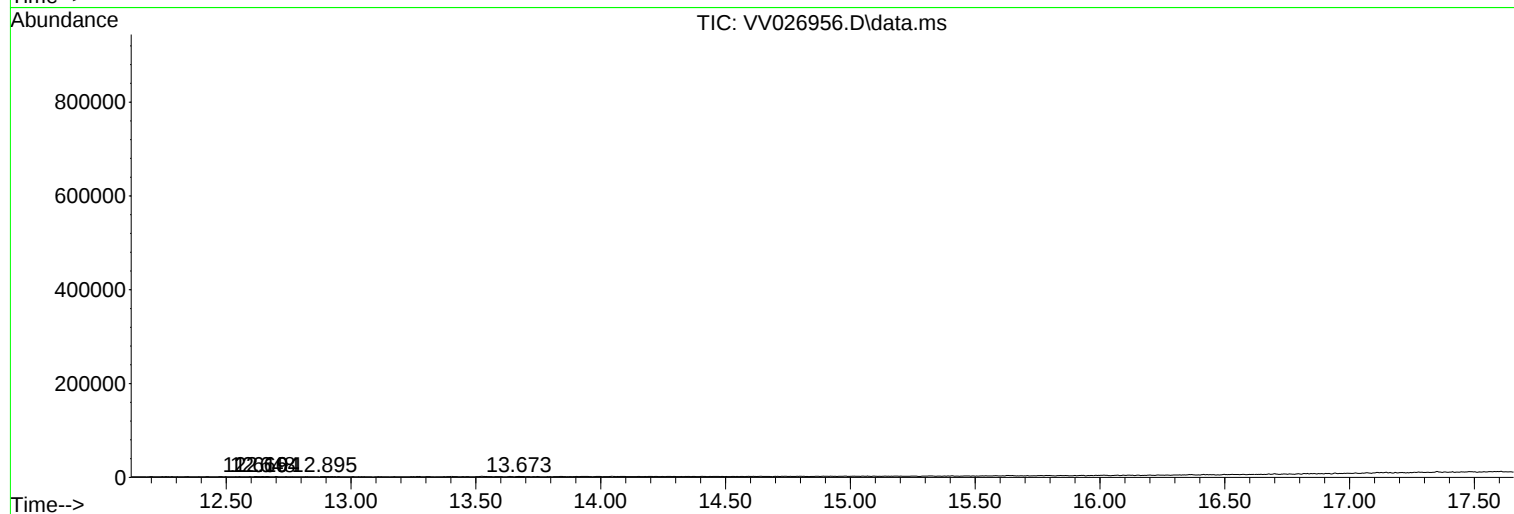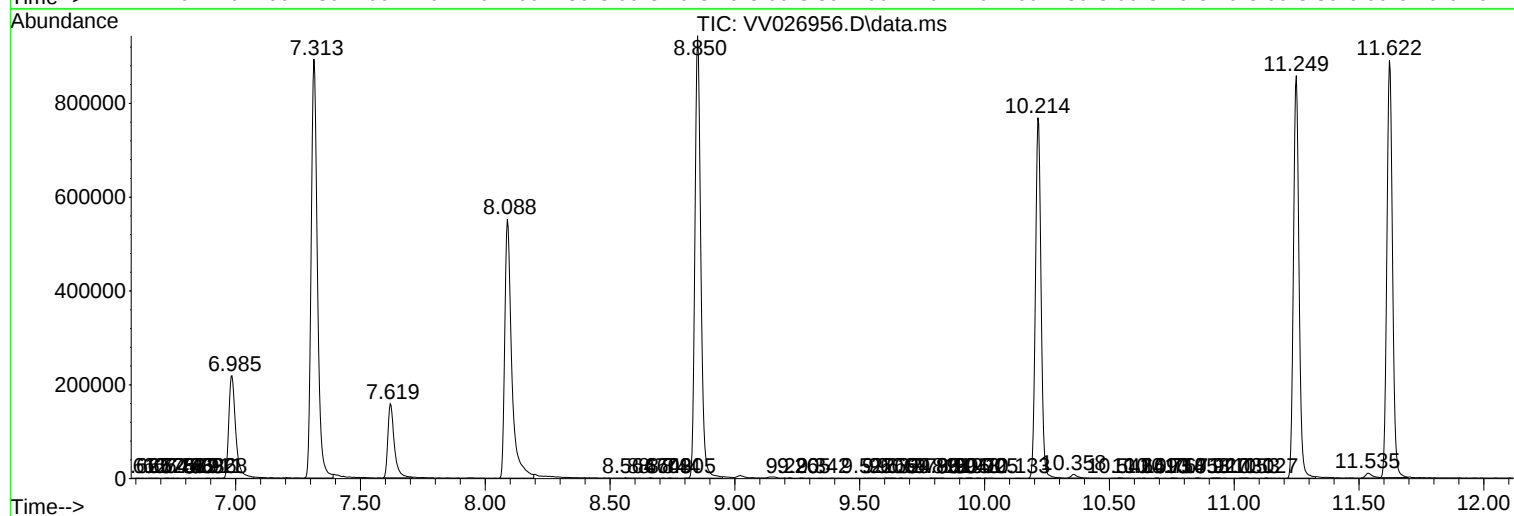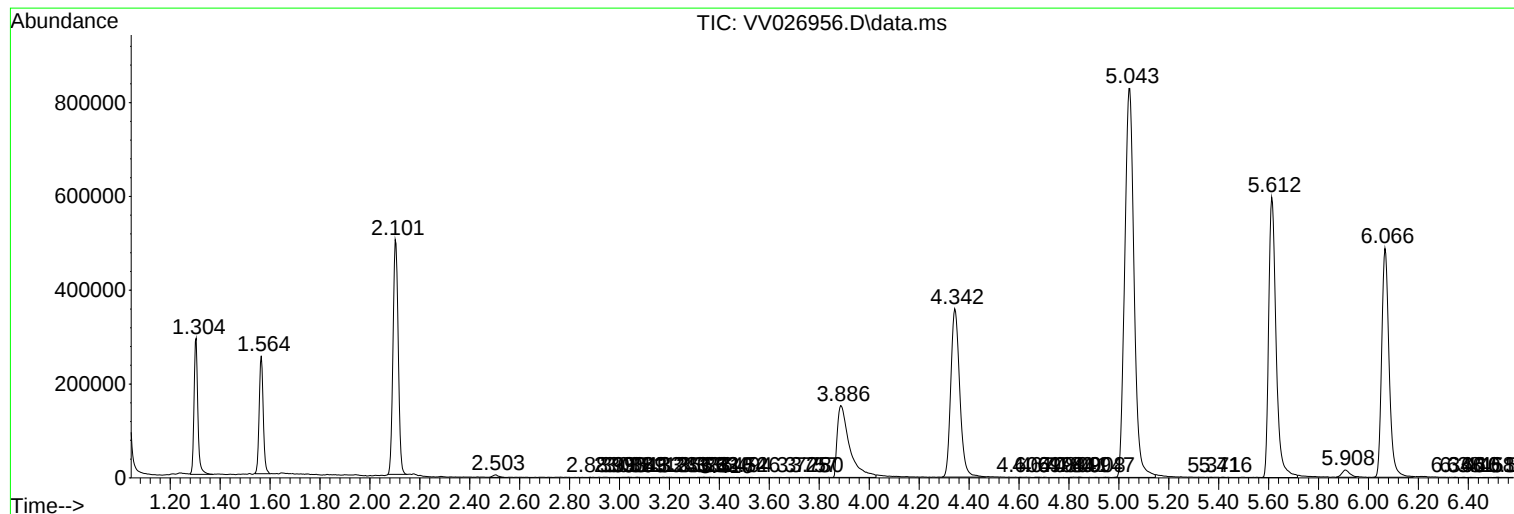

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026956.D
Acq On : 26 Jul 2022 17:09
Operator : SY/MD
Sample : N3841-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026956.D
Acq On : 26 Jul 2022 17:09
Operator : SY/MD
Sample : N3841-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------