

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026957.D
 Acq On : 26 Jul 2022 17:33
 Operator : SY/MD
 Sample : N3841-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	270449	283295	13.80%	1.849%
2	1.564	155	163	177	rVB	231533	263231	12.82%	1.718%
3	2.101	320	330	345	rBV	477384	679039	33.08%	4.432%
4	2.503	447	455	465	rVB	5394	8969	0.44%	0.059%
5	2.616	486	490	495	rVB3	374	408	0.02%	0.003%
6	2.712	518	520	524	rBV	443	363	0.02%	0.002%
7	2.738	526	528	530	rVV2	631	368	0.02%	0.002%
8	2.767	530	537	547	rVB4	3460	6604	0.32%	0.043%
9	2.834	553	558	563	rBV2	304	357	0.02%	0.002%
10	3.079	627	634	635	rBV3	427	432	0.02%	0.003%
11	3.127	644	649	655	rVB	359	446	0.02%	0.003%
12	3.182	662	666	670	rBV2	372	413	0.02%	0.003%
13	3.355	716	720	725	rBV2	411	293	0.01%	0.002%
14	3.381	725	728	732	rVB2	364	290	0.01%	0.002%
15	3.715	827	832	837	rBV2	411	358	0.02%	0.002%
16	3.831	866	868	873	rVB	725	518	0.03%	0.003%
17	3.883	873	884	921	rBV	152751	477098	23.24%	3.114%
18	4.342	1010	1027	1058	rBV	341802	856631	41.73%	5.591%
19	4.593	1103	1105	1109	rVB2	518	290	0.01%	0.002%
20	4.677	1127	1131	1134	rBV3	567	508	0.02%	0.003%
21	4.825	1174	1177	1182	rVV4	822	878	0.04%	0.006%
22	4.931	1205	1210	1211	rBV	451	282	0.01%	0.002%
23	5.043	1227	1245	1288	rBV2	787973	2052775	100.00%	13.397%
24	5.268	1312	1315	1318	rBV4	744	484	0.02%	0.003%
25	5.310	1324	1328	1330	rBV2	349	261	0.01%	0.002%
26	5.339	1334	1337	1340	rBV3	641	385	0.02%	0.003%
27	5.400	1354	1356	1361	rVB2	384	299	0.01%	0.002%
28	5.493	1380	1385	1386	rBV3	528	393	0.02%	0.003%
29	5.612	1410	1422	1459	rBV	580955	1207663	58.83%	7.882%
30	5.863	1496	1500	1501	rBV4	574	347	0.02%	0.002%
31	5.908	1503	1514	1528	rVV3	13814	29994	1.46%	0.196%
32	5.976	1533	1535	1539	rVB4	635	338	0.02%	0.002%
33	6.066	1549	1563	1599	rBV	466637	960631	46.80%	6.269%
34	6.268	1624	1626	1628	rVB3	654	270	0.01%	0.002%
35	6.291	1628	1633	1638	rVB5	1170	1377	0.07%	0.009%
36	6.323	1638	1643	1644	rBV	591	428	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026957.D
 Acq On : 26 Jul 2022 17:33
 Operator : SY/MD
 Sample : N3841-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.371	1655	1658	1661	rVB	526	289	0.01%	0.002%
38	6.410	1667	1670	1674	rVB2	493	334	0.02%	0.002%
39	6.452	1681	1683	1688	rVB2	396	263	0.01%	0.002%
40	6.651	1742	1745	1749	rVV2	433	399	0.02%	0.003%
41	6.815	1792	1796	1799	rBV2	372	302	0.01%	0.002%
42	6.905	1822	1824	1829	rVB	451	280	0.01%	0.002%
43	6.985	1836	1849	1872	rBV	209477	396818	19.33%	2.590%
44	7.207	1913	1918	1920	rBV5	919	869	0.04%	0.006%
45	7.313	1939	1951	1988	rBV	833922	1484025	72.29%	9.685%
46	7.622	2037	2047	2073	rBV	150972	269478	13.13%	1.759%
47	7.853	2116	2119	2124	rBV4	563	669	0.03%	0.004%
48	7.931	2137	2143	2144	rBV2	1202	867	0.04%	0.006%
49	7.982	2154	2159	2166	rVB6	1585	1897	0.09%	0.012%
50	8.040	2172	2177	2182	rBV3	375	413	0.02%	0.003%
51	8.088	2182	2192	2231	rBV	506257	1002167	48.82%	6.541%
52	8.561	2337	2339	2343	rVB	551	309	0.02%	0.002%
53	8.587	2343	2347	2349	rBV	593	475	0.02%	0.003%
54	8.706	2381	2384	2388	rBV3	430	327	0.02%	0.002%
55	8.850	2418	2429	2465	rBV	926172	1526952	74.38%	9.965%
56	9.014	2477	2480	2481	rBV2	934	579	0.03%	0.004%
57	9.088	2500	2503	2505	rBV2	549	281	0.01%	0.002%
58	9.130	2513	2516	2517	rBV2	763	395	0.02%	0.003%
59	9.143	2517	2520	2523	rVV3	608	543	0.03%	0.004%
60	9.249	2548	2553	2556	rBV2	571	642	0.03%	0.004%
61	9.339	2579	2581	2585	rBV2	534	325	0.02%	0.002%
62	9.358	2585	2587	2590	rVV2	381	257	0.01%	0.002%
63	9.394	2594	2598	2602	rBV4	540	415	0.02%	0.003%
64	9.455	2613	2617	2622	rBV2	479	578	0.03%	0.004%
65	9.542	2638	2644	2646	rBV3	520	526	0.03%	0.003%
66	9.593	2656	2660	2665	rBV2	564	645	0.03%	0.004%
67	9.619	2665	2668	2671	rVV	561	361	0.02%	0.002%
68	9.738	2701	2705	2707	rBV	455	351	0.02%	0.002%
69	9.783	2717	2719	2724	rVV3	487	301	0.01%	0.002%
70	9.812	2724	2728	2734	rVB2	310	337	0.02%	0.002%
71	9.934	2760	2766	2774	rVB3	775	1250	0.06%	0.008%
72	10.046	2796	2801	2803	rBV	289	283	0.01%	0.002%
73	10.214	2839	2853	2878	rBV	736761	1140485	55.56%	7.443%
74	10.355	2890	2897	2902	rBV4	1908	2563	0.12%	0.017%
75	10.381	2902	2905	2907	rBV2	1050	630	0.03%	0.004%
76	10.541	2950	2955	2957	rBV4	554	449	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026957.D
 Acq On : 26 Jul 2022 17:33
 Operator : SY/MD
 Sample : N3841-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.586	2964	2969	2970	rBV2	777	474	0.02%	0.003%
78	10.660	2990	2992	2998	rVB2	339	256	0.01%	0.002%
79	10.750	3015	3020	3024	rBV2	494	401	0.02%	0.003%
80	10.853	3048	3052	3054	rBV2	482	334	0.02%	0.002%
81	10.918	3069	3072	3074	rBV	709	539	0.03%	0.004%
82	10.956	3081	3084	3090	rVB2	518	424	0.02%	0.003%
83	10.995	3093	3096	3101	rBV3	329	340	0.02%	0.002%
84	11.120	3131	3135	3139	rVB3	541	469	0.02%	0.003%
85	11.249	3163	3175	3203	rBV	839095	1291649	62.92%	8.430%
86	11.413	3223	3226	3230	rVB3	717	412	0.02%	0.003%
87	11.541	3258	3266	3274	rVV4	3561	6788	0.33%	0.044%
88	11.622	3278	3291	3322	rBV	846977	1331779	64.88%	8.692%
89	11.808	3345	3349	3350	rBV2	766	481	0.02%	0.003%
90	12.246	3482	3485	3489	rBV2	463	462	0.02%	0.003%
91	12.342	3513	3515	3517	rBV2	506	273	0.01%	0.002%
92	12.635	3602	3606	3607	rBV2	493	347	0.02%	0.002%
93	13.030	3727	3729	3738	rVB3	693	674	0.03%	0.004%
94	13.175	3767	3774	3779	rBV3	789	968	0.05%	0.006%
95	13.300	3810	3813	3816	rBV2	549	387	0.02%	0.003%
96	13.474	3861	3867	3872	rBV4	626	907	0.04%	0.006%
97	14.091	4057	4059	4063	rBV4	380	366	0.02%	0.002%
98	14.496	4183	4185	4188	rBV2	510	316	0.02%	0.002%
99	15.625	4531	4536	4538	rBV4	1103	1179	0.06%	0.008%
100	16.229	4720	4724	4727	rVB	10979	6118	0.30%	0.040%




Sum of corrected areas: 15322388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026957.D
Acq On : 26 Jul 2022 17:33
Operator : SY/MD
Sample : N3841-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

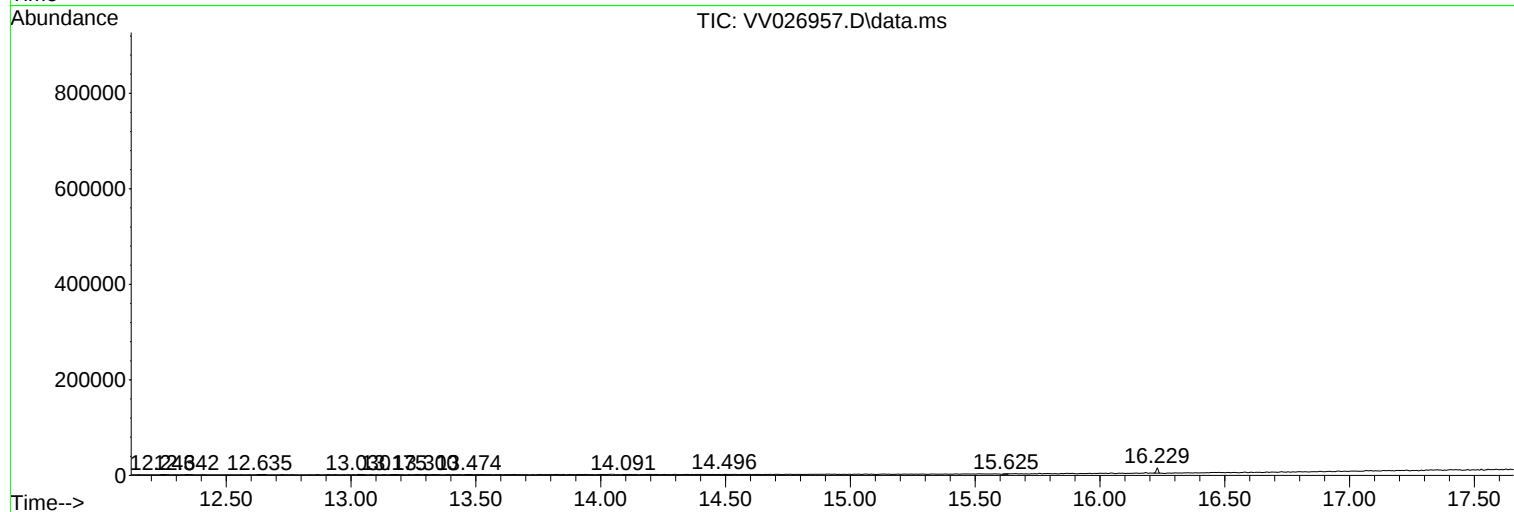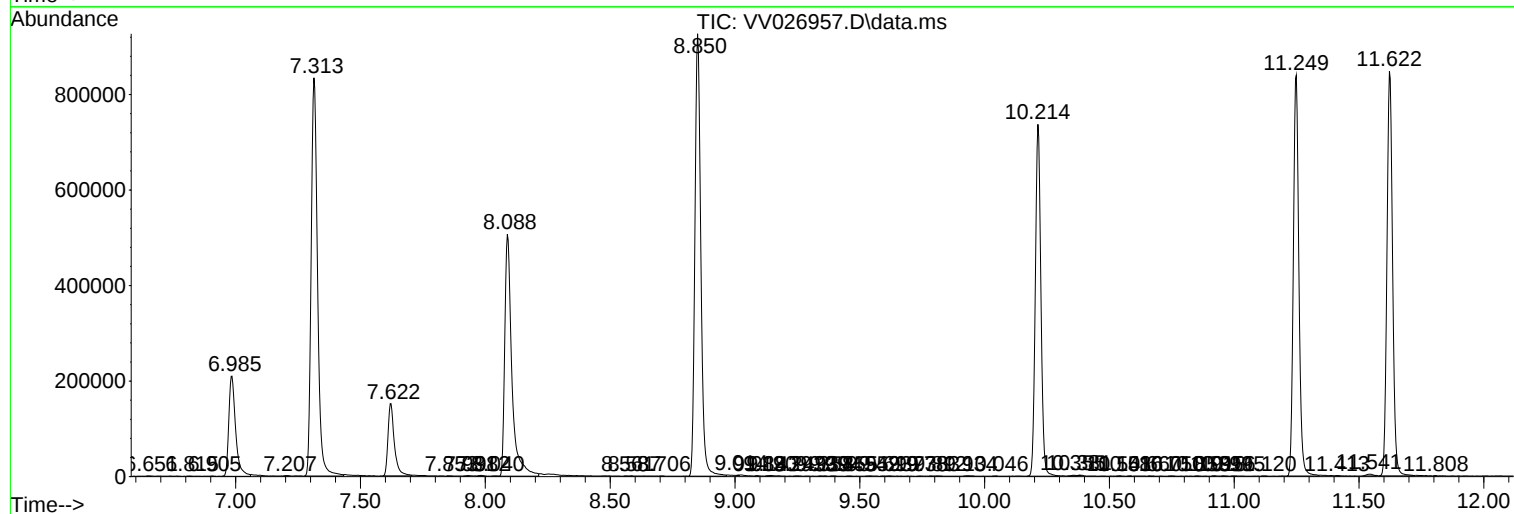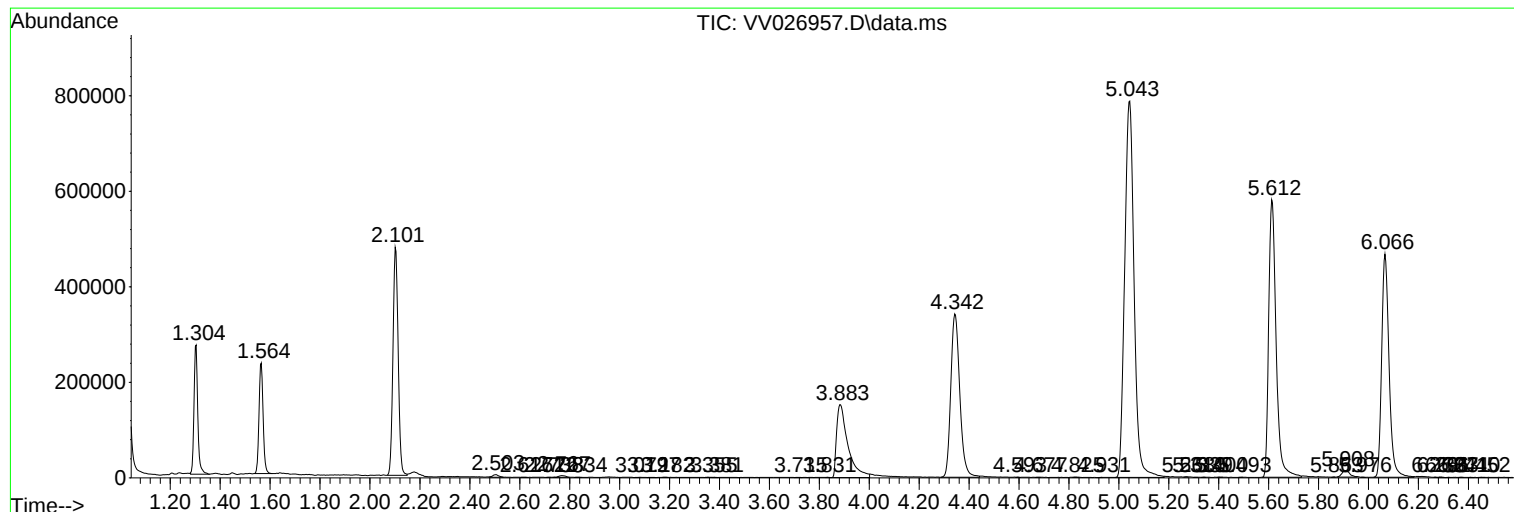

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026957.D
Acq On : 26 Jul 2022 17:33
Operator : SY/MD
Sample : N3841-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026957.D
Acq On : 26 Jul 2022 17:33
Operator : SY/MD
Sample : N3841-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------