

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026958.D
 Acq On : 26 Jul 2022 17:58
 Operator : SY/MD
 Sample : N3841-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.131	24	28	39	rVB	20941	24262	1.18%	0.160%
2	1.301	74	81	100	rVB	269895	283184	13.82%	1.867%
3	1.565	155	163	175	rBV	242994	272688	13.31%	1.798%
4	2.102	320	330	347	rBV	475237	676403	33.01%	4.459%
5	2.282	383	386	387	rBV2	1189	669	0.03%	0.004%
6	2.500	449	454	467	rVB5	5046	8492	0.41%	0.056%
7	2.548	467	469	474	rVB2	391	303	0.01%	0.002%
8	2.600	482	485	493	rVB2	545	553	0.03%	0.004%
9	2.642	493	498	499	rBV2	579	519	0.03%	0.003%
10	2.661	501	504	507	rBV3	686	531	0.03%	0.004%
11	2.777	539	540	546	rVB4	560	349	0.02%	0.002%
12	2.960	591	597	602	rBV2	598	817	0.04%	0.005%
13	3.044	620	623	628	rVB3	564	362	0.02%	0.002%
14	3.073	628	632	637	rVB2	412	313	0.02%	0.002%
15	3.172	658	663	666	rBV	306	336	0.02%	0.002%
16	3.352	714	719	723	rBV2	384	302	0.01%	0.002%
17	3.404	731	735	743	rBV3	424	490	0.02%	0.003%
18	3.635	804	807	813	rBV2	331	357	0.02%	0.002%
19	3.786	851	854	861	rVB2	364	365	0.02%	0.002%
20	3.818	861	864	869	rVB2	368	296	0.01%	0.002%
21	3.886	875	885	921	rBV	143150	473371	23.10%	3.121%
22	4.275	1003	1006	1010	rBV4	695	551	0.03%	0.004%
23	4.343	1010	1027	1069	rVV	349310	862723	42.10%	5.687%
24	4.490	1071	1073	1077	rVB3	1076	670	0.03%	0.004%
25	4.667	1125	1128	1131	rVB3	662	347	0.02%	0.002%
26	4.690	1131	1135	1136	rBV2	545	345	0.02%	0.002%
27	5.040	1227	1244	1293	rBV2	791058	2049178	100.00%	13.509%
28	5.243	1305	1307	1312	rVB4	608	331	0.02%	0.002%
29	5.288	1318	1321	1325	rVB4	687	389	0.02%	0.003%
30	5.371	1345	1347	1350	rVV3	475	315	0.02%	0.002%
31	5.545	1395	1401	1403	rBV2	498	427	0.02%	0.003%
32	5.613	1410	1422	1458	rBV	557876	1144884	55.87%	7.547%
33	5.831	1487	1490	1494	rBV4	640	513	0.03%	0.003%
34	5.905	1504	1513	1530	rVV5	9076	19771	0.96%	0.130%
35	6.066	1549	1563	1589	rBV	469609	963880	47.04%	6.354%
36	6.281	1627	1630	1636	rVB6	718	724	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026958.D
 Acq On : 26 Jul 2022 17:58
 Operator : SY/MD
 Sample : N3841-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.394	1663	1665	1667	rBV	606	348	0.02%	0.002%
38	6.449	1676	1682	1685	rBV2	456	499	0.02%	0.003%
39	6.481	1689	1692	1695	rBV4	500	358	0.02%	0.002%
40	6.571	1716	1720	1723	rVV2	327	342	0.02%	0.002%
41	6.892	1818	1820	1827	rVB2	524	456	0.02%	0.003%
42	6.986	1838	1849	1880	rBV	213024	400787	19.56%	2.642%
43	7.207	1913	1918	1920	rBV3	559	516	0.03%	0.003%
44	7.243	1927	1929	1935	rVB5	669	594	0.03%	0.004%
45	7.314	1938	1951	1985	rBV	832325	1480403	72.24%	9.759%
46	7.529	2016	2018	2021	rVB	652	341	0.02%	0.002%
47	7.545	2021	2023	2030	rVB3	713	608	0.03%	0.004%
48	7.622	2037	2047	2075	rBV	150632	275998	13.47%	1.819%
49	7.863	2118	2122	2125	rVB3	598	543	0.03%	0.004%
50	7.937	2136	2145	2148	rBV4	2185	3294	0.16%	0.022%
51	7.979	2156	2158	2171	rVB4	905	1333	0.07%	0.009%
52	8.088	2182	2192	2232	rBV	520097	1019032	49.73%	6.718%
53	8.413	2288	2293	2296	rBV5	864	781	0.04%	0.005%
54	8.490	2315	2317	2320	rBV2	454	317	0.02%	0.002%
55	8.555	2335	2337	2341	rVB3	583	388	0.02%	0.003%
56	8.741	2390	2395	2397	rBV2	426	344	0.02%	0.002%
57	8.850	2417	2429	2453	rBV	877417	1437499	70.15%	9.476%
58	9.117	2508	2512	2516	rBV4	626	520	0.03%	0.003%
59	9.143	2516	2520	2523	rVB4	679	576	0.03%	0.004%
60	9.178	2529	2531	2537	rVB3	626	428	0.02%	0.003%
61	9.268	2557	2559	2562	rBV2	544	379	0.02%	0.002%
62	9.555	2646	2648	2650	rVB	626	343	0.02%	0.002%
63	9.606	2659	2664	2668	rVB	518	440	0.02%	0.003%
64	9.815	2726	2729	2736	rVB3	460	513	0.03%	0.003%
65	9.937	2757	2767	2768	rVV4	462	622	0.03%	0.004%
66	10.214	2841	2853	2878	rBV	745240	1165099	56.86%	7.681%
67	10.378	2901	2904	2914	rVB6	2505	3278	0.16%	0.022%
68	10.545	2954	2956	2960	rVB4	620	400	0.02%	0.003%
69	10.571	2960	2964	2966	rBV4	461	359	0.02%	0.002%
70	10.709	3005	3007	3010	rVB2	585	297	0.01%	0.002%
71	10.738	3012	3016	3020	rVV2	447	421	0.02%	0.003%
72	10.764	3020	3024	3028	rVB3	602	532	0.03%	0.004%
73	10.796	3028	3034	3040	rBV3	525	779	0.04%	0.005%
74	10.857	3048	3053	3058	rVB4	697	579	0.03%	0.004%
75	11.249	3163	3175	3207	rBV	793770	1230844	60.07%	8.114%
76	11.413	3223	3226	3229	rVB4	618	362	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026958.D
 Acq On : 26 Jul 2022 17:58
 Operator : SY/MD
 Sample : N3841-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.535	3259	3264	3266	rBV3	2928	2676	0.13%	0.018%
78	11.622	3279	3291	3312	rVV	860099	1335062	65.15%	8.801%
79	11.847	3355	3361	3365	rBV4	534	572	0.03%	0.004%
80	12.664	3613	3615	3620	rVB3	510	320	0.02%	0.002%
81	13.011	3718	3723	3727	rVV3	381	509	0.02%	0.003%
82	13.223	3786	3789	3793	rBV	379	403	0.02%	0.003%
83	13.288	3807	3809	3813	rBV2	621	315	0.02%	0.002%
84	13.423	3845	3851	3853	rBV3	508	614	0.03%	0.004%
85	13.493	3869	3873	3875	rVB2	461	324	0.02%	0.002%
86	13.522	3879	3882	3886	rVV2	586	494	0.02%	0.003%
87	13.596	3902	3905	3908	rBV	532	487	0.02%	0.003%
88	13.632	3914	3916	3925	rVB4	401	471	0.02%	0.003%
89	13.686	3931	3933	3940	rVB2	515	436	0.02%	0.003%
90	13.738	3944	3949	3955	rVB4	714	689	0.03%	0.005%
91	13.773	3958	3960	3966	rVB4	531	388	0.02%	0.003%
92	13.853	3983	3985	3989	rBV3	418	341	0.02%	0.002%
93	13.898	3995	3999	4000	rBV	514	406	0.02%	0.003%
94	14.657	4233	4235	4238	rBV	525	330	0.02%	0.002%
95	14.754	4263	4265	4267	rBV	530	314	0.02%	0.002%
96	14.911	4312	4314	4317	rBV2	621	384	0.02%	0.003%
97	14.927	4317	4319	4324	rVV4	720	505	0.02%	0.003%
98	14.976	4330	4334	4338	rBV3	898	980	0.05%	0.006%
99	15.471	4486	4488	4491	rBV4	867	416	0.02%	0.003%
100	15.754	4574	4576	4579	rBV4	915	477	0.02%	0.003%




Sum of corrected areas: 15169475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026958.D
Acq On : 26 Jul 2022 17:58
Operator : SY/MD
Sample : N3841-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

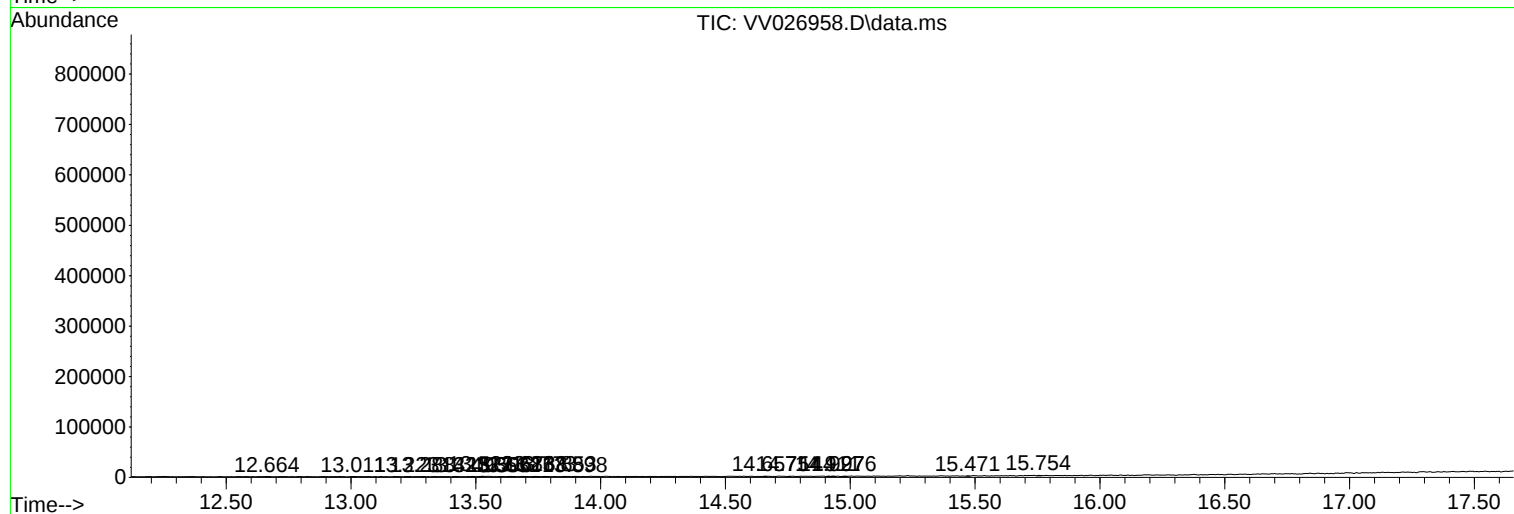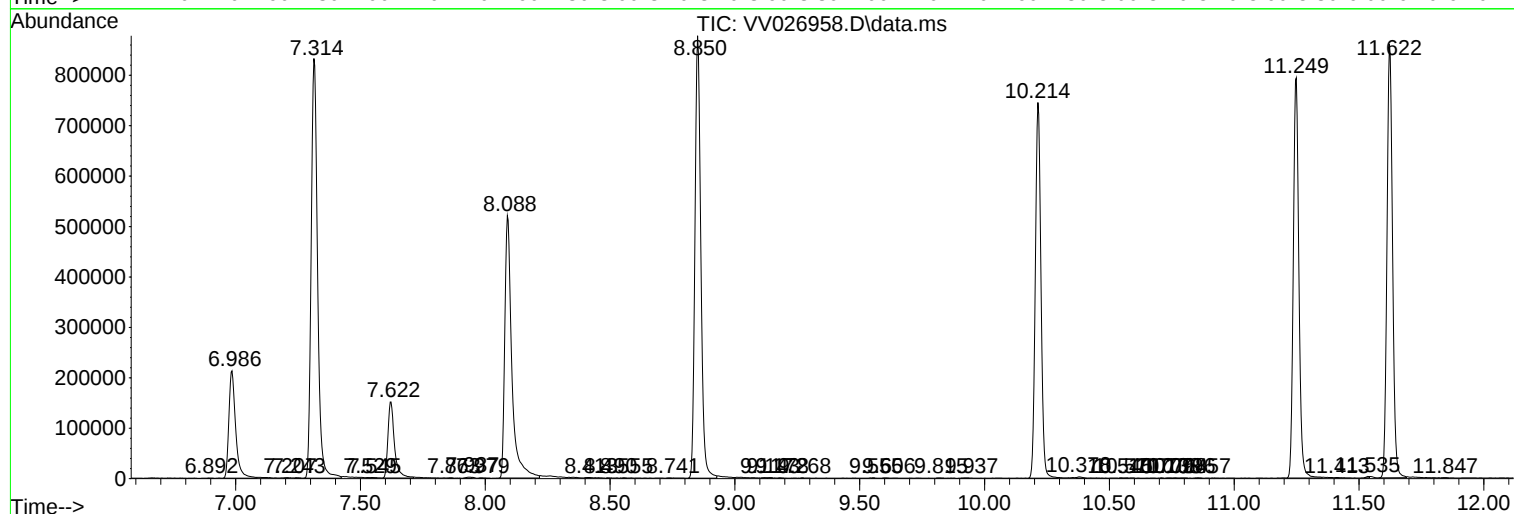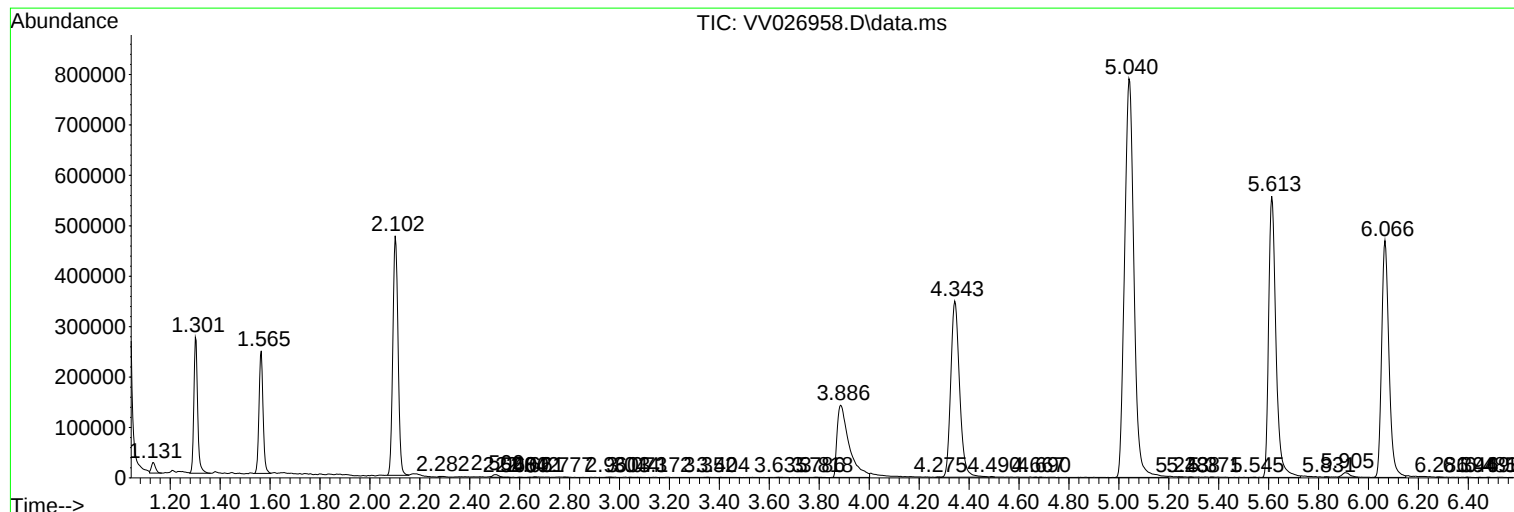

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026958.D
Acq On : 26 Jul 2022 17:58
Operator : SY/MD
Sample : N3841-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026958.D
Acq On : 26 Jul 2022 17:58
Operator : SY/MD
Sample : N3841-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc