

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026959.D
 Acq On : 26 Jul 2022 18:22
 Operator : SY/MD
 Sample : N3841-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	100	rVB	273201	286396	13.93%	1.886%
2	1.564	155	163	179	rBV	242240	279989	13.62%	1.843%
3	2.101	320	330	345	rBV	476699	681514	33.14%	4.487%
4	2.503	446	455	467	rVB2	8888	14522	0.71%	0.096%
5	2.600	482	485	489	rBV3	560	395	0.02%	0.003%
6	2.738	523	528	531	rBV3	536	617	0.03%	0.004%
7	2.761	531	535	538	rVV5	657	597	0.03%	0.004%
8	2.889	571	575	579	rBV3	292	295	0.01%	0.002%
9	2.960	588	597	613	rVV6	2485	5758	0.28%	0.038%
10	3.037	618	621	627	rVB3	806	727	0.04%	0.005%
11	3.069	628	631	635	rBV2	468	352	0.02%	0.002%
12	3.111	641	644	650	rVB2	448	339	0.02%	0.002%
13	3.146	651	655	659	rBV2	410	405	0.02%	0.003%
14	3.204	670	673	679	rVV3	444	444	0.02%	0.003%
15	3.606	794	798	808	rVB2	538	626	0.03%	0.004%
16	3.889	873	886	921	rBV2	141627	479454	23.32%	3.157%
17	4.342	1010	1027	1059	rBV	345728	863001	41.97%	5.682%
18	4.889	1194	1197	1201	rVB3	359	299	0.01%	0.002%
19	5.043	1227	1245	1284	rBV2	788185	2056295	100.00%	13.538%
20	5.362	1340	1344	1345	rBV3	589	459	0.02%	0.003%
21	5.378	1348	1349	1351	rVV	605	333	0.02%	0.002%
22	5.413	1354	1360	1366	rVB4	632	689	0.03%	0.005%
23	5.613	1410	1422	1461	rBV	553544	1146925	55.78%	7.551%
24	5.908	1503	1514	1538	rVB2	15031	35385	1.72%	0.233%
25	6.066	1545	1563	1591	rBV	471817	972146	47.28%	6.400%
26	6.285	1629	1631	1639	rVB5	546	649	0.03%	0.004%
27	6.330	1641	1645	1648	rBV3	616	434	0.02%	0.003%
28	6.346	1648	1650	1653	rVB2	569	321	0.02%	0.002%
29	6.452	1675	1683	1689	rVB3	516	684	0.03%	0.005%
30	6.632	1735	1739	1741	rBV2	383	316	0.02%	0.002%
31	6.664	1745	1749	1754	rVB4	421	408	0.02%	0.003%
32	6.699	1757	1760	1767	rVB3	488	426	0.02%	0.003%
33	6.738	1770	1772	1777	rVB	577	318	0.02%	0.002%
34	6.985	1837	1849	1887	rBV	213547	401996	19.55%	2.647%
35	7.172	1903	1907	1909	rBV4	413	299	0.01%	0.002%
36	7.211	1915	1919	1921	rBV5	496	344	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026959.D
 Acq On : 26 Jul 2022 18:22
 Operator : SY/MD
 Sample : N3841-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	7.313	1938	1951	1986	rBV	837251	1482272	72.08%	9.759%
38	7.619	2037	2046	2071	rBV	151182	274546	13.35%	1.808%
39	7.776	2094	2095	2099	rVB2	522	321	0.02%	0.002%
40	7.892	2128	2131	2135	rBV4	615	495	0.02%	0.003%
41	7.934	2138	2144	2147	rBV4	1210	1239	0.06%	0.008%
42	7.989	2159	2161	2163	rVB2	591	276	0.01%	0.002%
43	8.030	2171	2174	2175	rBV2	525	337	0.02%	0.002%
44	8.088	2182	2192	2233	rBV	508940	1020183	49.61%	6.717%
45	8.551	2333	2336	2341	rVB3	762	674	0.03%	0.004%
46	8.577	2341	2344	2349	rBV4	377	406	0.02%	0.003%
47	8.670	2369	2373	2378	rBV3	457	462	0.02%	0.003%
48	8.702	2378	2383	2387	rVB3	346	429	0.02%	0.003%
49	8.789	2405	2410	2415	rBV3	348	461	0.02%	0.003%
50	8.850	2416	2429	2452	rBV	887105	1445618	70.30%	9.518%
51	9.230	2543	2547	2553	rVB4	415	378	0.02%	0.002%
52	9.278	2560	2562	2568	rVB3	523	430	0.02%	0.003%
53	9.358	2582	2587	2590	rBV3	507	573	0.03%	0.004%
54	9.423	2603	2607	2611	rBV3	493	460	0.02%	0.003%
55	9.535	2636	2642	2646	rBV3	608	634	0.03%	0.004%
56	10.008	2784	2789	2792	rBV2	375	338	0.02%	0.002%
57	10.030	2793	2796	2803	rVB3	400	347	0.02%	0.002%
58	10.104	2815	2819	2831	rVB3	422	687	0.03%	0.005%
59	10.214	2841	2853	2876	rBV	734136	1145344	55.70%	7.541%
60	10.371	2899	2902	2903	rBV2	885	410	0.02%	0.003%
61	10.487	2935	2938	2943	rVB2	359	310	0.02%	0.002%
62	10.538	2950	2954	2957	rBV3	495	397	0.02%	0.003%
63	10.577	2961	2966	2969	rBV3	830	749	0.04%	0.005%
64	10.702	3000	3005	3008	rBV3	396	364	0.02%	0.002%
65	10.850	3049	3051	3055	rBV3	523	399	0.02%	0.003%
66	11.101	3126	3129	3136	rBV2	373	339	0.02%	0.002%
67	11.149	3136	3144	3150	rBV3	433	659	0.03%	0.004%
68	11.188	3154	3156	3159	rBV2	768	488	0.02%	0.003%
69	11.249	3163	3175	3199	rBV	781115	1223897	59.52%	8.058%
70	11.545	3258	3267	3271	rBV7	2463	3838	0.19%	0.025%
71	11.622	3280	3291	3314	rBV	849362	1331665	64.76%	8.767%
72	11.805	3345	3348	3351	rBV4	565	384	0.02%	0.003%
73	11.873	3366	3369	3374	rVB3	444	371	0.02%	0.002%
74	11.940	3386	3390	3392	rBV2	591	452	0.02%	0.003%
75	11.979	3396	3402	3406	rVB3	539	627	0.03%	0.004%
76	12.046	3419	3423	3426	rBV3	373	348	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026959.D
 Acq On : 26 Jul 2022 18:22
 Operator : SY/MD
 Sample : N3841-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.143	3451	3453	3458	rVB	577	366	0.02%	0.002%
78	12.172	3458	3462	3464	rBV	604	474	0.02%	0.003%
79	12.246	3480	3485	3486	rBV3	409	341	0.02%	0.002%
80	12.796	3653	3656	3660	rVB3	399	357	0.02%	0.002%
81	12.934	3697	3699	3702	rBV2	441	285	0.01%	0.002%
82	13.146	3762	3765	3768	rBV2	560	428	0.02%	0.003%
83	13.275	3801	3805	3809	rVB2	827	641	0.03%	0.004%
84	13.342	3823	3826	3832	rVB2	675	616	0.03%	0.004%
85	13.384	3837	3839	3844	rVB4	586	487	0.02%	0.003%
86	13.474	3864	3867	3871	rVB2	643	455	0.02%	0.003%
87	13.525	3881	3883	3886	rVV3	593	395	0.02%	0.003%
88	13.554	3889	3892	3896	rVV3	484	431	0.02%	0.003%
89	14.313	4124	4128	4133	rVB2	885	855	0.04%	0.006%
90	14.339	4133	4136	4140	rBV2	749	572	0.03%	0.004%
91	14.400	4150	4155	4161	rBV5	697	837	0.04%	0.006%
92	14.432	4161	4165	4167	rBV3	510	417	0.02%	0.003%
93	14.548	4198	4201	4203	rBV	564	354	0.02%	0.002%
94	14.590	4211	4214	4216	rBV4	599	395	0.02%	0.003%
95	14.619	4220	4223	4225	rBV	482	301	0.01%	0.002%
96	14.905	4309	4312	4316	rBV3	801	600	0.03%	0.004%
97	14.953	4324	4327	4329	rVB3	976	535	0.03%	0.004%
98	15.146	4384	4387	4389	rBV3	857	396	0.02%	0.003%
99	15.339	4445	4447	4453	rVB4	1356	821	0.04%	0.005%
100	15.422	4470	4473	4477	rBV3	802	707	0.03%	0.005%




Sum of corrected areas: 15188830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026959.D
Acq On : 26 Jul 2022 18:22
Operator : SY/MD
Sample : N3841-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

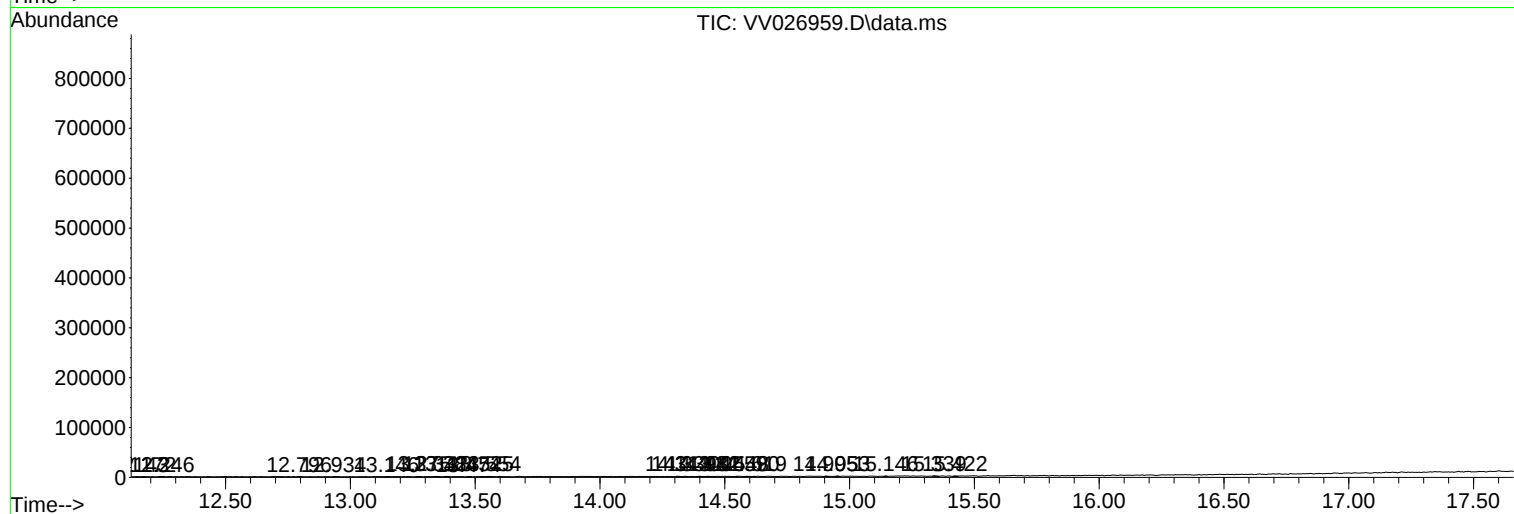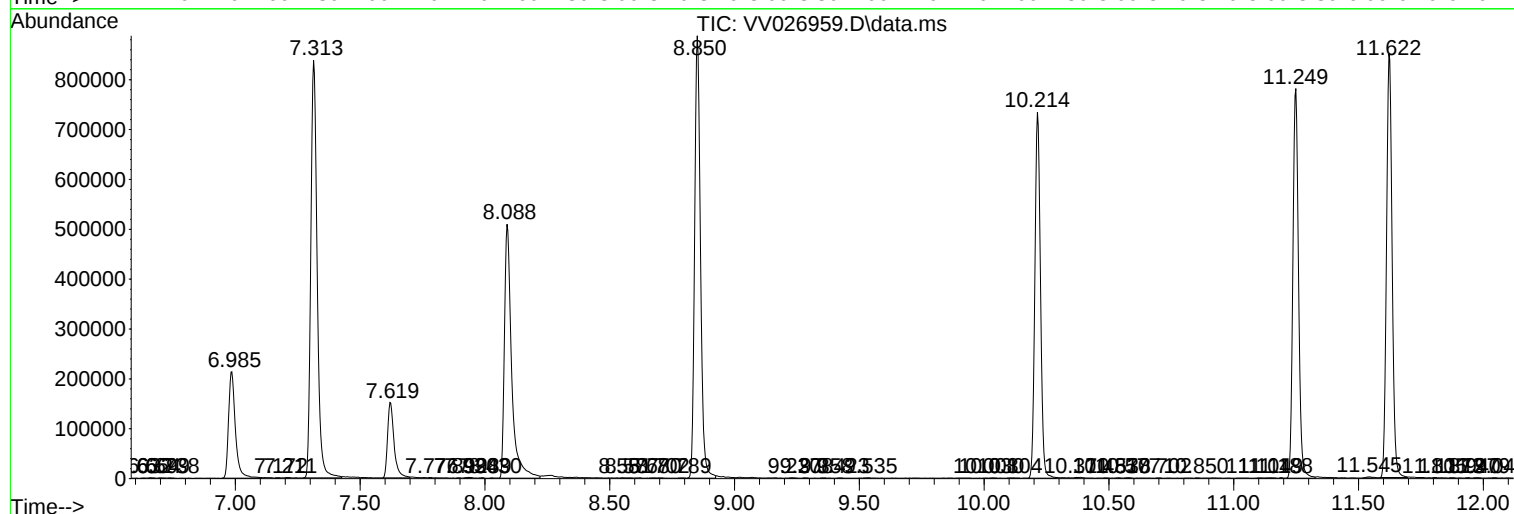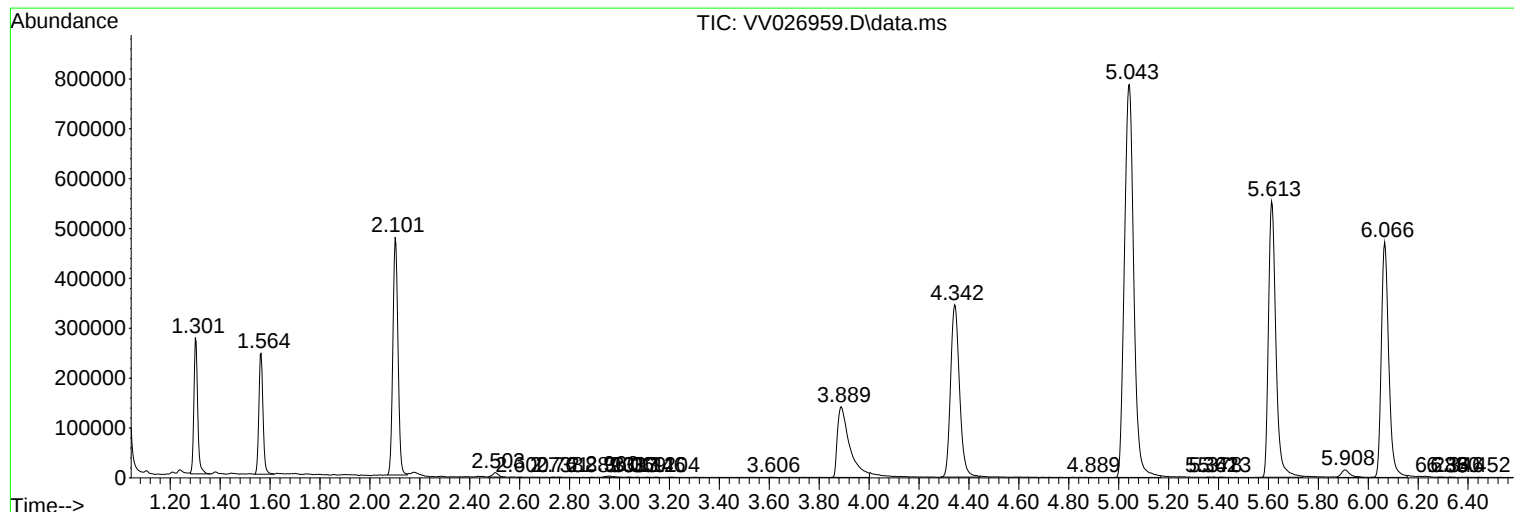

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026959.D
Acq On : 26 Jul 2022 18:22
Operator : SY/MD
Sample : N3841-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026959.D
Acq On : 26 Jul 2022 18:22
Operator : SY/MD
Sample : N3841-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc