

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026960.D
 Acq On : 26 Jul 2022 18:47
 Operator : SY/MD
 Sample : N3841-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026960.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	262825	280518	13.64%	1.859%
2	1.564	155	163	176	rBV	241001	276660	13.46%	1.833%
3	2.101	320	330	347	rBV	473301	674466	32.81%	4.470%
4	2.288	385	388	389	rBV2	699	372	0.02%	0.002%
5	2.323	396	399	400	rBV2	586	256	0.01%	0.002%
6	2.503	450	455	466	rVB5	3594	4997	0.24%	0.033%
7	2.564	471	474	476	rBV2	550	335	0.02%	0.002%
8	2.603	482	486	490	rVB3	317	274	0.01%	0.002%
9	2.760	531	535	538	rBV4	566	526	0.03%	0.003%
10	2.838	550	559	561	rBV2	371	428	0.02%	0.003%
11	2.950	588	594	595	rBV4	1114	940	0.05%	0.006%
12	2.992	604	607	611	rVB4	535	403	0.02%	0.003%
13	3.069	629	631	635	rVB3	502	231	0.01%	0.002%
14	3.127	643	649	653	rBV2	490	686	0.03%	0.005%
15	3.159	657	659	669	rVB2	255	237	0.01%	0.002%
16	3.204	671	673	677	rVB2	408	239	0.01%	0.002%
17	3.365	719	723	726	rBV2	366	270	0.01%	0.002%
18	3.397	730	733	736	rBV2	410	312	0.02%	0.002%
19	3.548	776	780	783	rVB2	377	290	0.01%	0.002%
20	3.632	802	806	812	rVB	319	243	0.01%	0.002%
21	3.664	812	816	822	rVB3	346	354	0.02%	0.002%
22	3.793	854	856	861	rVB2	454	315	0.02%	0.002%
23	3.821	861	865	868	rBV2	306	323	0.02%	0.002%
24	3.889	875	886	929	rBV	138156	484201	23.55%	3.209%
25	4.342	1010	1027	1052	rBV	347824	863235	41.99%	5.721%
26	4.577	1098	1100	1104	rBV3	316	258	0.01%	0.002%
27	4.738	1148	1150	1154	rBV2	303	266	0.01%	0.002%
28	4.776	1159	1162	1166	rVB4	311	275	0.01%	0.002%
29	5.043	1227	1245	1279	rBV2	796341	2055950	100.00%	13.625%
30	5.268	1313	1315	1321	rVB4	682	517	0.03%	0.003%
31	5.612	1410	1422	1456	rBV	543007	1133066	55.11%	7.509%
32	5.908	1503	1514	1528	rVV4	14331	30347	1.48%	0.201%
33	5.995	1538	1541	1544	rVB2	428	333	0.02%	0.002%
34	6.021	1546	1549	1550	rBV2	426	238	0.01%	0.002%
35	6.066	1550	1563	1589	rBV	466006	961183	46.75%	6.370%
36	6.304	1635	1637	1639	rBV	451	241	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026960.D
 Acq On : 26 Jul 2022 18:47
 Operator : SY/MD
 Sample : N3841-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.407	1661	1669	1673	rBV4	519	723	0.04%	0.005%
38	6.461	1682	1686	1689	rVB3	551	298	0.01%	0.002%
39	6.522	1699	1705	1707	rBV3	387	337	0.02%	0.002%
40	6.657	1740	1747	1749	rBV4	569	618	0.03%	0.004%
41	6.844	1801	1805	1808	rBV2	292	287	0.01%	0.002%
42	6.985	1837	1849	1880	rBV	210608	402887	19.60%	2.670%
43	7.210	1912	1919	1926	rBV6	1388	1859	0.09%	0.012%
44	7.313	1938	1951	1981	rBV	827787	1473164	71.65%	9.763%
45	7.619	2037	2046	2072	rVV	149376	271052	13.18%	1.796%
46	7.940	2137	2146	2147	rBV3	1401	1775	0.09%	0.012%
47	7.976	2155	2157	2159	rBV2	638	357	0.02%	0.002%
48	8.034	2172	2175	2178	rBV2	443	378	0.02%	0.003%
49	8.088	2182	2192	2236	rBV	513672	1011623	49.20%	6.704%
50	8.406	2288	2291	2294	rVB2	828	447	0.02%	0.003%
51	8.480	2311	2314	2322	rVB3	861	890	0.04%	0.006%
52	8.567	2339	2341	2345	rBV2	293	241	0.01%	0.002%
53	8.603	2349	2352	2356	rVB2	579	327	0.02%	0.002%
54	8.628	2356	2360	2362	rBV3	466	343	0.02%	0.002%
55	8.763	2399	2402	2405	rBV	381	293	0.01%	0.002%
56	8.850	2417	2429	2469	rBV	887324	1432776	69.69%	9.495%
57	9.014	2478	2480	2483	rBV2	731	413	0.02%	0.003%
58	9.152	2519	2523	2527	rBV4	1060	938	0.05%	0.006%
59	9.207	2538	2540	2542	rBV	534	257	0.01%	0.002%
60	9.432	2606	2610	2613	rBV	284	276	0.01%	0.002%
61	9.506	2630	2633	2635	rBV	416	290	0.01%	0.002%
62	9.551	2642	2647	2651	rBV3	454	390	0.02%	0.003%
63	9.667	2679	2683	2686	rBV2	319	331	0.02%	0.002%
64	9.763	2709	2713	2718	rVB3	370	413	0.02%	0.003%
65	9.789	2718	2721	2726	rVB	392	279	0.01%	0.002%
66	9.821	2726	2731	2736	rBV3	326	337	0.02%	0.002%
67	9.882	2745	2750	2752	rBV2	375	281	0.01%	0.002%
68	10.033	2792	2797	2800	rVV2	590	386	0.02%	0.003%
69	10.213	2840	2853	2879	rBV	733205	1152710	56.07%	7.639%
70	10.429	2917	2920	2923	rVB2	535	308	0.01%	0.002%
71	10.461	2927	2930	2935	rBV	319	320	0.02%	0.002%
72	10.670	2993	2995	3001	rBV2	400	370	0.02%	0.002%
73	10.783	3026	3030	3036	rBV2	293	316	0.02%	0.002%
74	10.853	3049	3052	3058	rVB5	1069	707	0.03%	0.005%
75	10.918	3069	3072	3074	rBV2	443	303	0.01%	0.002%
76	10.966	3085	3087	3091	rVB3	537	283	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026960.D
 Acq On : 26 Jul 2022 18:47
 Operator : SY/MD
 Sample : N3841-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.024	3099	3105	3107	rBV2	384	324	0.02%	0.002%
78	11.194	3150	3158	3163	rBV3	479	733	0.04%	0.005%
79	11.249	3163	3175	3202	rBV	778382	1202769	58.50%	7.971%
80	11.471	3242	3244	3252	rVB4	668	568	0.03%	0.004%
81	11.541	3257	3266	3278	rVB6	4607	9060	0.44%	0.060%
82	11.622	3279	3291	3320	rBV	835005	1334020	64.89%	8.841%
83	12.033	3416	3419	3421	rBV	406	225	0.01%	0.001%
84	12.168	3459	3461	3462	rVB	698	235	0.01%	0.002%
85	12.181	3462	3465	3469	rBV	478	375	0.02%	0.002%
86	12.381	3524	3527	3530	rBV3	557	415	0.02%	0.003%
87	12.654	3609	3612	3618	rBV2	621	438	0.02%	0.003%
88	12.709	3626	3629	3633	rBV	315	263	0.01%	0.002%
89	12.731	3633	3636	3641	rBV3	372	393	0.02%	0.003%
90	12.895	3683	3687	3690	rVB2	510	386	0.02%	0.003%
91	13.091	3743	3748	3750	rBV2	527	497	0.02%	0.003%
92	13.184	3773	3777	3778	rBV2	302	243	0.01%	0.002%
93	13.438	3852	3856	3859	rVB3	507	415	0.02%	0.003%
94	13.493	3870	3873	3877	rVB3	578	395	0.02%	0.003%
95	13.670	3925	3928	3930	rBV2	592	474	0.02%	0.003%
96	14.081	4053	4056	4059	rBV3	554	417	0.02%	0.003%
97	14.406	4155	4157	4160	rVB3	550	302	0.01%	0.002%
98	14.432	4160	4165	4166	rBV3	721	549	0.03%	0.004%
99	14.654	4230	4234	4237	rBV3	784	803	0.04%	0.005%
100	14.934	4319	4321	4325	rBV4	643	568	0.03%	0.004%




Sum of corrected areas: 15089235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026960.D
Acq On : 26 Jul 2022 18:47
Operator : SY/MD
Sample : N3841-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

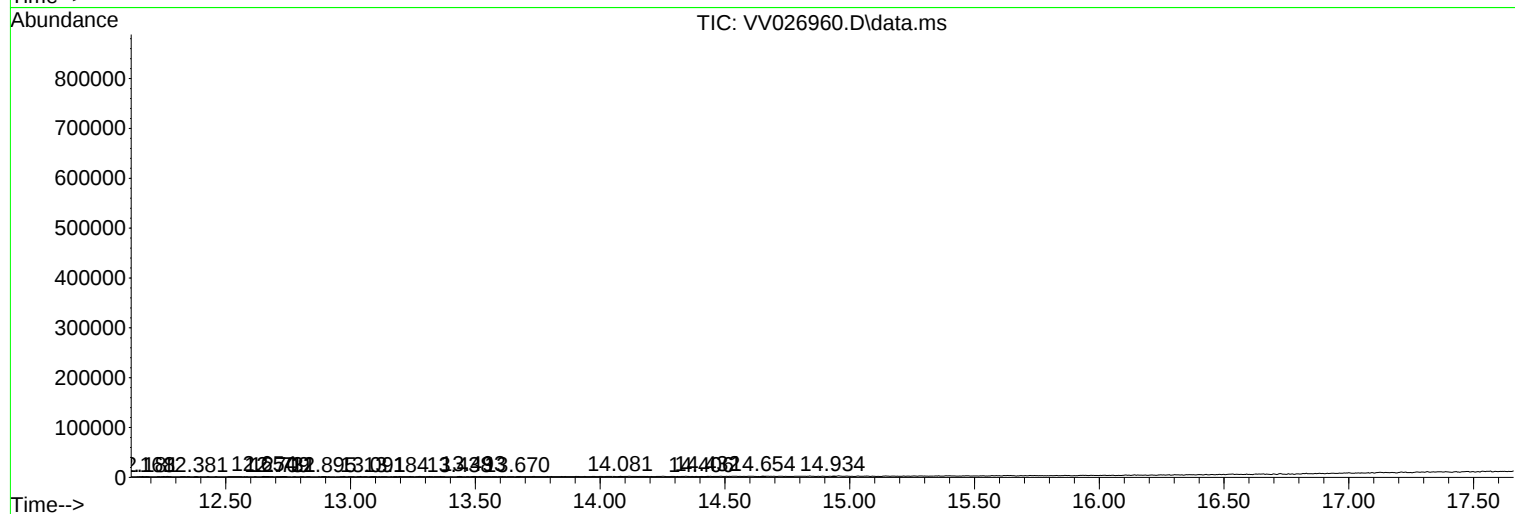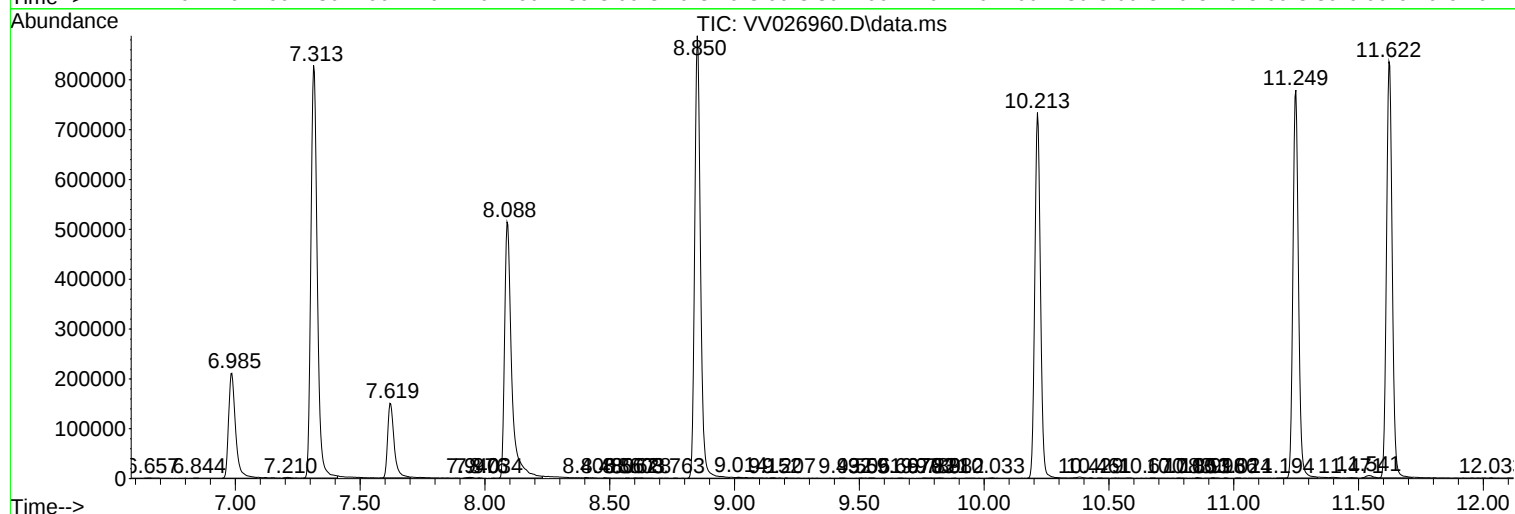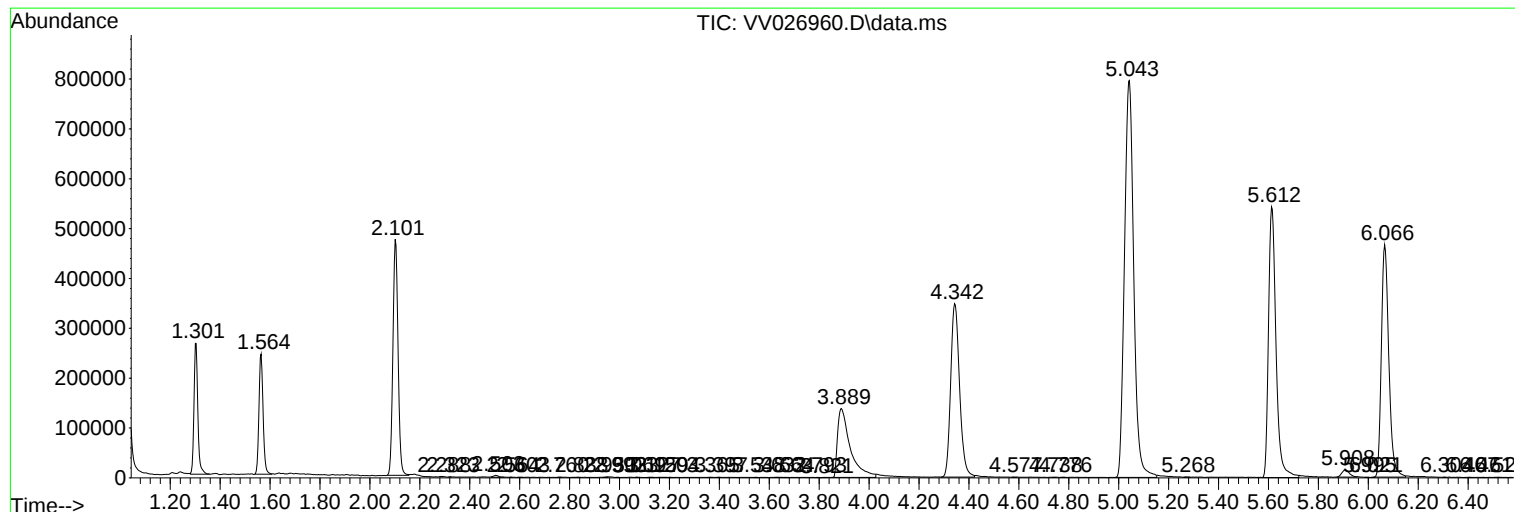

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026960.D
Acq On : 26 Jul 2022 18:47
Operator : SY/MD
Sample : N3841-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026960.D
Acq On : 26 Jul 2022 18:47
Operator : SY/MD
Sample : N3841-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------