

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V072622\
 Data File : VV026962.D
 Acq On : 26 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3843-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	96	rBV	267930	277027	13.23%	1.811%
2	1.561	155	162	178	rVB	233235	267393	12.77%	1.748%
3	2.101	320	330	347	rBV	477098	679776	32.46%	4.445%
4	2.275	380	384	386	rBV3	851	699	0.03%	0.005%
5	2.500	446	454	464	rVB4	4570	7082	0.34%	0.046%
6	2.564	471	474	484	rVB4	717	895	0.04%	0.006%
7	2.606	484	487	493	rBV2	322	403	0.02%	0.003%
8	2.744	526	530	533	rBV3	492	312	0.01%	0.002%
9	2.889	569	575	579	rBV2	344	495	0.02%	0.003%
10	3.137	648	652	656	rBV2	493	410	0.02%	0.003%
11	3.198	670	671	676	rVB2	754	300	0.01%	0.002%
12	3.304	700	704	708	rVB2	295	287	0.01%	0.002%
13	3.407	730	736	739	rBV3	324	340	0.02%	0.002%
14	3.706	825	829	833	rBV	434	346	0.02%	0.002%
15	3.886	874	885	946	rBV	153307	507815	24.25%	3.320%
16	4.233	991	993	999	rVB3	736	544	0.03%	0.004%
17	4.268	999	1004	1006	rBV2	554	453	0.02%	0.003%
18	4.342	1007	1027	1057	rBV	351326	878710	41.95%	5.745%
19	4.567	1093	1097	1103	rVB4	513	403	0.02%	0.003%
20	4.712	1140	1142	1147	rVB3	528	318	0.02%	0.002%
21	4.767	1154	1159	1164	rBV3	418	393	0.02%	0.003%
22	4.812	1170	1173	1174	rBV2	675	368	0.02%	0.002%
23	4.822	1174	1176	1177	rVV2	681	278	0.01%	0.002%
24	4.831	1177	1179	1182	rVB2	423	271	0.01%	0.002%
25	4.899	1195	1200	1203	rVB3	567	468	0.02%	0.003%
26	5.043	1227	1245	1295	rBV2	805486	2094461	100.00%	13.694%
27	5.285	1315	1320	1326	rVB5	796	774	0.04%	0.005%
28	5.436	1363	1367	1369	rBV3	401	271	0.01%	0.002%
29	5.503	1384	1388	1390	rBV2	419	383	0.02%	0.003%
30	5.542	1394	1400	1402	rBV3	389	301	0.01%	0.002%
31	5.612	1405	1422	1466	rBV	547008	1138674	54.37%	7.445%
32	5.908	1503	1514	1528	rBV4	14453	32312	1.54%	0.211%
33	6.005	1540	1544	1549	rVB3	461	451	0.02%	0.003%
34	6.066	1549	1563	1591	rBV	482881	987665	47.16%	6.458%
35	6.378	1656	1660	1664	rVB3	610	443	0.02%	0.003%
36	6.561	1713	1717	1720	rBV2	498	414	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026962.D
 Acq On : 26 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3843-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.686	1753	1756	1760	rBV2	356	309	0.01%	0.002%
38	6.706	1760	1762	1766	rVB4	544	386	0.02%	0.003%
39	6.985	1835	1849	1875	rBV	216935	403331	19.26%	2.637%
40	7.313	1938	1951	1982	rBV	854468	1500648	71.65%	9.812%
41	7.619	2036	2046	2076	rBV	153187	278203	13.28%	1.819%
42	7.847	2115	2117	2118	rVV2	718	279	0.01%	0.002%
43	7.860	2118	2121	2123	rVB3	673	399	0.02%	0.003%
44	7.882	2123	2128	2132	rBV4	515	461	0.02%	0.003%
45	7.940	2139	2146	2151	rBV6	1702	2237	0.11%	0.015%
46	7.979	2153	2158	2170	rVB5	1690	2758	0.13%	0.018%
47	8.088	2178	2192	2236	rBV	525351	1042923	49.79%	6.819%
48	8.471	2308	2311	2313	rBV3	622	388	0.02%	0.003%
49	8.551	2331	2336	2339	rBV5	600	583	0.03%	0.004%
50	8.619	2349	2357	2361	rVB6	698	803	0.04%	0.005%
51	8.648	2361	2366	2368	rBV3	430	377	0.02%	0.002%
52	8.715	2385	2387	2393	rVB2	370	350	0.02%	0.002%
53	8.760	2395	2401	2403	rBV2	398	378	0.02%	0.002%
54	8.850	2416	2429	2450	rBV	881648	1422139	67.90%	9.299%
55	9.082	2497	2501	2505	rVB6	640	515	0.02%	0.003%
56	9.156	2522	2524	2532	rVB5	974	802	0.04%	0.005%
57	9.243	2549	2551	2554	rVV	711	472	0.02%	0.003%
58	9.262	2555	2557	2564	rVB3	553	401	0.02%	0.003%
59	9.542	2639	2644	2648	rBV4	457	486	0.02%	0.003%
60	9.644	2670	2676	2679	rBV3	400	384	0.02%	0.003%
61	9.837	2733	2736	2739	rVV2	606	406	0.02%	0.003%
62	10.053	2800	2803	2810	rBV3	333	433	0.02%	0.003%
63	10.214	2841	2853	2878	rBV	754761	1181423	56.41%	7.725%
64	10.381	2901	2905	2914	rVB7	1863	2440	0.12%	0.016%
65	10.474	2930	2934	2938	rBV2	378	335	0.02%	0.002%
66	10.706	3004	3006	3010	rVV2	397	266	0.01%	0.002%
67	10.747	3013	3019	3024	rVB3	387	449	0.02%	0.003%
68	10.821	3039	3042	3048	rVB3	281	296	0.01%	0.002%
69	10.853	3048	3052	3056	rBV2	635	441	0.02%	0.003%
70	10.931	3068	3076	3080	rBV4	847	1065	0.05%	0.007%
71	10.972	3084	3089	3092	rVB2	482	421	0.02%	0.003%
72	11.027	3102	3106	3108	rBV2	420	289	0.01%	0.002%
73	11.181	3152	3154	3157	rBV3	485	383	0.02%	0.003%
74	11.197	3157	3159	3163	rVB2	601	302	0.01%	0.002%
75	11.246	3163	3174	3199	rBV	755780	1200985	57.34%	7.853%
76	11.439	3231	3234	3237	rBV3	302	270	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026962.D
 Acq On : 26 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3843-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.542	3256	3266	3272	rBV7	2327	3646	0.17%	0.024%
78	11.622	3278	3291	3317	rBV	847187	1347761	64.35%	8.812%
79	11.747	3327	3330	3335	rBV4	528	467	0.02%	0.003%
80	11.921	3381	3384	3391	rBV3	848	714	0.03%	0.005%
81	12.011	3409	3412	3416	rBV3	299	286	0.01%	0.002%
82	12.091	3434	3437	3439	rBV3	443	271	0.01%	0.002%
83	12.149	3452	3455	3459	rBV	389	384	0.02%	0.003%
84	12.651	3608	3611	3616	rBV4	592	560	0.03%	0.004%
85	12.702	3622	3627	3630	rBV3	388	365	0.02%	0.002%
86	12.795	3653	3656	3663	rVB4	458	577	0.03%	0.004%
87	12.844	3663	3671	3673	rBV3	501	628	0.03%	0.004%
88	13.101	3744	3751	3753	rBV2	519	572	0.03%	0.004%
89	13.271	3801	3804	3805	rBV	643	360	0.02%	0.002%
90	13.406	3844	3846	3850	rVB3	541	320	0.02%	0.002%
91	13.551	3889	3891	3895	rBV	422	313	0.01%	0.002%
92	13.863	3979	3988	3991	rBV4	545	854	0.04%	0.006%
93	13.969	4017	4021	4023	rBV2	618	477	0.02%	0.003%
94	14.011	4031	4034	4036	rBV2	460	274	0.01%	0.002%
95	14.201	4091	4093	4097	rBV3	316	316	0.02%	0.002%
96	14.509	4186	4189	4192	rBV3	510	318	0.02%	0.002%
97	14.548	4196	4201	4205	rBV3	830	790	0.04%	0.005%
98	14.824	4284	4287	4291	rBV3	756	691	0.03%	0.005%
99	15.426	4472	4474	4481	rBV5	715	811	0.04%	0.005%
100	15.545	4510	4511	4517	rVB3	735	294	0.01%	0.002%




Sum of corrected areas: 15294200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026962.D
Acq On : 26 Jul 2022 19:36
Operator : SY/MD
Sample : N3843-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

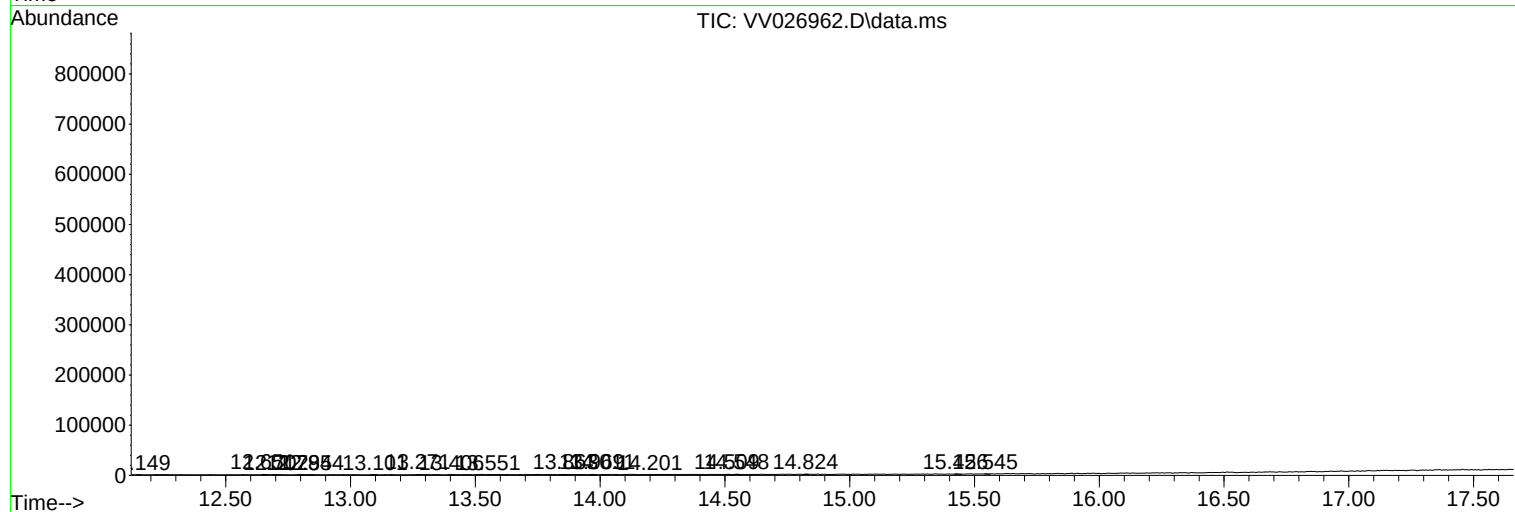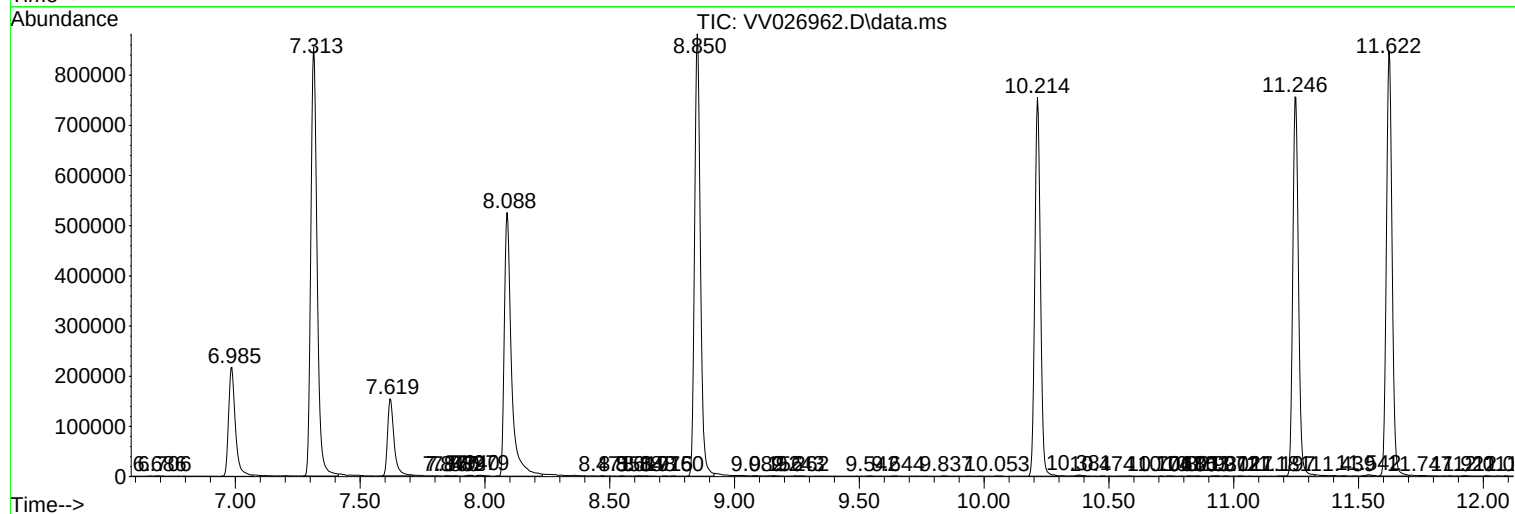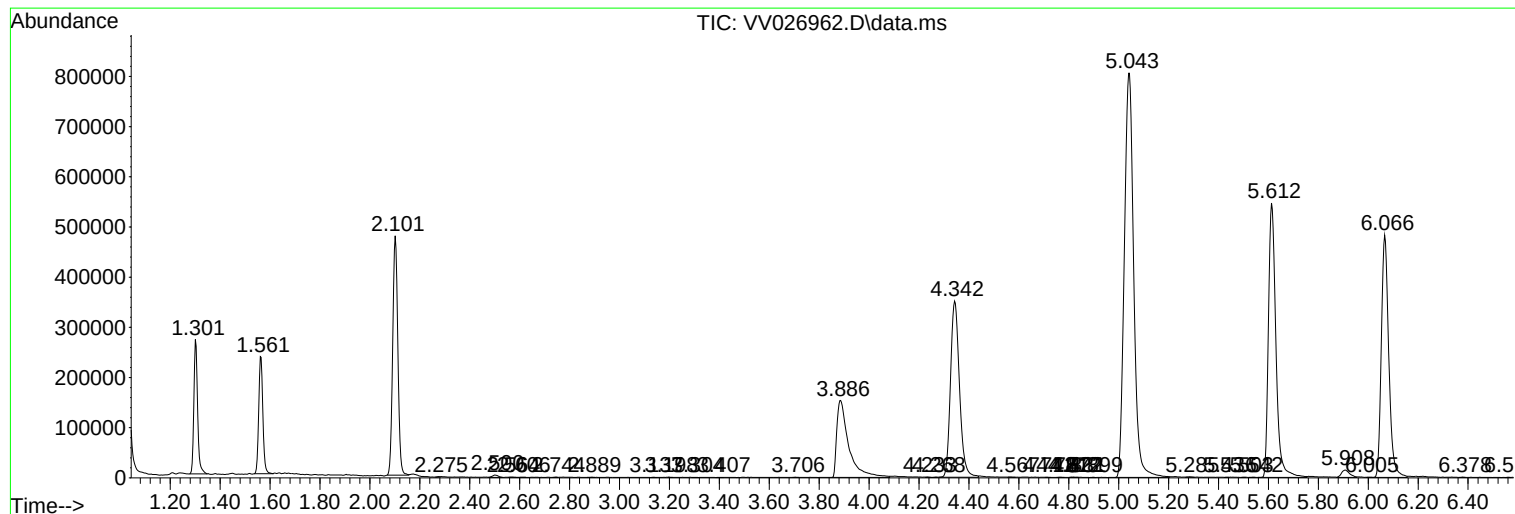

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026962.D
Acq On : 26 Jul 2022 19:36
Operator : SY/MD
Sample : N3843-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026962.D
Acq On : 26 Jul 2022 19:36
Operator : SY/MD
Sample : N3843-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc