

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026965.D
 Acq On : 26 Jul 2022 20:50
 Operator : SY/MD
 Sample : N3843-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	32	rVB3	12075	12328	0.62%	0.085%
2	1.201	45	50	57	rBV4	9325	11561	0.58%	0.080%
3	1.304	74	82	96	rVB	250098	269703	13.53%	1.863%
4	1.564	155	163	173	rBV	225911	259287	13.01%	1.791%
5	2.101	320	330	344	rBV	444430	634972	31.86%	4.386%
6	2.285	383	387	395	rVB2	2378	3038	0.15%	0.021%
7	2.507	448	456	466	rVB3	7407	12528	0.63%	0.087%
8	2.690	509	513	517	rBV4	561	516	0.03%	0.004%
9	2.712	517	520	523	rVB2	442	346	0.02%	0.002%
10	2.918	579	584	589	rBV2	398	360	0.02%	0.002%
11	2.950	589	594	598	rBV4	1050	1396	0.07%	0.010%
12	3.050	623	625	631	rVB3	436	366	0.02%	0.003%
13	3.166	653	661	663	rBV4	851	899	0.05%	0.006%
14	3.269	684	693	695	rBV2	424	578	0.03%	0.004%
15	3.590	789	793	799	rBV2	258	324	0.02%	0.002%
16	3.886	871	885	930	rBV	147269	485564	24.36%	3.354%
17	4.117	955	957	962	rVB3	741	552	0.03%	0.004%
18	4.342	1010	1027	1057	rBV	341409	850754	42.68%	5.876%
19	4.568	1093	1097	1098	rBV2	414	318	0.02%	0.002%
20	4.732	1143	1148	1151	rVB3	516	405	0.02%	0.003%
21	4.815	1169	1174	1176	rBV2	915	910	0.05%	0.006%
22	5.040	1227	1244	1285	rBV2	758713	1993208	100.00%	13.767%
23	5.236	1303	1305	1314	rVB3	1612	1188	0.06%	0.008%
24	5.275	1314	1317	1319	rBV4	655	335	0.02%	0.002%
25	5.358	1340	1343	1348	rBV2	458	357	0.02%	0.002%
26	5.413	1357	1360	1364	rVB5	509	435	0.02%	0.003%
27	5.477	1375	1380	1383	rBV3	532	585	0.03%	0.004%
28	5.539	1395	1399	1401	rBV3	532	343	0.02%	0.002%
29	5.613	1410	1422	1460	rBV	511027	1057407	53.05%	7.304%
30	5.908	1503	1514	1531	rBV4	11393	25941	1.30%	0.179%
31	5.989	1536	1539	1540	rBV2	535	316	0.02%	0.002%
32	6.066	1548	1563	1599	rBV	458050	948781	47.60%	6.553%
33	6.268	1624	1626	1630	rVB3	674	462	0.02%	0.003%
34	6.307	1636	1638	1642	rVB3	499	298	0.01%	0.002%
35	6.358	1650	1654	1657	rBV3	473	462	0.02%	0.003%
36	6.416	1670	1672	1676	rBV3	467	348	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026965.D
 Acq On : 26 Jul 2022 20:50
 Operator : SY/MD
 Sample : N3843-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.474	1688	1690	1694	rVB2	480	294	0.01%	0.002%
38	6.510	1694	1701	1702	rBV2	1001	845	0.04%	0.006%
39	6.648	1739	1744	1745	rBV2	708	599	0.03%	0.004%
40	6.883	1812	1817	1821	rBV2	336	318	0.02%	0.002%
41	6.985	1838	1849	1874	rBV	200295	379584	19.04%	2.622%
42	7.204	1912	1917	1921	rBV4	515	606	0.03%	0.004%
43	7.265	1934	1936	1939	rVB3	584	329	0.02%	0.002%
44	7.313	1939	1951	1973	rBV	780844	1373502	68.91%	9.487%
45	7.622	2036	2047	2071	rBV2	145176	264631	13.28%	1.828%
46	7.934	2136	2144	2146	rBV4	2569	2781	0.14%	0.019%
47	7.976	2150	2157	2170	rVB8	4659	9253	0.46%	0.064%
48	8.088	2182	2192	2230	rBV	502955	996758	50.01%	6.885%
49	8.436	2296	2300	2306	rVB5	555	576	0.03%	0.004%
50	8.612	2348	2355	2360	rBV4	809	1076	0.05%	0.007%
51	8.690	2376	2379	2383	rVB4	490	358	0.02%	0.002%
52	8.783	2404	2408	2413	rVB3	537	543	0.03%	0.004%
53	8.812	2413	2417	2418	rBV	585	385	0.02%	0.003%
54	8.850	2418	2429	2458	rBV	811431	1338192	67.14%	9.243%
55	9.059	2492	2494	2496	rBV2	529	314	0.02%	0.002%
56	9.104	2505	2508	2513	rVB3	779	685	0.03%	0.005%
57	9.188	2531	2534	2541	rBV2	795	861	0.04%	0.006%
58	9.387	2590	2596	2601	rVB2	380	310	0.02%	0.002%
59	9.413	2601	2604	2609	rVB2	521	445	0.02%	0.003%
60	9.442	2609	2613	2617	rBV2	386	368	0.02%	0.003%
61	9.526	2634	2639	2641	rBV2	479	393	0.02%	0.003%
62	9.696	2688	2692	2699	rVB3	324	376	0.02%	0.003%
63	9.738	2702	2705	2707	rVV	422	303	0.02%	0.002%
64	9.860	2740	2743	2747	rBV2	353	330	0.02%	0.002%
65	9.985	2776	2782	2787	rBV2	493	575	0.03%	0.004%
66	10.011	2787	2790	2794	rVV2	350	316	0.02%	0.002%
67	10.214	2840	2853	2880	rBV	722407	1138682	57.13%	7.865%
68	10.381	2896	2905	2915	rBV4	2975	4475	0.22%	0.031%
69	10.506	2941	2944	2947	rBV2	436	312	0.02%	0.002%
70	10.535	2950	2953	2955	rVV2	468	353	0.02%	0.002%
71	10.548	2955	2957	2963	rVV2	493	390	0.02%	0.003%
72	10.670	2992	2995	3000	rVB	8496	4640	0.23%	0.032%
73	10.747	3016	3019	3027	rVB2	416	377	0.02%	0.003%
74	10.911	3066	3070	3072	rBV	431	310	0.02%	0.002%
75	10.924	3072	3074	3081	rVV	913	791	0.04%	0.005%
76	10.976	3082	3090	3093	rVV3	377	553	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026965.D
 Acq On : 26 Jul 2022 20:50
 Operator : SY/MD
 Sample : N3843-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.008	3093	3100	3104	rVB2	541	442	0.02%	0.003%
78	11.120	3131	3135	3138	rBV2	306	298	0.01%	0.002%
79	11.249	3163	3175	3193	rBV	709288	1105756	55.48%	7.637%
80	11.458	3236	3240	3242	rBV2	619	389	0.02%	0.003%
81	11.538	3257	3265	3266	rBV3	2981	2731	0.14%	0.019%
82	11.622	3279	3291	3309	rBV	802082	1256586	63.04%	8.679%
83	12.011	3410	3412	3418	rVB2	439	319	0.02%	0.002%
84	12.181	3461	3465	3466	rBV2	676	453	0.02%	0.003%
85	12.403	3529	3534	3535	rBV2	421	378	0.02%	0.003%
86	12.445	3540	3547	3550	rVV3	478	577	0.03%	0.004%
87	12.648	3604	3610	3611	rBV2	546	518	0.03%	0.004%
88	12.799	3653	3657	3660	rVB2	471	341	0.02%	0.002%
89	12.914	3690	3693	3695	rBV2	466	300	0.02%	0.002%
90	12.966	3704	3709	3712	rBV3	466	538	0.03%	0.004%
91	13.104	3747	3752	3757	rBV3	481	660	0.03%	0.005%
92	13.194	3776	3780	3782	rBV2	514	401	0.02%	0.003%
93	13.471	3864	3866	3871	rVB3	633	400	0.02%	0.003%
94	13.545	3886	3889	3892	rVB	569	306	0.02%	0.002%
95	13.590	3899	3903	3905	rBV3	391	309	0.02%	0.002%
96	13.631	3911	3916	3919	rVB3	686	597	0.03%	0.004%
97	13.988	4024	4027	4029	rBV2	558	354	0.02%	0.002%
98	14.297	4120	4123	4128	rBV2	576	556	0.03%	0.004%
99	14.426	4159	4163	4164	rBV3	577	360	0.02%	0.002%
100	14.805	4278	4281	4285	rVB2	682	504	0.03%	0.003%




Sum of corrected areas: 14478033

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026965.D
Acq On : 26 Jul 2022 20:50
Operator : SY/MD
Sample : N3843-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

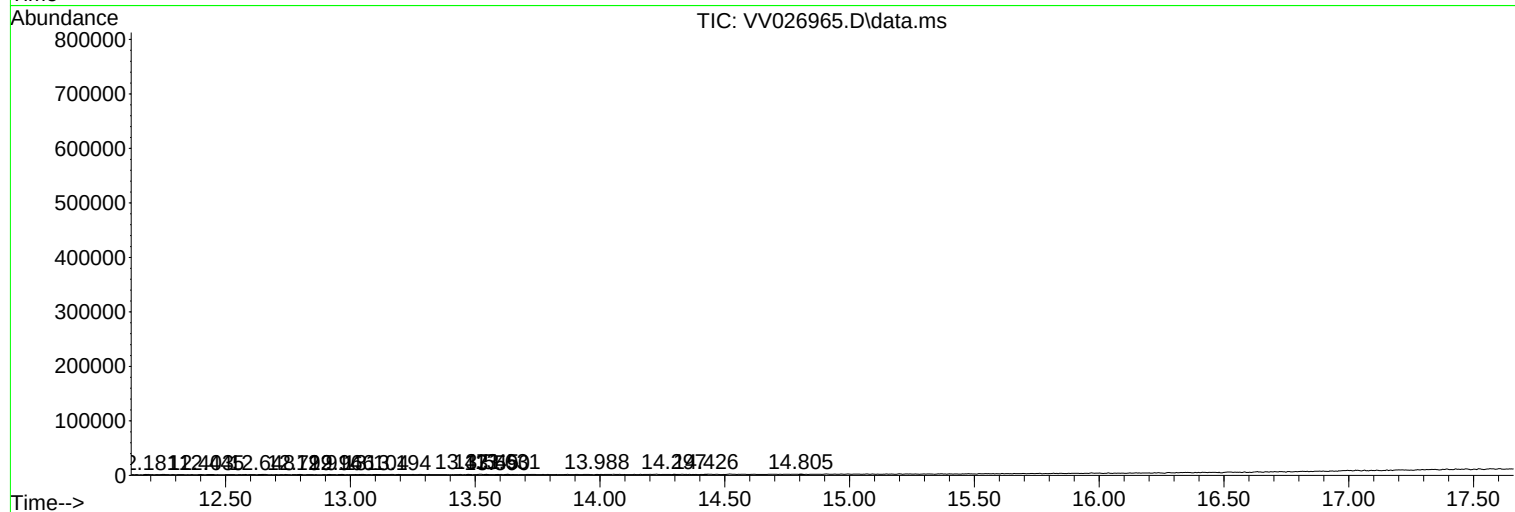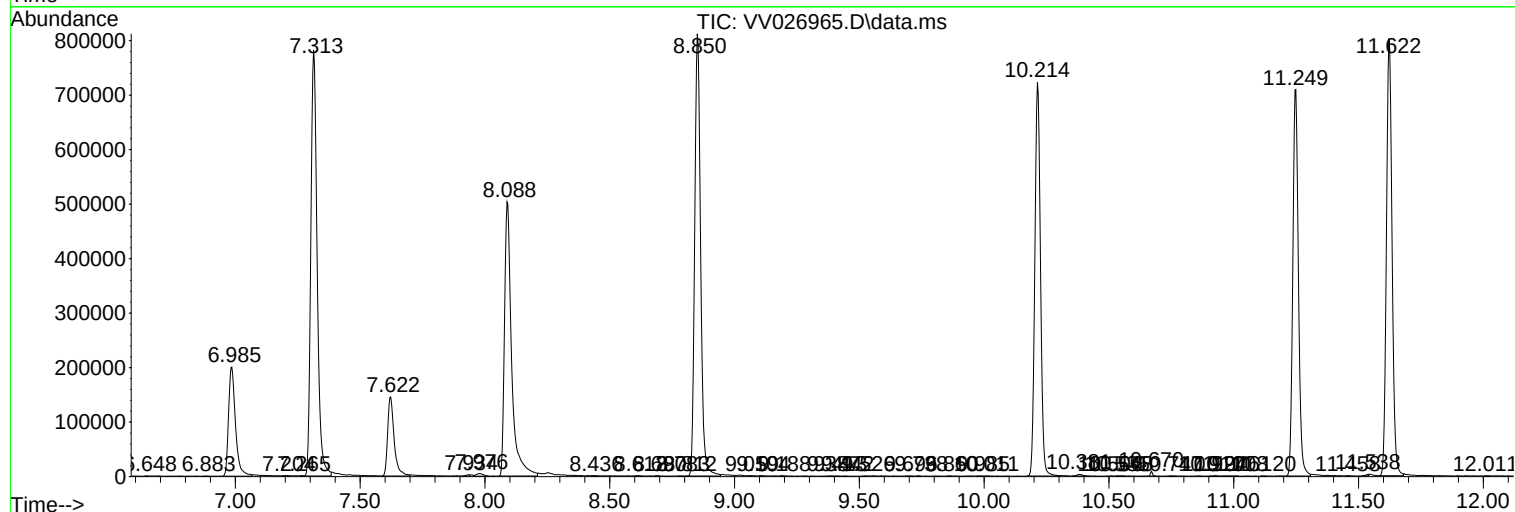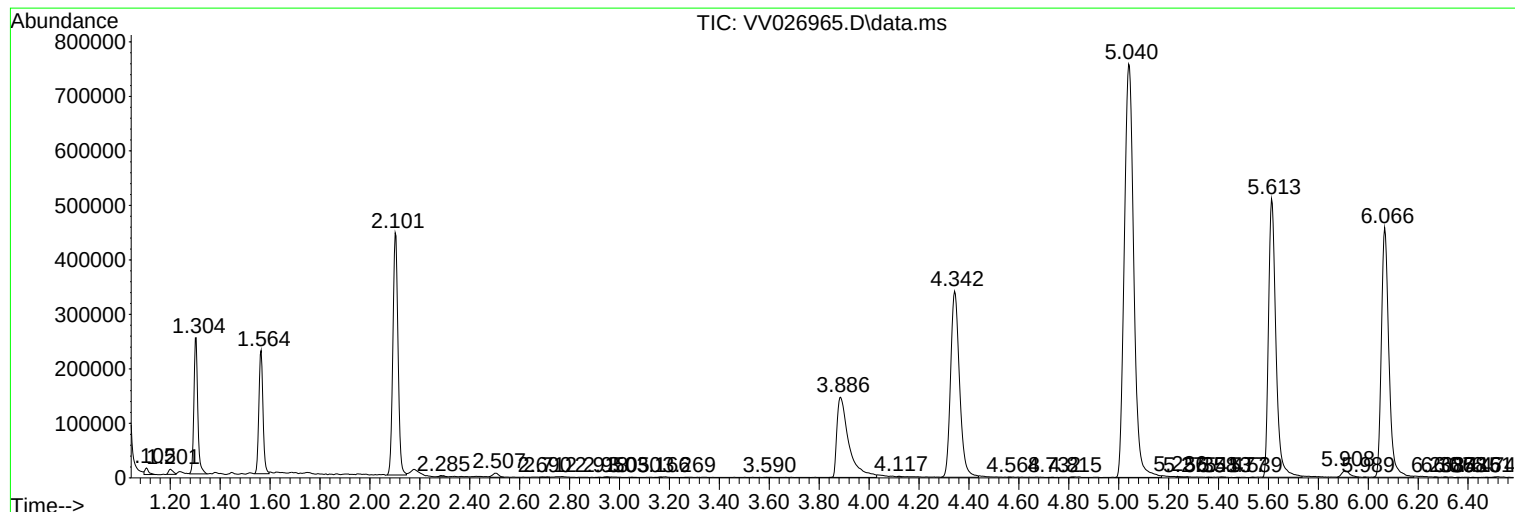

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026965.D
Acq On : 26 Jul 2022 20:50
Operator : SY/MD
Sample : N3843-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026965.D
Acq On : 26 Jul 2022 20:50
Operator : SY/MD
Sample : N3843-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc