

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	35	rVB	82232	80019	1.94%	0.418%
2	1.211	49	53	58	rBV3	10008	8311	0.20%	0.043%
3	1.301	73	81	95	rBV	289128	317949	7.72%	1.660%
4	1.561	154	162	175	rBV	230181	268919	6.53%	1.404%
5	1.761	219	224	230	rVB	14085	15004	0.36%	0.078%
6	1.799	231	236	252	rVB3	12715	19260	0.47%	0.101%
7	2.101	320	330	341	rBV	458525	649693	15.78%	3.392%
8	2.175	342	353	384	rVB	364442	894416	21.73%	4.669%
9	2.954	584	595	603	rBV7	4079	8999	0.22%	0.047%
10	3.002	608	610	614	rBV2	347	298	0.01%	0.002%
11	3.031	614	619	621	rBV4	1406	1389	0.03%	0.007%
12	3.137	648	652	654	rBV3	570	411	0.01%	0.002%
13	3.166	659	661	664	rVV2	539	400	0.01%	0.002%
14	3.198	664	671	673	rVV3	954	980	0.02%	0.005%
15	3.211	673	675	678	rVV2	872	629	0.02%	0.003%
16	3.230	678	681	685	rVV3	774	706	0.02%	0.004%
17	3.278	692	696	699	rVV2	405	338	0.01%	0.002%
18	3.452	745	750	752	rBV4	512	438	0.01%	0.002%
19	3.600	791	796	803	rVB2	492	487	0.01%	0.003%
20	3.883	873	884	910	rBV	145330	455846	11.07%	2.380%
21	4.333	1008	1024	1081	rBV2	1479697	4116260	100.00%	21.488%
22	4.867	1188	1190	1194	rVB3	581	348	0.01%	0.002%
23	4.899	1194	1200	1201	rBV3	987	969	0.02%	0.005%
24	5.040	1228	1244	1273	rBV2	798281	2049730	49.80%	10.700%
25	5.320	1324	1331	1334	rBV4	591	669	0.02%	0.003%
26	5.343	1336	1338	1341	rVB3	657	312	0.01%	0.002%
27	5.375	1344	1348	1351	rBV4	693	698	0.02%	0.004%
28	5.481	1375	1381	1383	rBV3	918	824	0.02%	0.004%
29	5.529	1394	1396	1399	rVB2	690	385	0.01%	0.002%
30	5.564	1404	1407	1409	rBV2	656	467	0.01%	0.002%
31	5.613	1409	1422	1461	rBV	540204	1122826	27.28%	5.862%
32	5.844	1492	1494	1499	rVB3	1104	819	0.02%	0.004%
33	5.908	1503	1514	1536	rVB3	12138	28152	0.68%	0.147%
34	5.986	1536	1538	1544	rVB5	523	441	0.01%	0.002%
35	6.066	1549	1563	1595	rBV	461095	946845	23.00%	4.943%
36	6.195	1600	1603	1604	rBV2	652	321	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.330	1640	1645	1647	rBV3	423	306	0.01%	0.002%
38	6.346	1647	1650	1654	rVV3	542	364	0.01%	0.002%
39	6.368	1654	1657	1660	rVB3	1174	617	0.01%	0.003%
40	6.513	1697	1702	1707	rBV4	556	636	0.02%	0.003%
41	6.918	1826	1828	1834	rVB2	565	393	0.01%	0.002%
42	6.986	1834	1849	1874	rBV	201929	388025	9.43%	2.026%
43	7.201	1911	1916	1917	rBV3	482	461	0.01%	0.002%
44	7.233	1922	1926	1928	rBV4	735	572	0.01%	0.003%
45	7.314	1939	1951	1975	rBV	811929	1440390	34.99%	7.519%
46	7.619	2035	2046	2068	rBV	147810	264664	6.43%	1.382%
47	7.847	2113	2117	2119	rBV2	713	537	0.01%	0.003%
48	7.860	2119	2121	2125	rVB4	668	401	0.01%	0.002%
49	7.937	2137	2145	2152	rBV4	2831	4436	0.11%	0.023%
50	7.976	2154	2157	2158	rBV3	1059	661	0.02%	0.003%
51	8.088	2181	2192	2236	rBV	507191	1000505	24.31%	5.223%
52	8.384	2283	2284	2287	rVB3	716	311	0.01%	0.002%
53	8.481	2310	2314	2317	rBV4	676	536	0.01%	0.003%
54	8.596	2346	2350	2352	rBV3	641	424	0.01%	0.002%
55	8.850	2417	2429	2450	rBV	838763	1376769	33.45%	7.187%
56	9.069	2495	2497	2503	rVB4	844	586	0.01%	0.003%
57	9.101	2504	2507	2512	rVB4	573	492	0.01%	0.003%
58	9.146	2512	2521	2525	rBV5	1062	1601	0.04%	0.008%
59	9.217	2539	2543	2545	rVB	502	363	0.01%	0.002%
60	9.239	2545	2550	2551	rBV	429	324	0.01%	0.002%
61	9.301	2567	2569	2574	rVB2	460	327	0.01%	0.002%
62	9.326	2574	2577	2580	rBV2	570	433	0.01%	0.002%
63	9.413	2601	2604	2608	rBV2	404	297	0.01%	0.002%
64	9.477	2617	2624	2628	rBV2	407	512	0.01%	0.003%
65	9.526	2636	2639	2643	rBV3	428	359	0.01%	0.002%
66	9.548	2643	2646	2648	rBV3	692	467	0.01%	0.002%
67	9.815	2720	2729	2730	rBV3	5119	5861	0.14%	0.031%
68	10.024	2785	2794	2805	rBV5	7130	12714	0.31%	0.066%
69	10.214	2838	2853	2878	rBV	732488	1146333	27.85%	5.984%
70	10.384	2900	2906	2913	rVB5	2902	4148	0.10%	0.022%
71	10.754	3017	3021	3025	rBV3	323	301	0.01%	0.002%
72	10.815	3037	3040	3045	rVB2	573	462	0.01%	0.002%
73	10.847	3045	3050	3052	rBV2	822	813	0.02%	0.004%
74	10.915	3067	3071	3072	rBV	764	496	0.01%	0.003%
75	10.982	3085	3092	3096	rBV2	400	426	0.01%	0.002%
76	11.043	3105	3111	3115	rVV3	457	587	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026966.D
 Acq On : 26 Jul 2022 21:14
 Operator : SY/MD
 Sample : N3843-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.111	3127	3132	3138	rBV	412	587	0.01%	0.003%
78	11.249	3163	3175	3203	rBV	750737	1171638	28.46%	6.116%
79	11.423	3227	3229	3234	rVB	763	506	0.01%	0.003%
80	11.445	3234	3236	3241	rBV3	487	394	0.01%	0.002%
81	11.535	3257	3264	3265	rBV4	3121	2678	0.07%	0.014%
82	11.622	3279	3291	3314	rBV	844160	1318229	32.02%	6.882%
83	11.889	3372	3374	3378	rVB2	469	309	0.01%	0.002%
84	11.976	3398	3401	3406	rBV3	382	323	0.01%	0.002%
85	12.506	3562	3566	3568	rBV	426	310	0.01%	0.002%
86	12.628	3600	3604	3607	rBV3	425	319	0.01%	0.002%
87	12.651	3607	3611	3615	rBV3	544	423	0.01%	0.002%
88	12.712	3628	3630	3634	rBV	479	390	0.01%	0.002%
89	12.805	3655	3659	3662	rVB4	484	362	0.01%	0.002%
90	12.940	3698	3701	3704	rBV2	491	347	0.01%	0.002%
91	12.992	3713	3717	3724	rVB2	362	422	0.01%	0.002%
92	13.040	3724	3732	3733	rBV	570	724	0.02%	0.004%
93	13.201	3780	3782	3787	rVB3	591	456	0.01%	0.002%
94	13.519	3877	3881	3887	rVB4	1027	1181	0.03%	0.006%
95	13.783	3960	3963	3967	rBV	665	444	0.01%	0.002%
96	13.879	3989	3993	3995	rBV4	508	413	0.01%	0.002%
97	14.101	4060	4062	4066	rBV2	397	341	0.01%	0.002%
98	14.304	4121	4125	4128	rBV3	584	539	0.01%	0.003%
99	14.757	4264	4266	4271	rBV4	584	460	0.01%	0.002%
100	14.889	4303	4307	4309	rBV2	560	456	0.01%	0.002%




Sum of corrected areas: 19155719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026966.D
Acq On : 26 Jul 2022 21:14
Operator : SY/MD
Sample : N3843-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

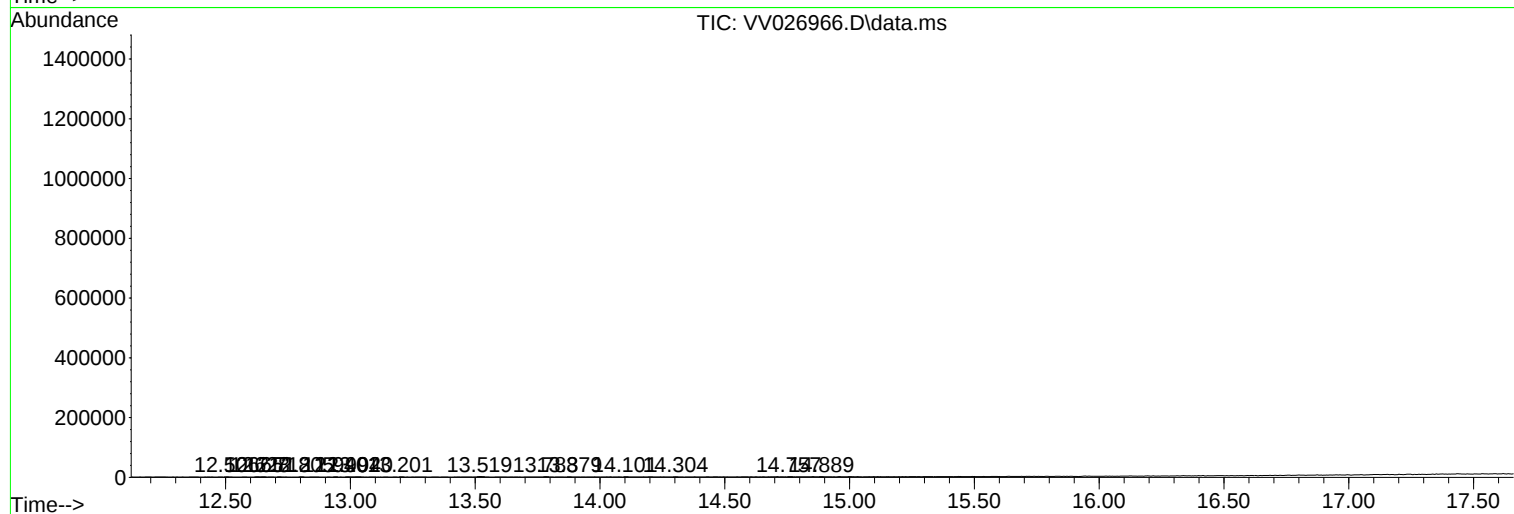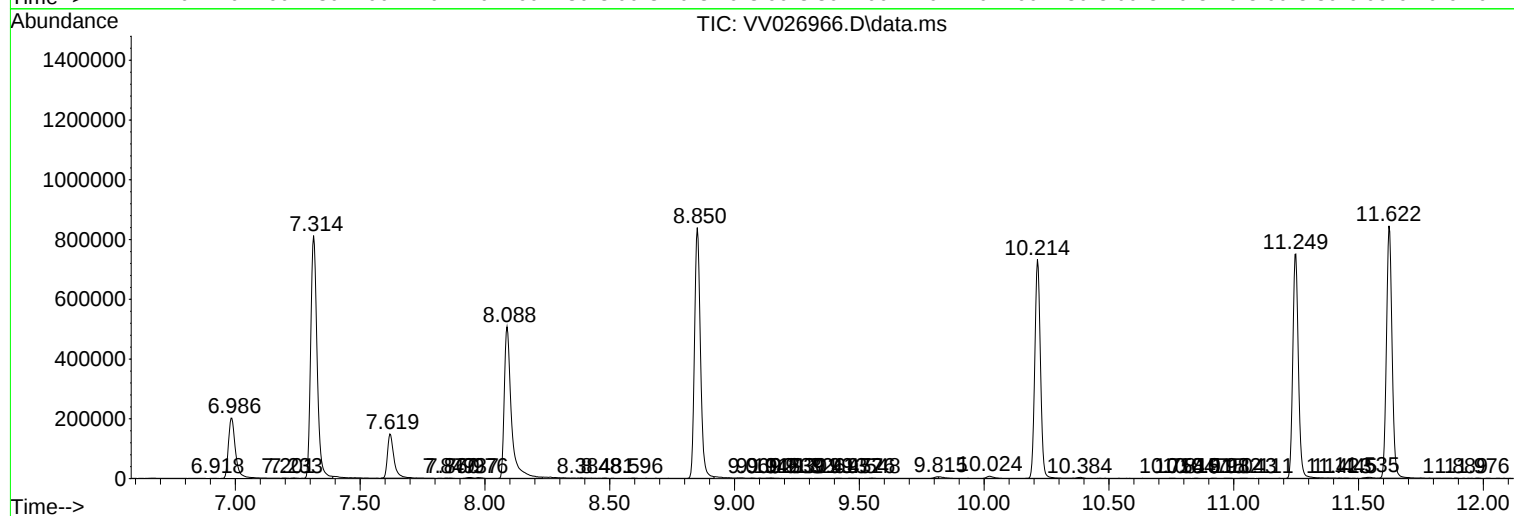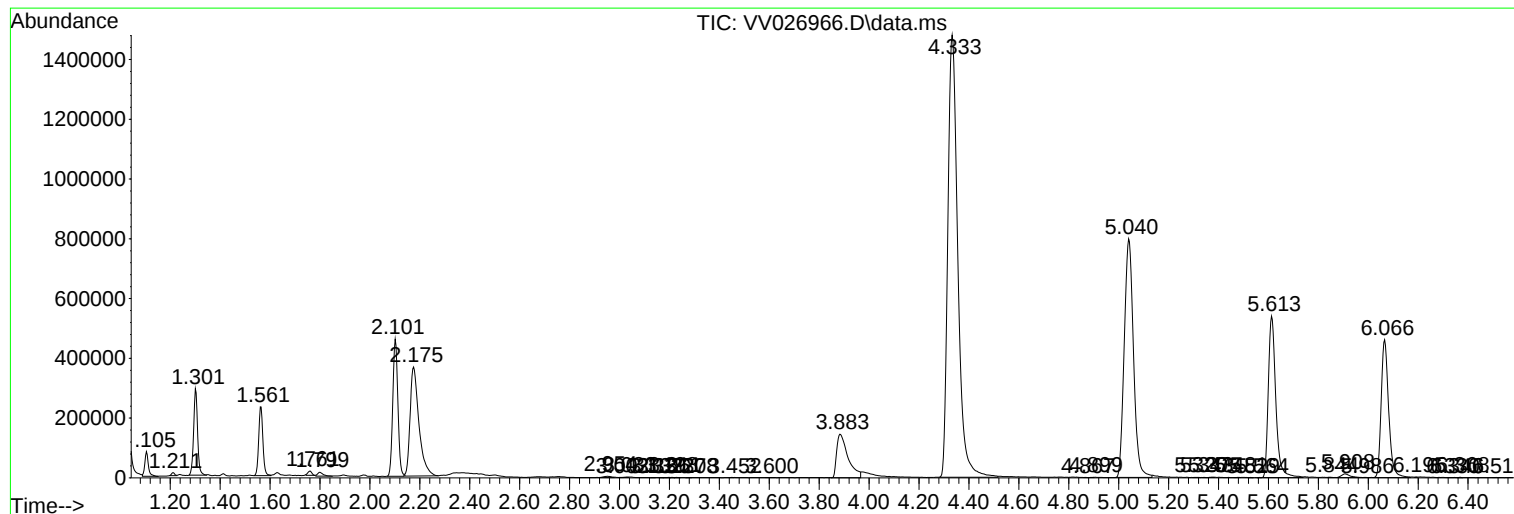

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026966.D
Acq On : 26 Jul 2022 21:14
Operator : SY/MD
Sample : N3843-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.105	3.56 ug/L	80019	1,4-Difluorobenzene	5.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	86
2			Propene	42	C3H6	000115-07-1	42
3			Chloro(prop-2-yn-1-yloxy)methanone	118	C4H3ClO2	035718-08-2	39
4			Cyclopropane	42	C3H6	000075-19-4	9
5			Cyclopropene	40	C3H4	002781-85-3	9

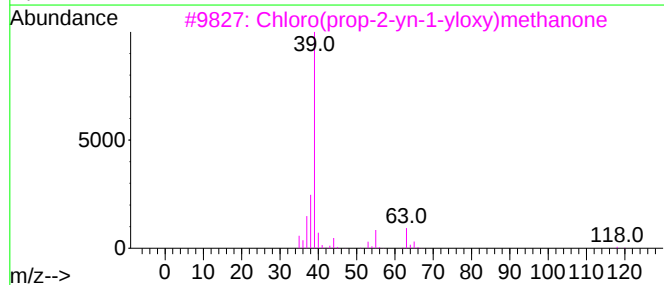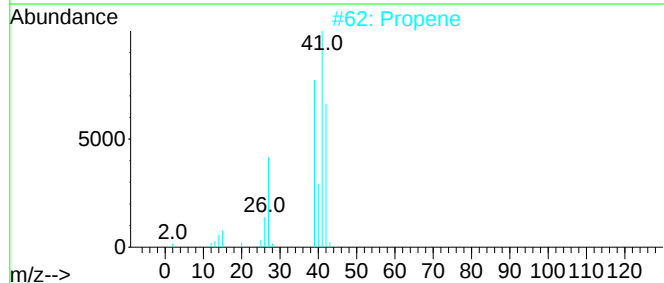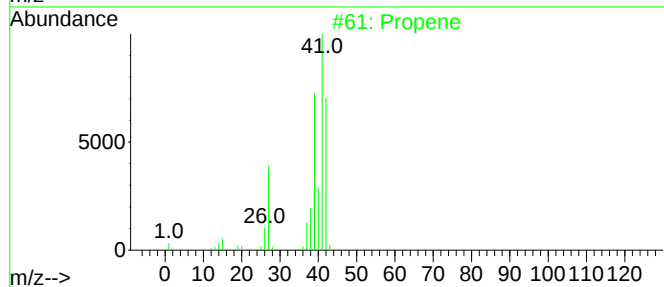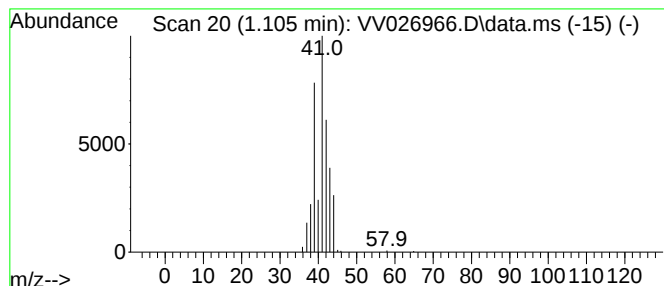

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026966.D
Acq On : 26 Jul 2022 21:14
Operator : SY/MD
Sample : N3843-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.105	3.6	ug/L	80019	1	5.613	1122830	50.0