

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026967.D
 Acq On : 26 Jul 2022 21:39
 Operator : SY/MD
 Sample : N3843-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	254704	269406	13.29%	1.813%
2	1.565	155	163	175	rBV	226684	261130	12.88%	1.757%
3	2.101	319	330	344	rBV	460925	655436	32.33%	4.411%
4	2.285	383	387	394	rVB3	1687	1886	0.09%	0.013%
5	2.433	429	433	435	rBV3	501	363	0.02%	0.002%
6	2.503	447	455	464	rVB3	4277	6571	0.32%	0.044%
7	2.574	470	477	481	rBV5	499	739	0.04%	0.005%
8	2.767	532	537	540	rBV3	667	476	0.02%	0.003%
9	3.018	610	615	617	rBV	271	232	0.01%	0.002%
10	3.275	689	695	699	rVB2	246	249	0.01%	0.002%
11	3.330	708	712	714	rBV	333	260	0.01%	0.002%
12	3.526	767	773	777	rBV2	382	391	0.02%	0.003%
13	3.671	815	818	820	rBV2	373	245	0.01%	0.002%
14	3.693	820	825	828	rBV2	274	288	0.01%	0.002%
15	3.886	873	885	935	rBV	143781	477142	23.54%	3.211%
16	4.343	1009	1027	1064	rBV	343818	862738	42.56%	5.805%
17	4.619	1109	1113	1116	rVV4	363	271	0.01%	0.002%
18	4.809	1167	1172	1175	rBV3	392	347	0.02%	0.002%
19	4.941	1209	1213	1217	rVB2	325	284	0.01%	0.002%
20	4.970	1217	1222	1225	rBV2	295	286	0.01%	0.002%
21	5.040	1227	1244	1283	rBV2	780984	2027304	100.00%	13.642%
22	5.272	1313	1316	1321	rBV4	529	546	0.03%	0.004%
23	5.355	1339	1342	1347	rVB3	432	284	0.01%	0.002%
24	5.407	1357	1358	1363	rVV2	713	412	0.02%	0.003%
25	5.613	1410	1422	1447	rBV	543765	1106646	54.59%	7.447%
26	5.793	1475	1478	1481	rVB3	857	571	0.03%	0.004%
27	5.908	1503	1514	1536	rVB4	12034	28334	1.40%	0.191%
28	6.066	1549	1563	1591	rBV	464110	951753	46.95%	6.404%
29	6.246	1616	1619	1625	rVB4	666	688	0.03%	0.005%
30	6.342	1647	1649	1651	rBV2	463	247	0.01%	0.002%
31	6.384	1659	1662	1665	rVB2	522	329	0.02%	0.002%
32	6.410	1665	1670	1675	rBV	461	421	0.02%	0.003%
33	6.500	1691	1698	1699	rVV3	282	306	0.02%	0.002%
34	6.590	1723	1726	1732	rBV3	261	279	0.01%	0.002%
35	6.664	1746	1749	1754	rVV3	601	455	0.02%	0.003%
36	6.722	1763	1767	1770	rVB3	557	456	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026967.D
 Acq On : 26 Jul 2022 21:39
 Operator : SY/MD
 Sample : N3843-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.741	1770	1773	1777	rVB2	495	282	0.01%	0.002%
38	6.770	1777	1782	1787	rVB2	470	440	0.02%	0.003%
39	6.796	1787	1790	1795	rBV	472	348	0.02%	0.002%
40	6.982	1838	1848	1876	rBV	203824	385242	19.00%	2.592%
41	7.256	1931	1933	1938	rVB5	464	304	0.01%	0.002%
42	7.313	1939	1951	1979	rBV	818504	1448897	71.47%	9.750%
43	7.619	2035	2046	2071	rBV	145996	265964	13.12%	1.790%
44	7.937	2138	2145	2151	rVV3	2363	3761	0.19%	0.025%
45	7.979	2151	2158	2169	rVB7	5152	8630	0.43%	0.058%
46	8.088	2182	2192	2230	rBV	506610	996482	49.15%	6.705%
47	8.487	2312	2316	2320	rVB3	471	417	0.02%	0.003%
48	8.645	2361	2365	2372	rVB5	579	636	0.03%	0.004%
49	8.712	2381	2386	2388	rBV2	404	271	0.01%	0.002%
50	8.850	2417	2429	2457	rBV	853614	1404304	69.27%	9.450%
51	9.014	2478	2480	2483	rVB	719	298	0.01%	0.002%
52	9.114	2508	2511	2514	rBV4	601	473	0.02%	0.003%
53	9.397	2596	2599	2602	rVB3	503	334	0.02%	0.002%
54	9.423	2602	2607	2611	rBV3	557	506	0.02%	0.003%
55	9.702	2689	2694	2697	rBV3	354	301	0.01%	0.002%
56	9.780	2714	2718	2720	rBV2	297	256	0.01%	0.002%
57	9.940	2761	2768	2774	rBV2	706	827	0.04%	0.006%
58	9.973	2776	2778	2782	rVB2	407	261	0.01%	0.002%
59	10.050	2797	2802	2804	rBV2	568	400	0.02%	0.003%
60	10.101	2814	2818	2823	rVB2	365	366	0.02%	0.002%
61	10.214	2838	2853	2884	rBV	734409	1155328	56.99%	7.774%
62	10.323	2884	2887	2890	rBV2	436	269	0.01%	0.002%
63	10.381	2897	2905	2916	rVB3	3522	5988	0.30%	0.040%
64	10.548	2952	2957	2961	rBV3	724	587	0.03%	0.004%
65	10.574	2961	2965	2970	rVB5	650	663	0.03%	0.004%
66	10.641	2982	2986	2992	rVB2	488	505	0.02%	0.003%
67	10.670	2992	2995	2999	rBV2	356	371	0.02%	0.002%
68	10.760	3015	3023	3026	rBV2	498	751	0.04%	0.005%
69	10.854	3048	3052	3058	rBV6	598	671	0.03%	0.005%
70	10.924	3068	3074	3082	rVV4	904	1135	0.06%	0.008%
71	10.963	3082	3086	3091	rVV3	437	405	0.02%	0.003%
72	10.992	3092	3095	3099	rVB3	373	279	0.01%	0.002%
73	11.104	3127	3130	3138	rVB2	534	634	0.03%	0.004%
74	11.188	3153	3156	3161	rVB3	569	455	0.02%	0.003%
75	11.249	3163	3175	3195	rBV	758357	1183739	58.39%	7.966%
76	11.493	3248	3251	3256	rVB3	469	373	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026967.D
 Acq On : 26 Jul 2022 21:39
 Operator : SY/MD
 Sample : N3843-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.538	3256	3265	3270	rBV6	2589	3903	0.19%	0.026%
78	11.622	3278	3291	3314	rBV	843499	1316139	64.92%	8.856%
79	11.921	3382	3384	3388	rVB2	476	245	0.01%	0.002%
80	12.143	3447	3453	3456	rBV2	623	501	0.02%	0.003%
81	12.178	3460	3464	3466	rBV2	320	234	0.01%	0.002%
82	12.616	3596	3600	3603	rBV3	359	281	0.01%	0.002%
83	12.702	3622	3627	3633	rBV4	538	721	0.04%	0.005%
84	13.130	3756	3760	3764	rBV3	397	419	0.02%	0.003%
85	13.156	3765	3768	3770	rVV2	512	391	0.02%	0.003%
86	13.268	3798	3803	3804	rBV2	491	461	0.02%	0.003%
87	13.503	3870	3876	3879	rBV3	773	776	0.04%	0.005%
88	13.525	3879	3883	3888	rVV3	849	810	0.04%	0.005%
89	13.577	3896	3899	3902	rBV2	465	286	0.01%	0.002%
90	13.660	3920	3925	3928	rBV3	392	338	0.02%	0.002%
91	13.709	3936	3940	3946	rBV4	631	825	0.04%	0.006%
92	13.796	3963	3967	3972	rBV	577	601	0.03%	0.004%
93	13.873	3988	3991	3996	rVB2	631	532	0.03%	0.004%
94	13.898	3996	3999	4001	rBV2	488	241	0.01%	0.002%
95	13.914	4001	4004	4007	rBV3	611	532	0.03%	0.004%
96	14.030	4038	4040	4044	rBV3	539	377	0.02%	0.003%
97	14.104	4060	4063	4065	rBV2	508	378	0.02%	0.003%
98	15.361	4450	4454	4456	rBV2	679	572	0.03%	0.004%
99	15.590	4522	4525	4526	rBV3	717	315	0.02%	0.002%
100	15.985	4645	4648	4651	rBV3	1153	924	0.05%	0.006%




Sum of corrected areas: 14860726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026967.D
Acq On : 26 Jul 2022 21:39
Operator : SY/MD
Sample : N3843-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

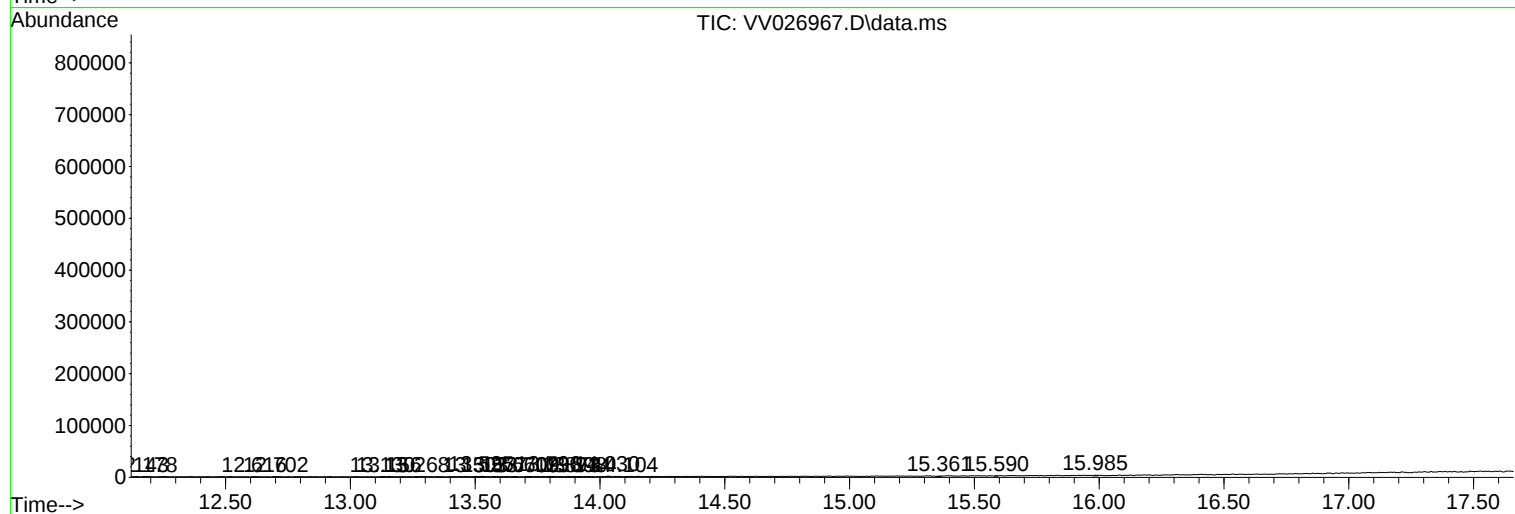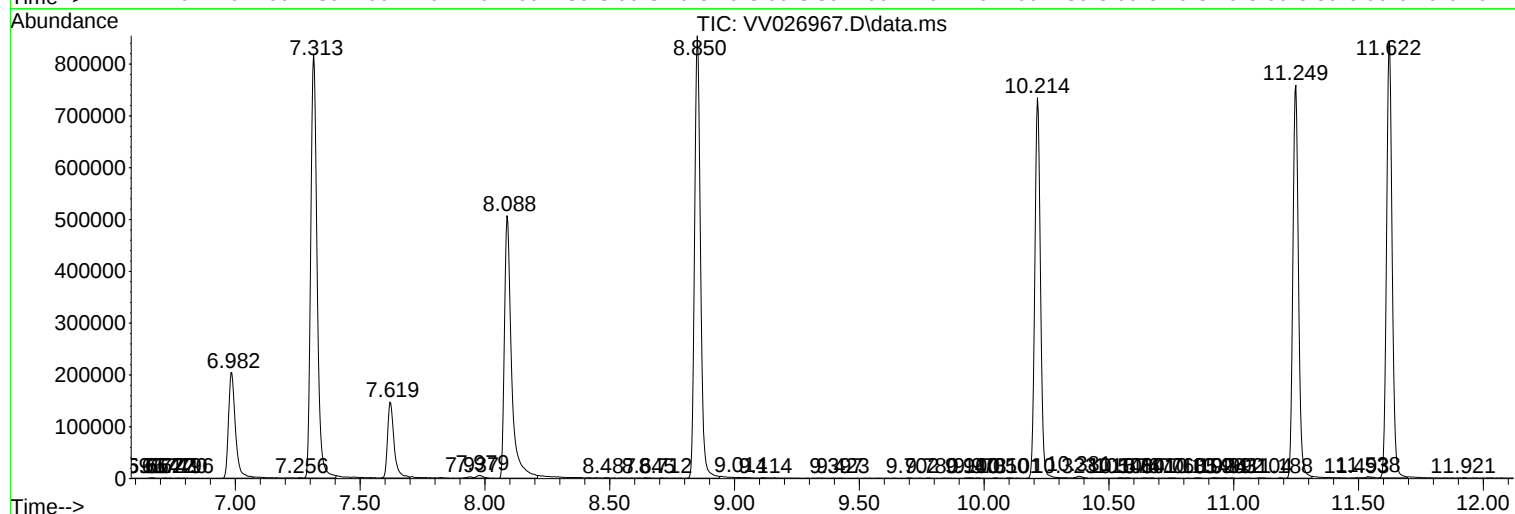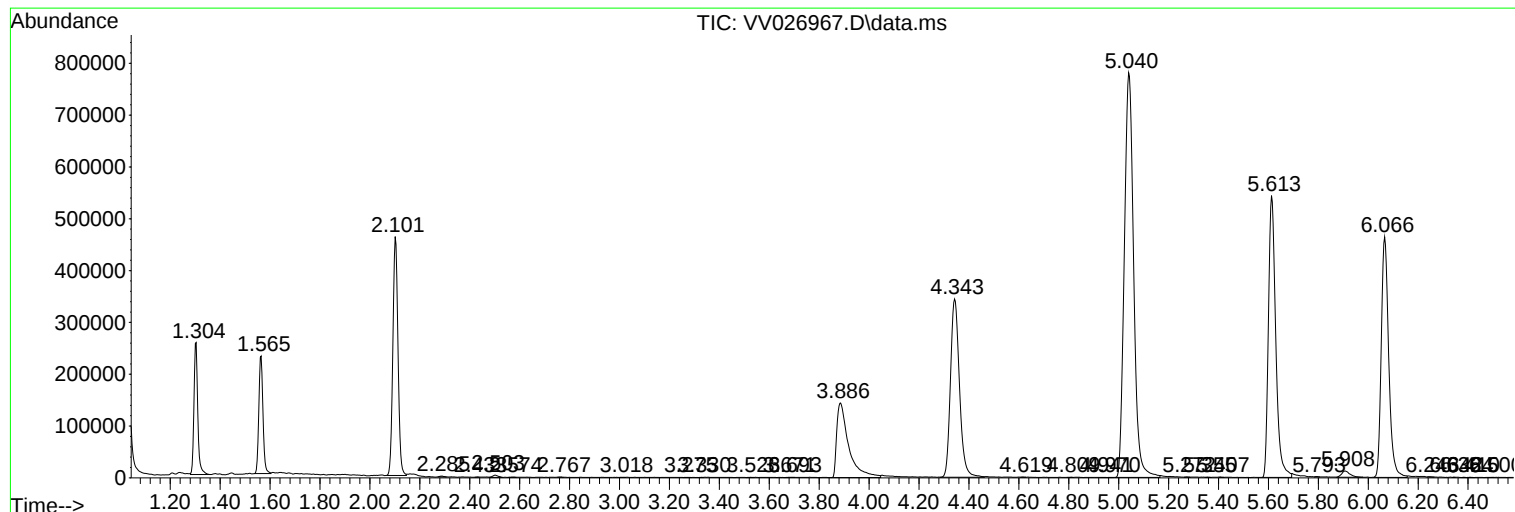

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026967.D
Acq On : 26 Jul 2022 21:39
Operator : SY/MD
Sample : N3843-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026967.D
Acq On : 26 Jul 2022 21:39
Operator : SY/MD
Sample : N3843-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc