

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026971.D
 Acq On : 26 Jul 2022 23:40
 Operator : SY/MD
 Sample : VV0726WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	251368	257171	12.83%	1.740%
2	1.564	155	163	175	rBV	227673	257910	12.86%	1.745%
3	2.101	320	330	347	rBV	443061	640551	31.95%	4.334%
4	2.288	383	388	396	rVB	3728	4908	0.24%	0.033%
5	2.503	447	455	467	rVB3	12714	21396	1.07%	0.145%
6	2.619	480	491	502	rBV5	1797	3897	0.19%	0.026%
7	2.661	502	504	507	rVV5	408	294	0.01%	0.002%
8	2.680	507	510	513	rVB2	477	279	0.01%	0.002%
9	2.764	525	536	548	rBV7	3435	6800	0.34%	0.046%
10	2.844	557	561	567	rBV3	300	363	0.02%	0.002%
11	2.905	573	580	583	rBV2	445	507	0.03%	0.003%
12	3.092	636	638	645	rVB2	347	310	0.02%	0.002%
13	3.182	658	666	669	rBV4	911	1338	0.07%	0.009%
14	3.240	680	684	688	rBV2	342	324	0.02%	0.002%
15	3.278	691	696	699	rBV3	315	329	0.02%	0.002%
16	3.407	733	736	741	rBV2	354	298	0.01%	0.002%
17	3.529	767	774	777	rBV2	482	616	0.03%	0.004%
18	3.664	812	816	820	rBV2	283	264	0.01%	0.002%
19	3.889	875	886	937	rBV2	156040	583329	29.10%	3.947%
20	4.342	1010	1027	1063	rBV	333950	832316	41.52%	5.632%
21	4.535	1084	1087	1091	rVB3	509	438	0.02%	0.003%
22	4.555	1091	1093	1095	rBV4	454	278	0.01%	0.002%
23	4.593	1101	1105	1106	rBV3	676	423	0.02%	0.003%
24	4.674	1124	1130	1133	rVV6	1219	1380	0.07%	0.009%
25	4.725	1143	1146	1150	rVB4	613	432	0.02%	0.003%
26	4.821	1168	1176	1178	rBV5	1356	1913	0.10%	0.013%
27	4.834	1178	1180	1183	rVB4	799	453	0.02%	0.003%
28	5.043	1227	1245	1288	rBV2	770307	2004838	100.00%	13.566%
29	5.352	1336	1341	1344	rBV3	630	606	0.03%	0.004%
30	5.375	1346	1348	1353	rVB4	616	474	0.02%	0.003%
31	5.513	1389	1391	1393	rVB2	625	259	0.01%	0.002%
32	5.558	1400	1405	1410	rBV4	709	824	0.04%	0.006%
33	5.612	1410	1422	1460	rBV	525245	1077001	53.72%	7.288%
34	5.911	1503	1515	1534	rVB4	12779	30236	1.51%	0.205%
35	6.066	1547	1563	1593	rBV	453836	943758	47.07%	6.386%
36	6.403	1664	1668	1674	rVB3	417	341	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026971.D
 Acq On : 26 Jul 2022 23:40
 Operator : SY/MD
 Sample : VV0726WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.477	1685	1691	1695	rBV3	501	550	0.03%	0.004%
38	6.510	1698	1701	1704	rBV3	508	431	0.02%	0.003%
39	6.625	1732	1737	1742	rBV2	330	469	0.02%	0.003%
40	6.661	1742	1748	1751	rVV5	733	780	0.04%	0.005%
41	6.690	1754	1757	1763	rVB2	755	724	0.04%	0.005%
42	6.815	1794	1796	1800	rBV3	298	267	0.01%	0.002%
43	6.940	1831	1835	1838	rBV3	435	428	0.02%	0.003%
44	6.985	1838	1849	1874	rBV	200608	383757	19.14%	2.597%
45	7.146	1896	1899	1901	rBV3	609	358	0.02%	0.002%
46	7.239	1921	1928	1939	rVB8	1598	2497	0.12%	0.017%
47	7.313	1939	1951	1973	rBV	810035	1433905	71.52%	9.703%
48	7.574	2030	2032	2036	rVV2	408	274	0.01%	0.002%
49	7.622	2036	2047	2079	rVV	143104	264933	13.21%	1.793%
50	7.847	2112	2117	2118	rBV5	1156	999	0.05%	0.007%
51	7.918	2137	2139	2142	rBV2	562	355	0.02%	0.002%
52	7.934	2142	2144	2148	rBV2	364	297	0.01%	0.002%
53	7.979	2151	2158	2168	rVB9	3036	5445	0.27%	0.037%
54	8.037	2174	2176	2181	rVB3	482	338	0.02%	0.002%
55	8.088	2182	2192	2225	rBV	491662	985486	49.16%	6.668%
56	8.352	2269	2274	2278	rBV6	1222	968	0.05%	0.007%
57	8.587	2343	2347	2348	rBV	402	291	0.01%	0.002%
58	8.622	2354	2358	2362	rVB4	663	467	0.02%	0.003%
59	8.644	2362	2365	2367	rBV2	397	257	0.01%	0.002%
60	8.747	2394	2397	2403	rVB3	532	445	0.02%	0.003%
61	8.796	2409	2412	2418	rBV3	448	536	0.03%	0.004%
62	8.850	2418	2429	2458	rBV	812626	1331300	66.40%	9.008%
63	9.149	2515	2522	2533	rBV6	2063	4098	0.20%	0.028%
64	9.313	2570	2573	2577	rBV3	347	273	0.01%	0.002%
65	9.342	2580	2582	2587	rVB3	453	329	0.02%	0.002%
66	9.371	2587	2591	2600	rVB3	491	523	0.03%	0.004%
67	9.419	2602	2606	2611	rBV	619	409	0.02%	0.003%
68	9.448	2611	2615	2619	rVB3	622	554	0.03%	0.004%
69	9.477	2619	2624	2626	rBV	372	339	0.02%	0.002%
70	9.554	2640	2648	2653	rBV5	2463	3941	0.20%	0.027%
71	9.731	2700	2703	2705	rBV2	715	464	0.02%	0.003%
72	9.937	2758	2767	2777	rVB5	2690	4338	0.22%	0.029%
73	10.101	2814	2818	2819	rBV2	580	300	0.01%	0.002%
74	10.111	2819	2821	2825	rVB2	428	265	0.01%	0.002%
75	10.214	2841	2853	2882	rBV	720555	1130184	56.37%	7.648%
76	10.490	2935	2939	2941	rBV3	385	289	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026971.D
 Acq On : 26 Jul 2022 23:40
 Operator : SY/MD
 Sample : VV0726WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.542	2948	2955	2962	rBV5	2813	3512	0.18%	0.024%
78	10.683	2995	2999	3001	rBV	480	342	0.02%	0.002%
79	10.808	3035	3038	3042	rBV2	427	311	0.02%	0.002%
80	10.857	3049	3053	3057	rBV3	828	821	0.04%	0.006%
81	10.924	3065	3074	3082	rBV6	2286	3620	0.18%	0.024%
82	10.998	3093	3097	3100	rBV2	364	276	0.01%	0.002%
83	11.188	3148	3156	3163	rBV6	3825	5648	0.28%	0.038%
84	11.249	3163	3175	3198	rVV	732944	1159565	57.84%	7.846%
85	11.541	3263	3266	3270	rVV2	451	319	0.02%	0.002%
86	11.622	3279	3291	3318	rBV	844087	1322461	65.96%	8.949%
87	12.046	3420	3423	3426	rBV2	424	325	0.02%	0.002%
88	12.091	3435	3437	3442	rBV2	456	370	0.02%	0.003%
89	12.252	3480	3487	3494	rBV2	1050	1540	0.08%	0.010%
90	12.651	3602	3611	3619	rBV4	4396	6340	0.32%	0.043%
91	12.934	3696	3699	3702	rBV2	458	257	0.01%	0.002%
92	12.988	3713	3716	3720	rVB2	577	435	0.02%	0.003%
93	13.082	3742	3745	3750	rBV4	472	431	0.02%	0.003%
94	13.127	3757	3759	3763	rVB2	535	288	0.01%	0.002%
95	13.149	3763	3766	3771	rBV	507	376	0.02%	0.003%
96	13.271	3795	3804	3814	rVB6	4870	8162	0.41%	0.055%
97	13.509	3871	3878	3897	rVB2	8363	13524	0.67%	0.092%
98	13.747	3944	3952	3963	rBV4	5639	8716	0.43%	0.059%
99	15.377	4457	4459	4461	rBV	641	361	0.02%	0.002%
100	15.509	4498	4500	4507	rVB5	929	664	0.03%	0.004%




Sum of corrected areas: 14778381

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026971.D
Acq On : 26 Jul 2022 23:40
Operator : SY/MD
Sample : VV0726WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

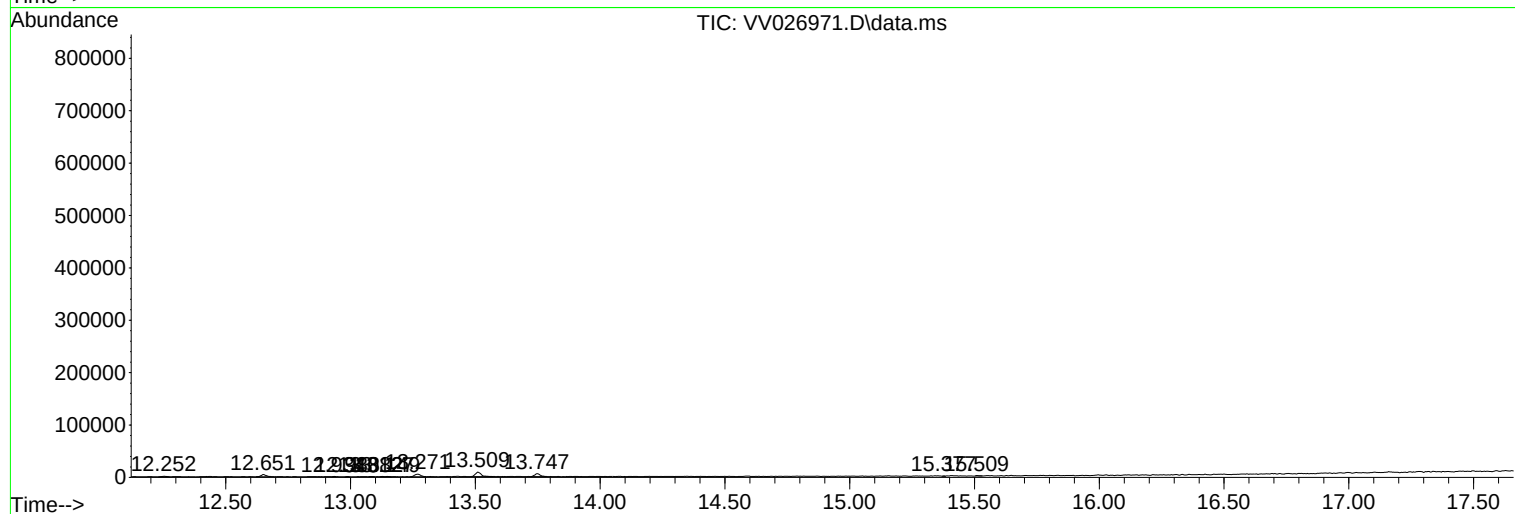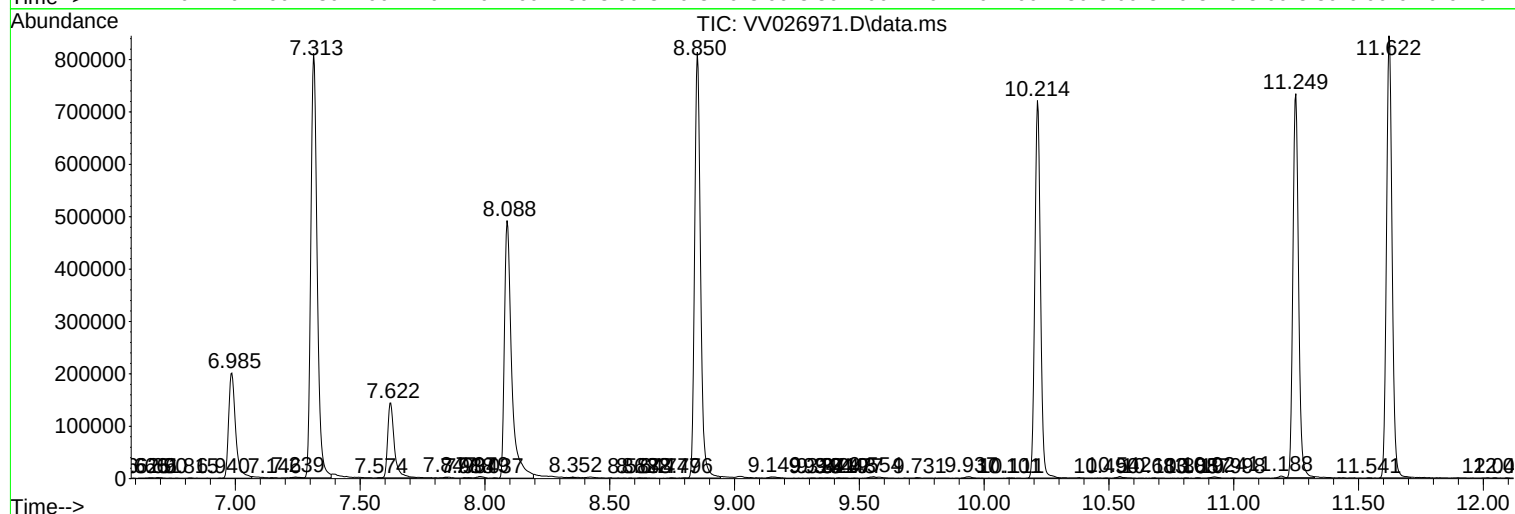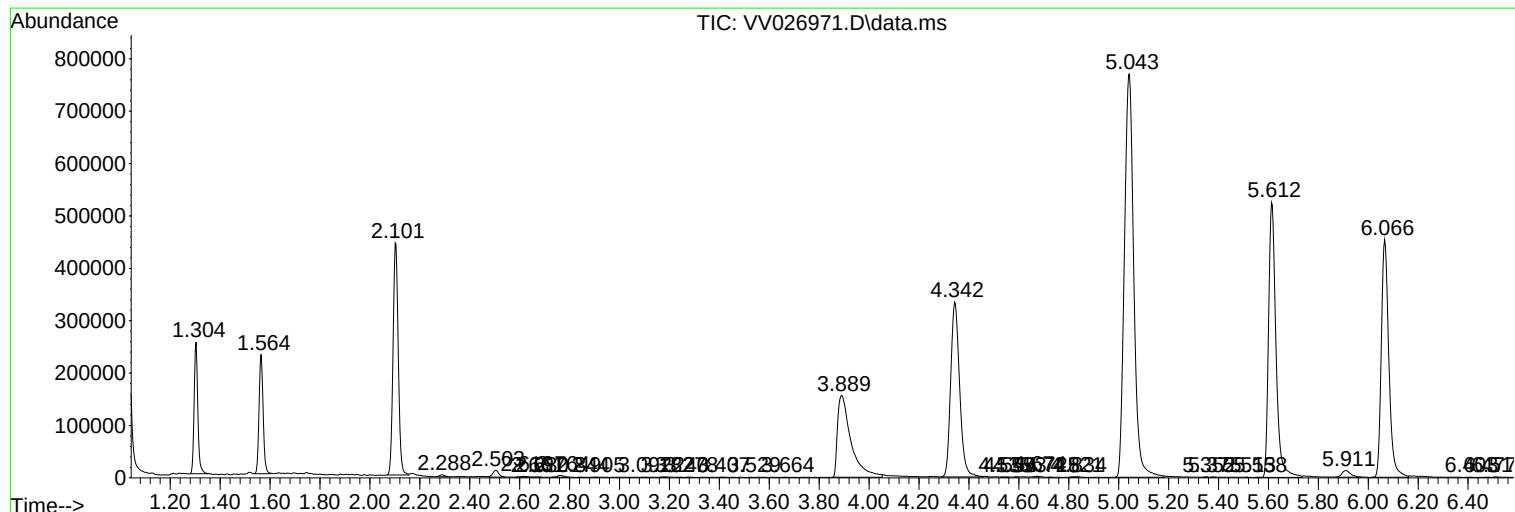

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026971.D
Acq On : 26 Jul 2022 23:40
Operator : SY/MD
Sample : VV0726WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026971.D
Acq On : 26 Jul 2022 23:40
Operator : SY/MD
Sample : VV0726WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------