

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026976.D
 Acq On : 27 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3843-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	269514	272049	13.03%	1.779%
2	1.564	155	163	180	rBV	239245	271379	13.00%	1.774%
3	2.105	320	331	346	rBV	464428	660573	31.65%	4.319%
4	2.375	412	415	417	rBV2	617	351	0.02%	0.002%
5	2.503	447	455	464	rBV4	3202	5137	0.25%	0.034%
6	2.761	527	535	547	rBV6	1191	2258	0.11%	0.015%
7	2.934	585	589	593	rBV	338	387	0.02%	0.003%
8	3.082	632	635	639	rVB	499	346	0.02%	0.002%
9	3.191	664	669	670	rBV	350	296	0.01%	0.002%
10	3.452	746	750	755	rVB2	469	366	0.02%	0.002%
11	3.551	774	781	785	rBV2	518	692	0.03%	0.005%
12	3.744	837	841	846	rVB2	264	311	0.01%	0.002%
13	3.777	846	851	853	rBV	417	286	0.01%	0.002%
14	3.886	875	885	936	rBV	142615	497729	23.85%	3.254%
15	4.342	1010	1027	1064	rVV	349769	870568	41.71%	5.692%
16	4.548	1089	1091	1095	rVB2	743	434	0.02%	0.003%
17	4.625	1111	1115	1116	rBV3	580	356	0.02%	0.002%
18	4.751	1151	1154	1160	rBV	507	454	0.02%	0.003%
19	4.825	1169	1177	1180	rBV5	1346	1891	0.09%	0.012%
20	5.040	1226	1244	1277	rBV2	805027	2087110	100.00%	13.647%
21	5.548	1399	1402	1405	rBB3	408	281	0.01%	0.002%
22	5.612	1410	1422	1454	rBV	550571	1131603	54.22%	7.399%
23	5.908	1503	1514	1528	rBV3	12730	26591	1.27%	0.174%
24	5.989	1537	1539	1545	rVB3	747	547	0.03%	0.004%
25	6.066	1547	1563	1589	rBV	478559	977841	46.85%	6.394%
26	6.191	1598	1602	1604	rBV3	863	690	0.03%	0.005%
27	6.291	1630	1633	1639	rVB4	607	592	0.03%	0.004%
28	6.355	1649	1653	1654	rBV	630	298	0.01%	0.002%
29	6.394	1661	1665	1668	rVB3	518	379	0.02%	0.002%
30	6.516	1700	1703	1708	rVV4	970	766	0.04%	0.005%
31	6.538	1708	1710	1715	rVB3	511	435	0.02%	0.003%
32	6.638	1736	1741	1744	rBV3	313	352	0.02%	0.002%
33	6.661	1744	1748	1753	rBV4	362	430	0.02%	0.003%
34	6.709	1761	1763	1769	rVB3	742	597	0.03%	0.004%
35	6.754	1775	1777	1781	rVB2	627	374	0.02%	0.002%
36	6.780	1781	1785	1789	rBV4	529	391	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026976.D
 Acq On : 27 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3843-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.809	1792	1794	1798	rBV2	382	290	0.01%	0.002%
38	6.857	1806	1809	1814	rVB3	531	371	0.02%	0.002%
39	6.982	1838	1848	1876	rBV	207531	393697	18.86%	2.574%
40	7.194	1912	1914	1916	rBV2	486	336	0.02%	0.002%
41	7.239	1924	1928	1934	rBV4	700	639	0.03%	0.004%
42	7.313	1939	1951	1975	rBV	857324	1518387	72.75%	9.928%
43	7.619	2037	2046	2069	rBV	146562	266346	12.76%	1.742%
44	7.940	2134	2146	2152	rBV5	2697	4402	0.21%	0.029%
45	7.969	2152	2155	2156	rBV2	787	419	0.02%	0.003%
46	7.982	2156	2159	2170	rVB6	2445	2906	0.14%	0.019%
47	8.088	2182	2192	2238	rBV	519309	1030346	49.37%	6.737%
48	8.596	2346	2350	2354	rBV2	349	287	0.01%	0.002%
49	8.699	2378	2382	2385	rVV4	385	291	0.01%	0.002%
50	8.754	2395	2399	2402	rBV2	352	299	0.01%	0.002%
51	8.850	2418	2429	2464	rBV	877500	1430954	68.56%	9.356%
52	9.079	2496	2500	2502	rBV3	631	451	0.02%	0.003%
53	9.249	2548	2553	2559	rBV3	533	660	0.03%	0.004%
54	9.291	2563	2566	2571	rVB3	372	293	0.01%	0.002%
55	9.429	2605	2609	2613	rBV2	308	340	0.02%	0.002%
56	9.593	2654	2660	2662	rBV2	304	312	0.01%	0.002%
57	9.606	2662	2664	2670	rVB3	496	294	0.01%	0.002%
58	9.654	2675	2679	2681	rBV2	405	316	0.02%	0.002%
59	9.934	2761	2766	2768	rBV2	699	708	0.03%	0.005%
60	10.011	2786	2790	2792	rBV2	372	291	0.01%	0.002%
61	10.214	2841	2853	2875	rBV	747662	1167709	55.95%	7.635%
62	10.381	2899	2905	2912	rVV3	2920	3545	0.17%	0.023%
63	10.429	2916	2920	2924	rVB3	324	279	0.01%	0.002%
64	10.625	2976	2981	2986	rVB3	508	658	0.03%	0.004%
65	10.651	2986	2989	2992	rBV2	437	352	0.02%	0.002%
66	10.686	2998	3000	3004	rVV3	365	277	0.01%	0.002%
67	10.902	3065	3067	3070	rBV2	457	294	0.01%	0.002%
68	10.921	3070	3073	3075	rVV2	522	291	0.01%	0.002%
69	11.005	3092	3099	3105	rVB3	388	606	0.03%	0.004%
70	11.037	3105	3109	3112	rBV2	350	336	0.02%	0.002%
71	11.072	3118	3120	3124	rBV2	414	308	0.01%	0.002%
72	11.169	3140	3150	3153	rBV3	576	898	0.04%	0.006%
73	11.188	3153	3156	3161	rBV3	567	461	0.02%	0.003%
74	11.246	3163	3174	3194	rBV	775356	1221613	58.53%	7.988%
75	11.538	3257	3265	3277	rBV7	4686	8868	0.42%	0.058%
76	11.622	3279	3291	3315	rBV	881350	1385887	66.40%	9.062%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026976.D
 Acq On : 27 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3843-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.866	3365	3367	3374	rVB3	482	321	0.02%	0.002%
78	12.220	3472	3477	3480	rBV2	608	597	0.03%	0.004%
79	12.307	3501	3504	3510	rBV3	345	406	0.02%	0.003%
80	12.429	3537	3542	3544	rBV2	432	402	0.02%	0.003%
81	12.644	3606	3609	3611	rBV	687	493	0.02%	0.003%
82	12.741	3637	3639	3643	rBV2	434	374	0.02%	0.002%
83	12.866	3675	3678	3686	rBV3	378	311	0.01%	0.002%
84	13.040	3727	3732	3735	rBV3	418	409	0.02%	0.003%
85	13.197	3775	3781	3786	rBV3	445	539	0.03%	0.004%
86	13.265	3798	3802	3804	rBV3	897	690	0.03%	0.005%
87	13.365	3829	3833	3838	rBV4	468	555	0.03%	0.004%
88	13.387	3838	3840	3845	rVB2	441	356	0.02%	0.002%
89	13.416	3845	3849	3850	rBV3	771	539	0.03%	0.004%
90	13.516	3869	3880	3888	rBV	4439	7734	0.37%	0.051%
91	13.628	3907	3915	3920	rBV3	976	1497	0.07%	0.010%
92	14.069	4048	4052	4053	rBV	363	286	0.01%	0.002%
93	14.204	4092	4094	4098	rBV3	527	375	0.02%	0.002%
94	14.226	4098	4101	4106	rVV3	530	500	0.02%	0.003%
95	14.699	4246	4248	4251	rBV	618	430	0.02%	0.003%
96	14.818	4276	4285	4294	rBV2	8818	14398	0.69%	0.094%
97	14.869	4299	4301	4303	rBV2	542	279	0.01%	0.002%
98	14.988	4335	4338	4342	rVB3	723	527	0.03%	0.003%
99	15.030	4349	4351	4352	rBV	799	335	0.02%	0.002%
100	15.184	4397	4399	4400	rBV3	761	301	0.01%	0.002%




Sum of corrected areas: 15293811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026976.D
Acq On : 27 Jul 2022 01:43
Operator : SY/MD
Sample : N3843-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

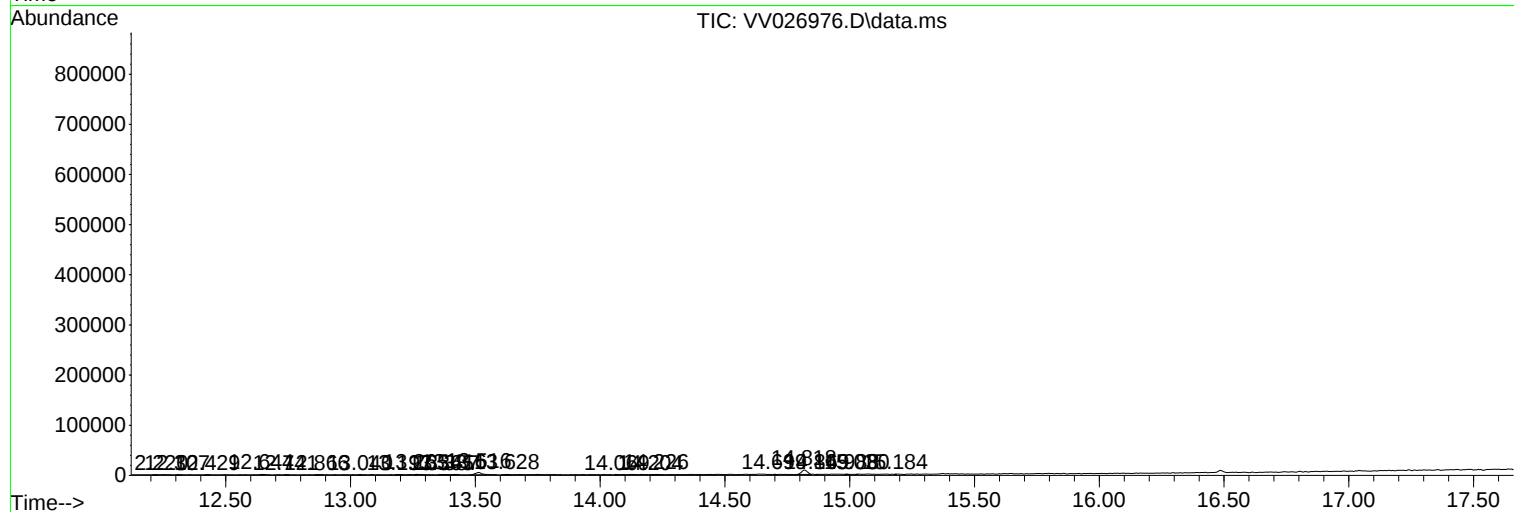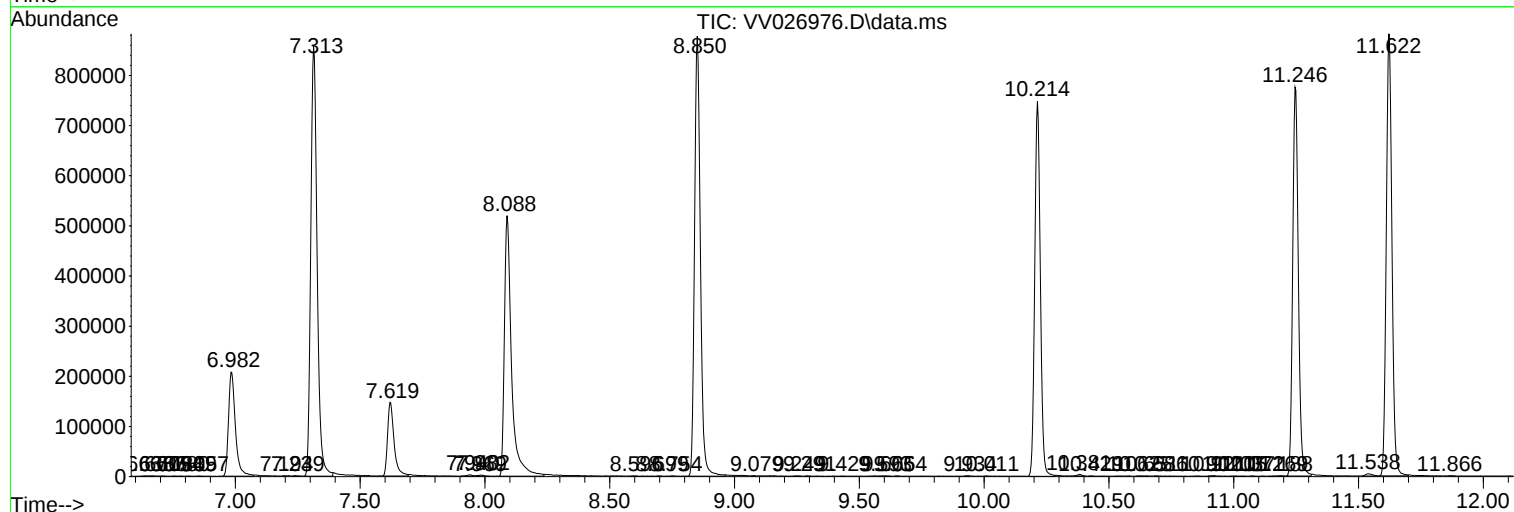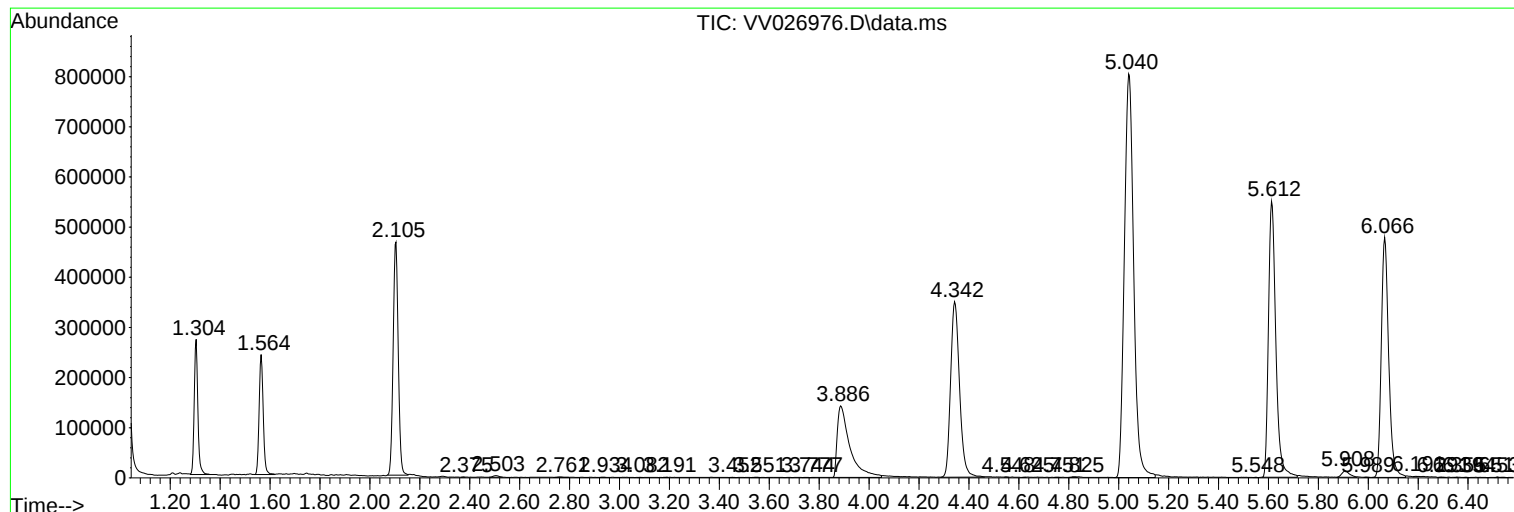

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026976.D
Acq On : 27 Jul 2022 01:43
Operator : SY/MD
Sample : N3843-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026976.D
Acq On : 27 Jul 2022 01:43
Operator : SY/MD
Sample : N3843-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc