

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026977.D
 Acq On : 27 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3880-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	356864	367360	3.86%	1.331%
2	1.564	155	163	175	rBV	302124	342477	3.60%	1.241%
3	2.105	319	331	349	rBV	605098	872554	9.18%	3.161%
4	2.291	382	389	397	rVB4	1725	2608	0.03%	0.009%
5	2.442	434	436	444	rVB4	803	696	0.01%	0.003%
6	2.481	444	448	449	rVV2	558	387	0.00%	0.001%
7	2.503	449	455	467	rVB6	3683	5800	0.06%	0.021%
8	2.654	498	502	504	rBV	435	314	0.00%	0.001%
9	2.764	526	536	547	rVB6	3506	6841	0.07%	0.025%
10	2.867	565	568	574	rBV3	322	422	0.00%	0.002%
11	2.957	593	596	601	rVB	464	336	0.00%	0.001%
12	2.995	601	608	609	rBV2	224	254	0.00%	0.001%
13	3.153	653	657	659	rBV3	427	317	0.00%	0.001%
14	3.185	664	667	672	rBV2	321	372	0.00%	0.001%
15	3.278	693	696	701	rVB2	468	420	0.00%	0.002%
16	3.349	715	718	721	rBV3	355	285	0.00%	0.001%
17	3.603	793	797	800	rVB2	426	316	0.00%	0.001%
18	3.690	820	824	828	rBV2	355	394	0.00%	0.001%
19	3.770	844	849	852	rBV2	314	257	0.00%	0.001%
20	3.812	857	862	867	rVB2	565	538	0.01%	0.002%
21	3.844	867	872	874	rBV2	425	347	0.00%	0.001%
22	3.899	874	889	937	rBV3	207251	772770	8.13%	2.800%
23	4.342	1011	1027	1066	rBV	403844	1015549	10.68%	3.679%
24	4.735	1147	1149	1159	rVV5	485	618	0.01%	0.002%
25	4.937	1210	1212	1217	rVB2	450	335	0.00%	0.001%
26	4.982	1221	1226	1228	rBV2	393	308	0.00%	0.001%
27	5.043	1228	1245	1280	rBV2	962105	2488651	26.17%	9.016%
28	5.291	1319	1322	1325	rVB3	593	381	0.00%	0.001%
29	5.326	1329	1333	1334	rVB3	581	320	0.00%	0.001%
30	5.429	1363	1365	1371	rVB3	460	247	0.00%	0.001%
31	5.529	1393	1396	1399	rVB3	520	356	0.00%	0.001%
32	5.548	1399	1402	1405	rBV2	553	358	0.00%	0.001%
33	5.612	1408	1422	1457	rBV	569136	1180401	12.41%	4.276%
34	5.844	1490	1494	1497	rBV4	774	673	0.01%	0.002%
35	5.911	1502	1515	1540	rVV	251921	519176	5.46%	1.881%
36	6.066	1549	1563	1592	rBV	558767	1135923	11.95%	4.115%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026977.D
 Acq On : 27 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3880-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.339	1645	1648	1650	rBV3	411	275	0.00%	0.001%
38	6.358	1651	1654	1656	rVB	471	294	0.00%	0.001%
39	6.378	1656	1660	1661	rBV2	396	261	0.00%	0.001%
40	6.397	1664	1666	1670	rVB3	534	309	0.00%	0.001%
41	6.468	1686	1688	1691	rVB2	568	314	0.00%	0.001%
42	6.493	1691	1696	1702	rBV4	509	442	0.00%	0.002%
43	6.606	1728	1731	1734	rVB3	321	249	0.00%	0.001%
44	6.645	1734	1743	1745	rBV3	719	884	0.01%	0.003%
45	6.741	1769	1773	1775	rBV2	547	428	0.00%	0.002%
46	6.792	1784	1789	1790	rBV2	370	250	0.00%	0.001%
47	6.802	1790	1792	1797	rVB2	393	274	0.00%	0.001%
48	6.831	1797	1801	1805	rBV	617	416	0.00%	0.002%
49	6.895	1815	1821	1823	rBV2	399	326	0.00%	0.001%
50	6.982	1836	1848	1883	rBV	210363	394633	4.15%	1.430%
51	7.313	1939	1951	1974	rBV	1057362	1850182	19.46%	6.703%
52	7.535	2018	2020	2023	rVB4	692	280	0.00%	0.001%
53	7.619	2036	2046	2071	rBV	147199	265019	2.79%	0.960%
54	7.821	2108	2109	2114	rVB3	478	289	0.00%	0.001%
55	7.972	2134	2156	2182	rBV	5836629	9508954	100.00%	34.450%
56	8.088	2183	2192	2234	rVB	596612	1161763	12.22%	4.209%
57	8.558	2336	2338	2343	rBV3	484	325	0.00%	0.001%
58	8.580	2343	2345	2348	rBV3	618	266	0.00%	0.001%
59	8.596	2348	2350	2353	rBV3	528	424	0.00%	0.002%
60	8.644	2362	2365	2367	rBV3	504	324	0.00%	0.001%
61	8.657	2367	2369	2373	rVB3	543	385	0.00%	0.001%
62	8.850	2415	2429	2469	rBV	918589	1498267	15.76%	5.428%
63	9.172	2527	2529	2533	rVB4	603	333	0.00%	0.001%
64	9.220	2540	2544	2549	rBV4	501	633	0.01%	0.002%
65	9.310	2566	2572	2574	rBV2	563	558	0.01%	0.002%
66	9.522	2634	2638	2641	rBV2	336	315	0.00%	0.001%
67	9.545	2643	2645	2648	rVB2	456	251	0.00%	0.001%
68	9.593	2656	2660	2663	rVB3	285	261	0.00%	0.001%
69	9.853	2737	2741	2744	rBV2	420	341	0.00%	0.001%
70	10.030	2794	2796	2802	rVB2	444	393	0.00%	0.001%
71	10.059	2802	2805	2808	rBV2	406	341	0.00%	0.001%
72	10.136	2825	2829	2832	rBV	443	404	0.00%	0.001%
73	10.214	2840	2853	2880	rBV	838321	1297498	13.65%	4.701%
74	10.381	2897	2905	2914	rVB3	5020	7693	0.08%	0.028%
75	10.545	2951	2956	2963	rVB3	615	916	0.01%	0.003%
76	10.587	2963	2969	2973	rBV2	757	831	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026977.D
 Acq On : 27 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3880-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.857	3049	3053	3057	rVB3	787	832	0.01%	0.003%
78	11.172	3147	3151	3153	rBV3	459	385	0.00%	0.001%
79	11.249	3163	3175	3208	rBV	808597	1283935	13.50%	4.652%
80	11.464	3240	3242	3245	rVB2	498	288	0.00%	0.001%
81	11.529	3257	3262	3263	rBV2	569	427	0.00%	0.002%
82	11.622	3277	3291	3315	rBV	1002339	1591794	16.74%	5.767%
83	12.172	3457	3462	3469	rBV4	366	574	0.01%	0.002%
84	12.651	3608	3611	3615	rBV2	560	458	0.00%	0.002%
85	13.001	3715	3720	3728	rVV3	451	751	0.01%	0.003%
86	13.139	3759	3763	3764	rBV	537	272	0.00%	0.001%
87	13.252	3795	3798	3801	rBV3	505	310	0.00%	0.001%
88	13.294	3809	3811	3814	rVB	624	345	0.00%	0.001%
89	13.316	3814	3818	3821	rBV2	303	304	0.00%	0.001%
90	13.493	3871	3873	3874	rBV2	567	251	0.00%	0.001%
91	13.512	3875	3879	3880	rVV3	943	659	0.01%	0.002%
92	13.744	3948	3951	3952	rBV2	622	369	0.00%	0.001%
93	13.860	3985	3987	3991	rBV	934	407	0.00%	0.001%
94	13.882	3991	3994	4000	rBV3	472	521	0.01%	0.002%
95	13.995	4026	4029	4031	rBV3	392	273	0.00%	0.001%
96	14.262	4109	4112	4115	rBV3	621	511	0.01%	0.002%
97	14.644	4228	4231	4234	rBV3	626	514	0.01%	0.002%
98	14.921	4313	4317	4318	rBV2	782	547	0.01%	0.002%
99	15.329	4440	4444	4446	rBV3	1251	985	0.01%	0.004%
100	15.483	4489	4492	4493	rBV2	913	587	0.01%	0.002%




Sum of corrected areas: 27602261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026977.D
Acq On : 27 Jul 2022 02:07
Operator : SY/MD
Sample : N3880-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

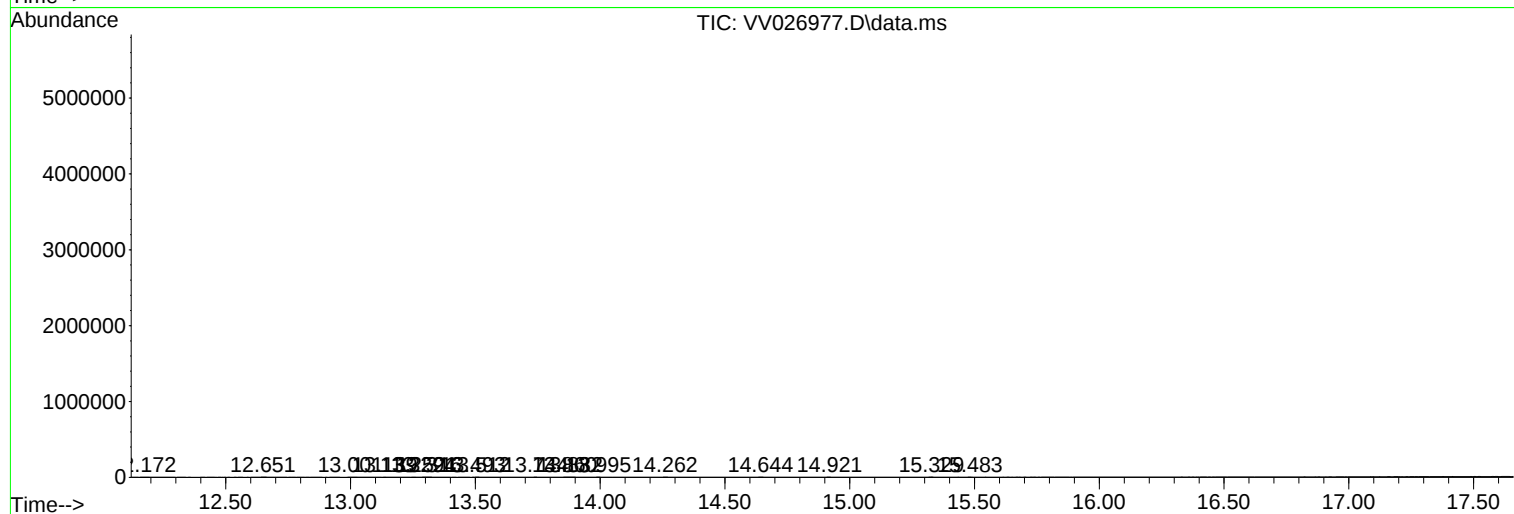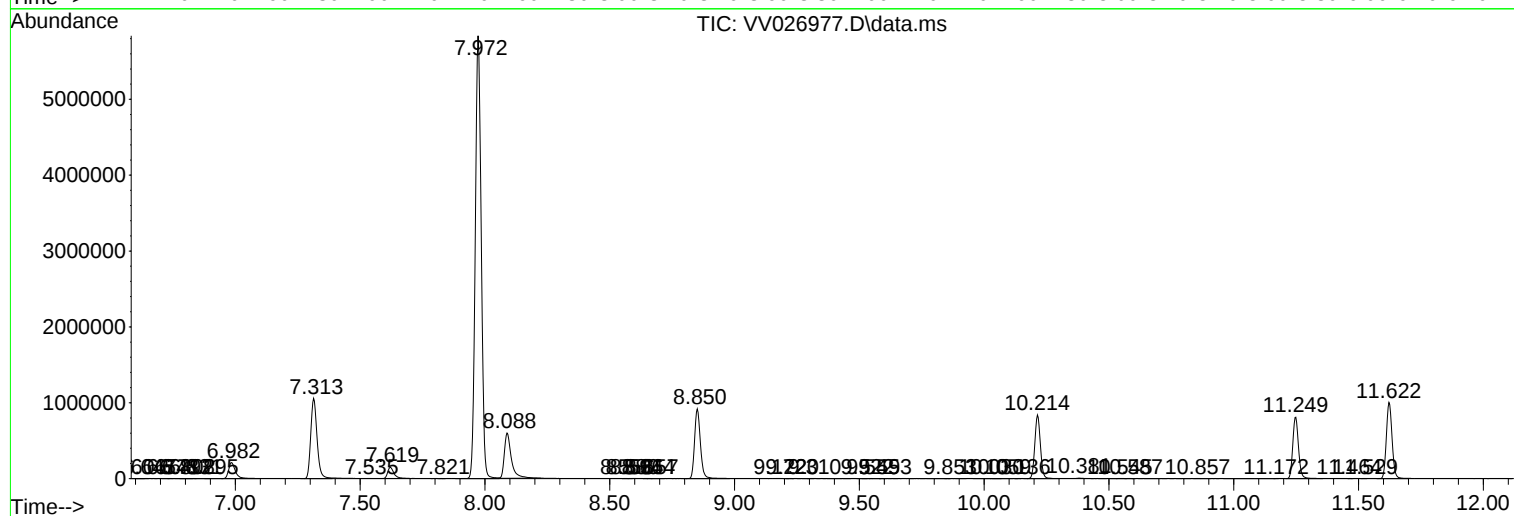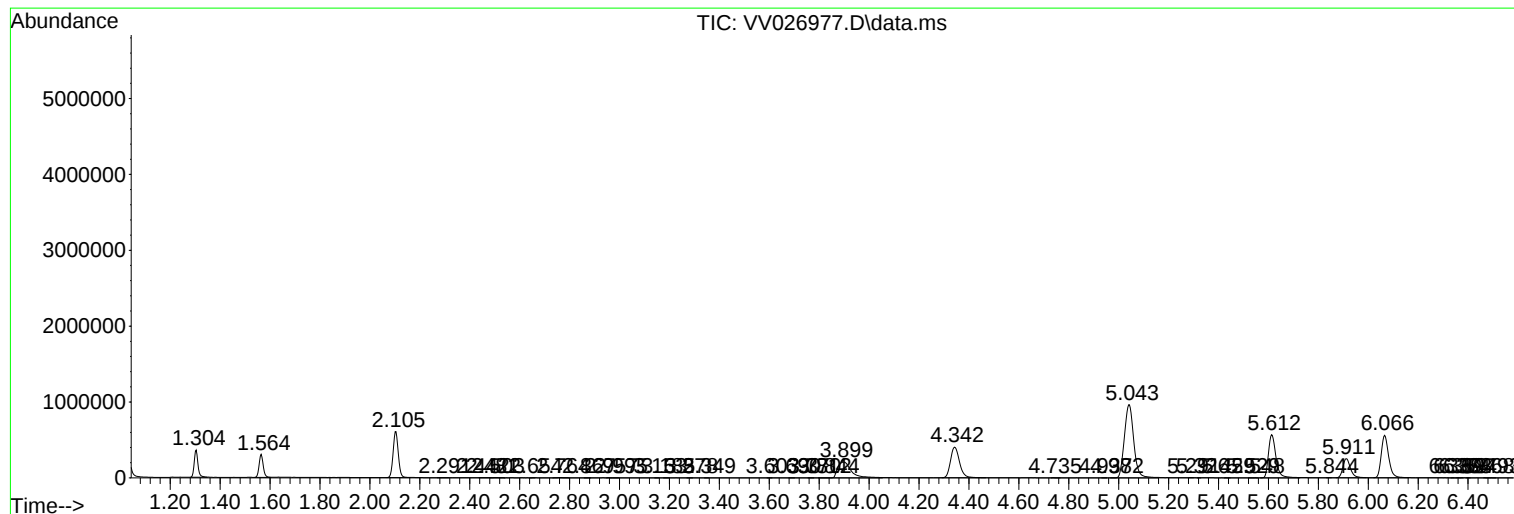

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026977.D
Acq On : 27 Jul 2022 02:07
Operator : SY/MD
Sample : N3880-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026977.D
Acq On : 27 Jul 2022 02:07
Operator : SY/MD
Sample : N3880-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------