

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026978.D
 Acq On : 27 Jul 2022 02:32
 Operator : SY/MD
 Sample : N3880-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	104	rVB	336567	354697	2.08%	0.959%
2	1.565	155	163	174	rBV	300492	334343	1.96%	0.904%
3	2.101	320	330	347	rBV	548059	790112	4.64%	2.137%
4	2.291	382	389	401	rBV3	1793	3182	0.02%	0.009%
5	2.471	442	445	447	rBV2	718	445	0.00%	0.001%
6	2.507	447	456	467	rVB4	6860	11983	0.07%	0.032%
7	2.555	467	471	474	rVB4	584	478	0.00%	0.001%
8	2.671	503	507	511	rBV3	655	679	0.00%	0.002%
9	2.757	526	534	547	rVB6	2363	4455	0.03%	0.012%
10	3.111	637	644	646	rBV2	318	325	0.00%	0.001%
11	3.372	722	725	729	rBV2	381	343	0.00%	0.001%
12	3.552	777	781	784	rBV3	387	297	0.00%	0.001%
13	3.626	800	804	808	rVB	409	325	0.00%	0.001%
14	3.667	814	817	822	rVB2	355	261	0.00%	0.001%
15	3.703	824	828	831	rBV3	288	275	0.00%	0.001%
16	3.748	836	842	847	rVB2	351	422	0.00%	0.001%
17	3.902	874	890	938	rBV2	611116	1792279	10.53%	4.848%
18	4.343	1008	1027	1056	rBV	395482	979411	5.76%	2.649%
19	4.638	1116	1119	1122	rBV4	395	258	0.00%	0.001%
20	4.796	1165	1168	1171	rBV2	544	311	0.00%	0.001%
21	4.851	1181	1185	1188	rBV	394	282	0.00%	0.001%
22	4.937	1209	1212	1214	rBV2	373	278	0.00%	0.001%
23	5.040	1224	1244	1290	rBV2	922199	2384799	14.02%	6.450%
24	5.613	1410	1422	1453	rBV	528769	1088607	6.40%	2.944%
25	5.854	1494	1497	1499	rVB2	638	366	0.00%	0.001%
26	5.908	1500	1514	1546	rBV	1248719	2462321	14.47%	6.660%
27	6.066	1550	1563	1590	rVV	536846	1096271	6.44%	2.965%
28	6.249	1617	1620	1625	rVB5	1252	923	0.01%	0.002%
29	6.291	1630	1633	1641	rVB6	824	995	0.01%	0.003%
30	6.326	1641	1644	1648	rVB5	817	645	0.00%	0.002%
31	6.352	1648	1652	1654	rBV4	640	527	0.00%	0.001%
32	6.387	1659	1663	1668	rBV3	556	507	0.00%	0.001%
33	6.519	1702	1704	1711	rVB2	472	475	0.00%	0.001%
34	6.558	1711	1716	1719	rBV3	336	319	0.00%	0.001%
35	6.616	1729	1734	1736	rBV3	663	471	0.00%	0.001%
36	6.648	1740	1744	1747	rVB4	637	494	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026978.D
 Acq On : 27 Jul 2022 02:32
 Operator : SY/MD
 Sample : N3880-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.780	1782	1785	1791	rVB2	418	381	0.00%	0.001%
38	6.818	1795	1797	1800	rVV2	403	255	0.00%	0.001%
39	6.834	1800	1802	1805	rVB2	649	320	0.00%	0.001%
40	6.854	1805	1808	1811	rBV	318	262	0.00%	0.001%
41	6.924	1823	1830	1835	rVB3	563	666	0.00%	0.002%
42	6.982	1835	1848	1872	rBV	200298	378073	2.22%	1.023%
43	7.166	1903	1905	1909	rVB4	499	278	0.00%	0.001%
44	7.313	1939	1951	1971	rBV	951637	1672599	9.83%	4.524%
45	7.619	2036	2046	2077	rBV	138316	254148	1.49%	0.687%
46	7.973	2134	2156	2182	rBV	10375371	17015018	100.00%	46.020%
47	8.088	2183	2192	2224	rVB	598132	1146647	6.74%	3.101%
48	8.561	2336	2339	2342	rBV3	555	384	0.00%	0.001%
49	8.600	2347	2351	2354	rVB4	322	263	0.00%	0.001%
50	8.629	2358	2360	2364	rVB4	743	406	0.00%	0.001%
51	8.654	2364	2368	2372	rBV3	792	782	0.00%	0.002%
52	8.680	2373	2376	2379	rBV3	394	271	0.00%	0.001%
53	8.850	2417	2429	2451	rBV	821999	1338619	7.87%	3.621%
54	9.143	2516	2520	2522	rBV5	1270	930	0.01%	0.003%
55	9.191	2532	2535	2538	rBV2	622	414	0.00%	0.001%
56	9.239	2547	2550	2553	rBV2	388	317	0.00%	0.001%
57	9.352	2581	2585	2589	rBV2	265	261	0.00%	0.001%
58	9.394	2595	2598	2600	rBV3	353	270	0.00%	0.001%
59	9.458	2615	2618	2622	rVB2	440	261	0.00%	0.001%
60	9.555	2642	2648	2651	rBV3	669	749	0.00%	0.002%
61	9.590	2655	2659	2663	rVB3	970	879	0.01%	0.002%
62	9.751	2706	2709	2713	rVB3	448	325	0.00%	0.001%
63	9.934	2759	2766	2775	rVB4	1083	1392	0.01%	0.004%
64	10.079	2808	2811	2815	rVB2	393	263	0.00%	0.001%
65	10.214	2838	2853	2879	rBV	804471	1267552	7.45%	3.428%
66	10.381	2897	2905	2914	rVB4	6280	10865	0.06%	0.029%
67	10.448	2924	2926	2930	rBV3	349	277	0.00%	0.001%
68	10.542	2951	2955	2957	rBV	593	427	0.00%	0.001%
69	10.577	2962	2966	2969	rBV4	341	270	0.00%	0.001%
70	10.622	2974	2980	2986	rBV3	312	450	0.00%	0.001%
71	10.805	3034	3037	3041	rBV2	438	278	0.00%	0.001%
72	10.854	3047	3052	3057	rVV5	668	767	0.00%	0.002%
73	10.953	3079	3083	3087	rBV3	328	337	0.00%	0.001%
74	11.188	3152	3156	3163	rBV3	500	573	0.00%	0.002%
75	11.246	3163	3174	3202	rBV	718363	1116784	6.56%	3.021%
76	11.371	3211	3213	3220	rVB5	993	794	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026978.D
 Acq On : 27 Jul 2022 02:32
 Operator : SY/MD
 Sample : N3880-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.484	3244	3248	3251	rBV3	352	316	0.00%	0.001%
78	11.545	3259	3267	3274	rBV7	2102	3038	0.02%	0.008%
79	11.622	3278	3291	3315	rBV	912146	1431472	8.41%	3.872%
80	11.853	3360	3363	3366	rBV2	520	357	0.00%	0.001%
81	11.882	3368	3372	3376	rBV2	368	395	0.00%	0.001%
82	12.107	3439	3442	3446	rVB3	617	436	0.00%	0.001%
83	12.133	3447	3450	3453	rBV2	398	258	0.00%	0.001%
84	12.236	3479	3482	3484	rBV2	469	371	0.00%	0.001%
85	12.458	3548	3551	3556	rVB2	566	545	0.00%	0.001%
86	12.487	3556	3560	3562	rBV2	542	408	0.00%	0.001%
87	12.516	3566	3569	3573	rBV2	584	439	0.00%	0.001%
88	12.738	3634	3638	3643	rVB3	582	566	0.00%	0.002%
89	12.915	3690	3693	3700	rBV	224	263	0.00%	0.001%
90	13.088	3742	3747	3751	rVB3	428	417	0.00%	0.001%
91	13.111	3751	3754	3758	rBV	317	281	0.00%	0.001%
92	13.159	3766	3769	3772	rVB2	477	308	0.00%	0.001%
93	13.355	3827	3830	3832	rBV2	549	306	0.00%	0.001%
94	13.516	3874	3880	3884	rBV4	1124	1440	0.01%	0.004%
95	13.744	3948	3951	3954	rVB3	411	275	0.00%	0.001%
96	13.805	3967	3970	3974	rBV3	477	382	0.00%	0.001%
97	14.072	4050	4053	4055	rBV2	379	270	0.00%	0.001%
98	14.098	4059	4061	4063	rBV2	450	269	0.00%	0.001%
99	14.175	4083	4085	4089	rBV	482	339	0.00%	0.001%
100	15.297	4429	4434	4444	rVB6	1632	1937	0.01%	0.005%




Sum of corrected areas: 36973056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026978.D
Acq On : 27 Jul 2022 02:32
Operator : SY/MD
Sample : N3880-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

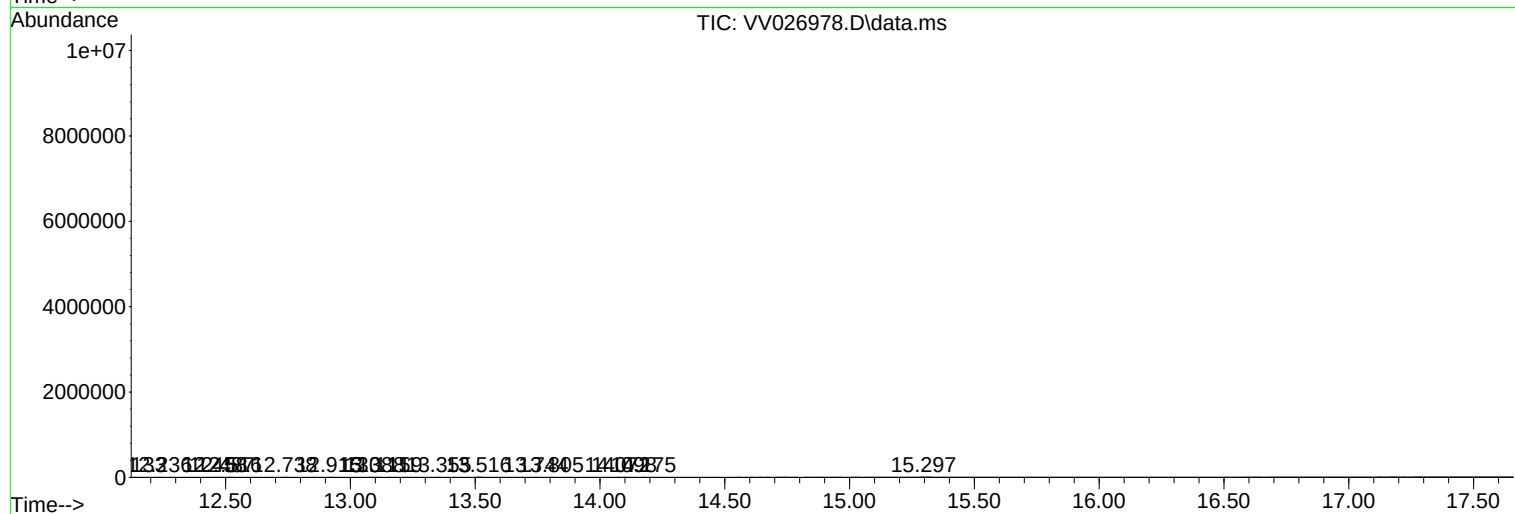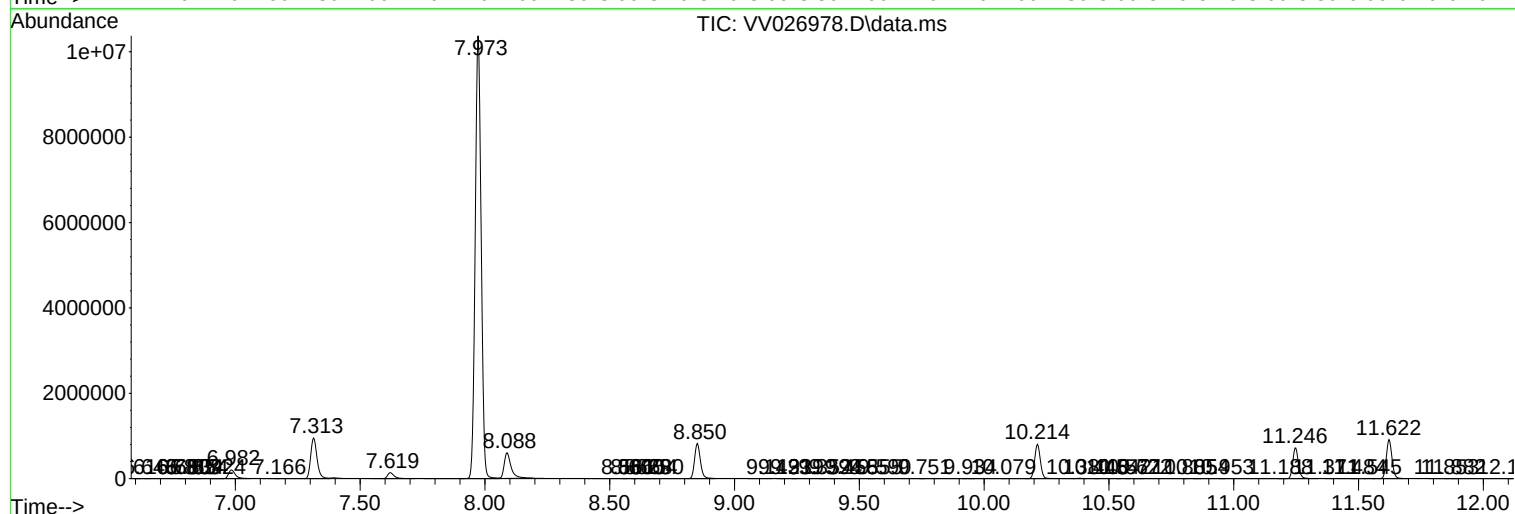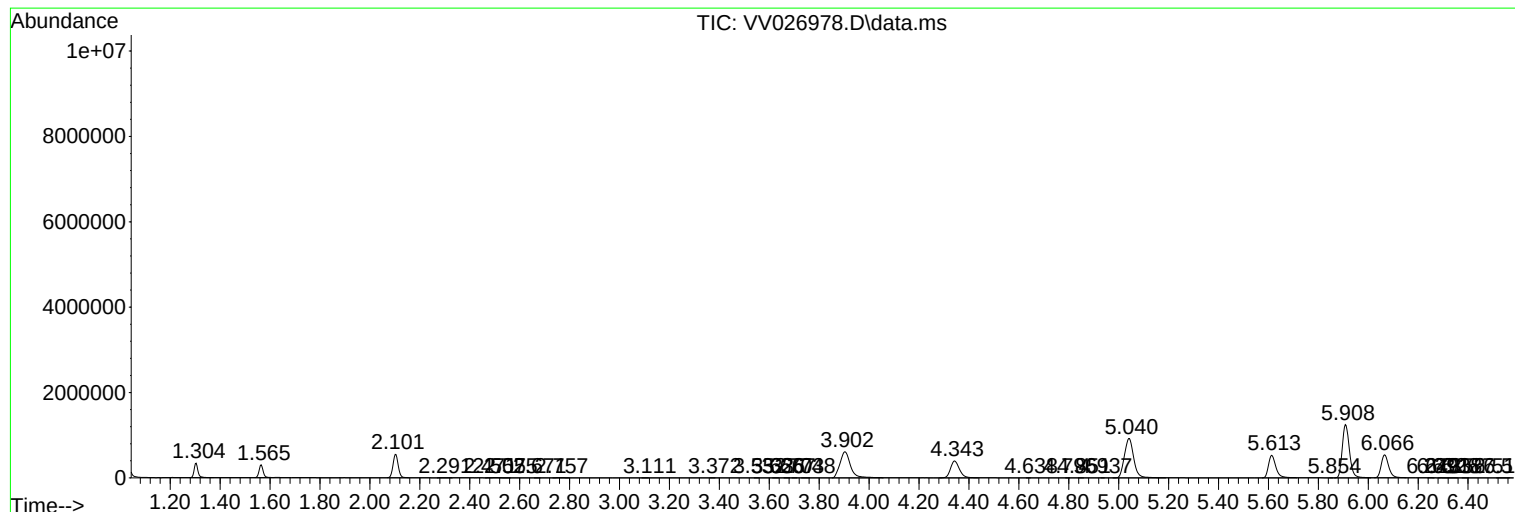

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026978.D
Acq On : 27 Jul 2022 02:32
Operator : SY/MD
Sample : N3880-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026978.D
Acq On : 27 Jul 2022 02:32
Operator : SY/MD
Sample : N3880-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------