

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026980.D
 Acq On : 27 Jul 2022 03:21
 Operator : SY/MD
 Sample : N3880-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	321619	338501	0.29%	0.248%
2	1.564	155	163	178	rBV	286562	324749	0.27%	0.238%
3	2.101	319	330	350	rBV	533720	770208	0.65%	0.564%
4	2.291	383	389	394	rBV4	1307	1779	0.00%	0.001%
5	2.320	396	398	401	rBV3	619	381	0.00%	0.000%
6	2.503	446	455	466	rVB2	8043	13071	0.01%	0.010%
7	2.609	484	488	492	rBV3	352	342	0.00%	0.000%
8	2.761	525	535	548	rVV2	10869	19610	0.02%	0.014%
9	3.044	620	623	630	rVB3	353	311	0.00%	0.000%
10	3.182	663	666	669	rBV2	320	255	0.00%	0.000%
11	3.211	673	675	680	rVB3	571	389	0.00%	0.000%
12	3.458	749	752	756	rBV2	339	299	0.00%	0.000%
13	3.632	801	806	809	rBV2	351	327	0.00%	0.000%
14	3.690	819	824	827	rVB2	565	376	0.00%	0.000%
15	3.905	874	891	938	rBV2	751060	2112566	1.78%	1.547%
16	4.236	991	994	997	rBV3	589	329	0.00%	0.000%
17	4.342	1010	1027	1067	rBV	393655	987285	0.83%	0.723%
18	4.715	1140	1143	1146	rVB3	407	274	0.00%	0.000%
19	4.744	1146	1152	1156	rBV4	462	514	0.00%	0.000%
20	4.783	1161	1164	1167	rBV3	289	242	0.00%	0.000%
21	4.831	1175	1179	1184	rBV4	296	332	0.00%	0.000%
22	4.912	1196	1204	1205	rBV	376	380	0.00%	0.000%
23	4.918	1205	1206	1210	rVB2	495	256	0.00%	0.000%
24	4.953	1214	1217	1223	rVB3	398	363	0.00%	0.000%
25	5.043	1227	1245	1280	rBV2	904517	2344810	1.98%	1.717%
26	5.326	1330	1333	1337	rVB3	817	593	0.00%	0.000%
27	5.349	1337	1340	1346	rBV2	409	393	0.00%	0.000%
28	5.413	1355	1360	1362	rBV4	306	239	0.00%	0.000%
29	5.613	1408	1422	1455	rBV	507794	1050767	0.89%	0.769%
30	5.828	1487	1489	1496	rVB5	923	681	0.00%	0.000%
31	5.912	1500	1515	1543	rBV	300486	611159	0.52%	0.447%
32	6.066	1549	1563	1591	rBV	530658	1078226	0.91%	0.789%
33	6.346	1648	1650	1652	rVB3	505	243	0.00%	0.000%
34	6.362	1652	1655	1656	rBV2	550	300	0.00%	0.000%
35	6.571	1715	1720	1724	rBV4	556	480	0.00%	0.000%
36	6.664	1745	1749	1754	rBV4	452	536	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026980.D
 Acq On : 27 Jul 2022 03:21
 Operator : SY/MD
 Sample : N3880-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.776	1779	1784	1789	rBV4	517	567	0.00%	0.000%
38	6.883	1814	1817	1823	rBV2	367	412	0.00%	0.000%
39	6.940	1830	1835	1837	rBV3	309	252	0.00%	0.000%
40	6.985	1837	1849	1882	rBV	194297	374883	0.32%	0.274%
41	7.204	1912	1917	1918	rBV3	416	372	0.00%	0.000%
42	7.313	1940	1951	1971	rBV	925445	1602870	1.35%	1.174%
43	7.622	2035	2047	2069	rBV	143751	257538	0.22%	0.189%
44	7.780	2093	2096	2098	rVB4	643	379	0.00%	0.000%
45	7.847	2110	2117	2127	rVB5	2911	4922	0.00%	0.004%
46	7.905	2130	2135	2136	rBV3	563	365	0.00%	0.000%
47	7.982	2138	2159	2183	rBV2	63018924	118455650	100.00%	86.728%
48	8.088	2184	2192	2229	rVB	633387	1246554	1.05%	0.913%
49	8.789	2407	2410	2412	rBV2	351	248	0.00%	0.000%
50	8.850	2417	2429	2456	rBV	774433	1275248	1.08%	0.934%
51	8.973	2461	2467	2480	rVB4	10689	18758	0.02%	0.014%
52	9.182	2530	2532	2535	rVB	729	300	0.00%	0.000%
53	9.410	2600	2603	2605	rBV2	504	307	0.00%	0.000%
54	9.516	2632	2636	2639	rBV2	389	335	0.00%	0.000%
55	9.638	2670	2674	2678	rVV4	379	382	0.00%	0.000%
56	9.718	2696	2699	2705	rVB3	693	608	0.00%	0.000%
57	9.751	2705	2709	2711	rBV3	345	269	0.00%	0.000%
58	9.825	2725	2732	2734	rBV3	515	622	0.00%	0.000%
59	9.937	2763	2767	2771	rBV3	450	500	0.00%	0.000%
60	10.011	2785	2790	2796	rBV3	524	710	0.00%	0.001%
61	10.040	2796	2799	2803	rVV2	414	324	0.00%	0.000%
62	10.095	2814	2816	2819	rBV2	689	296	0.00%	0.000%
63	10.214	2840	2853	2875	rBV	791515	1238184	1.05%	0.907%
64	10.384	2898	2906	2915	rVB3	5793	9029	0.01%	0.007%
65	10.464	2928	2931	2936	rVB3	607	574	0.00%	0.000%
66	10.580	2964	2967	2968	rBV	466	287	0.00%	0.000%
67	10.641	2982	2986	2988	rBV2	428	260	0.00%	0.000%
68	10.693	3000	3002	3009	rVB2	474	442	0.00%	0.000%
69	10.792	3030	3033	3037	rVB4	375	241	0.00%	0.000%
70	10.921	3070	3073	3076	rVB4	392	249	0.00%	0.000%
71	11.037	3105	3109	3111	rBV3	315	256	0.00%	0.000%
72	11.165	3145	3149	3151	rBV3	439	302	0.00%	0.000%
73	11.191	3154	3157	3162	rBV3	412	306	0.00%	0.000%
74	11.249	3162	3175	3202	rBV	673794	1055671	0.89%	0.773%
75	11.490	3248	3250	3256	rBV3	419	318	0.00%	0.000%
76	11.545	3264	3267	3268	rBV	550	324	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026980.D
 Acq On : 27 Jul 2022 03:21
 Operator : SY/MD
 Sample : N3880-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.577	3274	3277	3279	rBV3	588	356	0.00%	0.000%
78	11.622	3279	3291	3309	rBV	863663	1360498	1.15%	0.996%
79	12.062	3425	3428	3430	rVV2	418	249	0.00%	0.000%
80	12.143	3450	3453	3456	rBV2	376	257	0.00%	0.000%
81	12.246	3477	3485	3491	rBV6	1029	1625	0.00%	0.001%
82	12.381	3524	3527	3530	rBV	450	289	0.00%	0.000%
83	12.400	3530	3533	3538	rVV3	479	436	0.00%	0.000%
84	12.426	3538	3541	3546	rVV3	331	281	0.00%	0.000%
85	12.542	3574	3577	3582	rBV3	417	475	0.00%	0.000%
86	12.651	3606	3611	3613	rBV2	517	415	0.00%	0.000%
87	12.709	3624	3629	3633	rBV2	647	669	0.00%	0.000%
88	12.834	3665	3668	3670	rBV2	324	239	0.00%	0.000%
89	12.876	3678	3681	3686	rVB2	405	295	0.00%	0.000%
90	12.966	3706	3709	3711	rBV2	618	378	0.00%	0.000%
91	13.281	3803	3807	3809	rBV2	604	518	0.00%	0.000%
92	13.480	3865	3869	3871	rBV	564	390	0.00%	0.000%
93	13.786	3960	3964	3973	rVB3	764	1069	0.00%	0.001%
94	13.969	4018	4021	4024	rBV3	383	249	0.00%	0.000%
95	14.242	4102	4106	4108	rBV2	502	459	0.00%	0.000%
96	14.394	4150	4153	4157	rVB	679	535	0.00%	0.000%
97	14.416	4157	4160	4162	rVV4	411	278	0.00%	0.000%
98	14.442	4165	4168	4172	rVB3	472	424	0.00%	0.000%
99	14.799	4277	4279	4282	rVB2	622	281	0.00%	0.000%
100	15.181	4396	4398	4404	rVB5	842	617	0.00%	0.000%




Sum of corrected areas: 136582962

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026980.D
Acq On : 27 Jul 2022 03:21
Operator : SY/MD
Sample : N3880-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

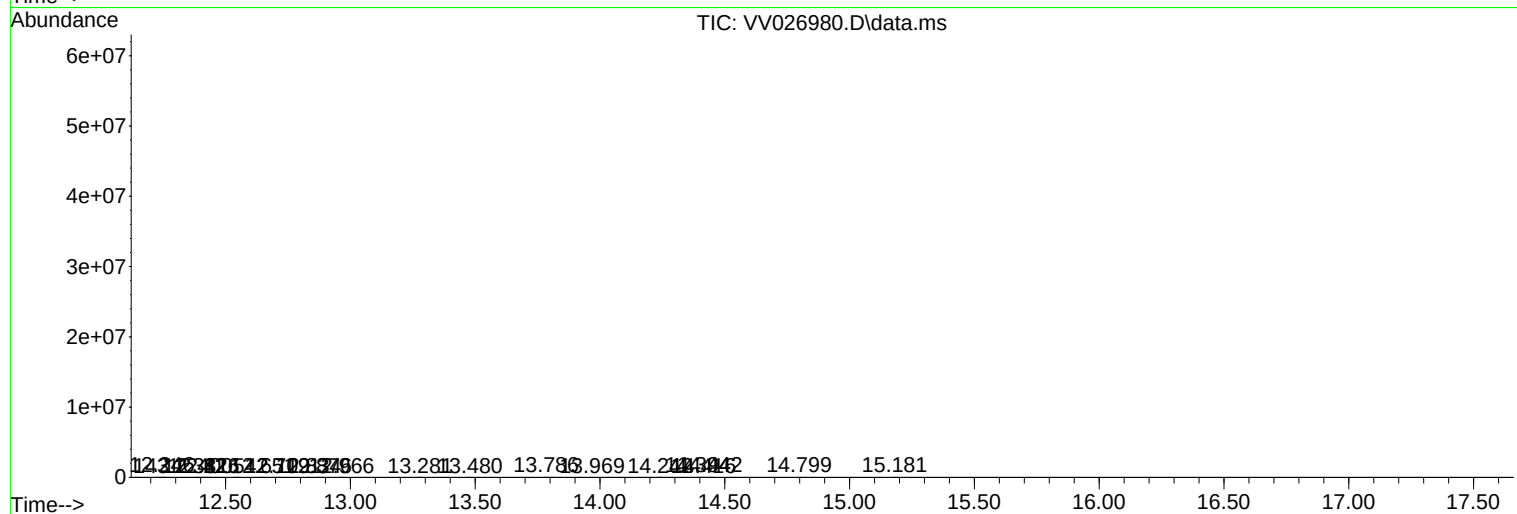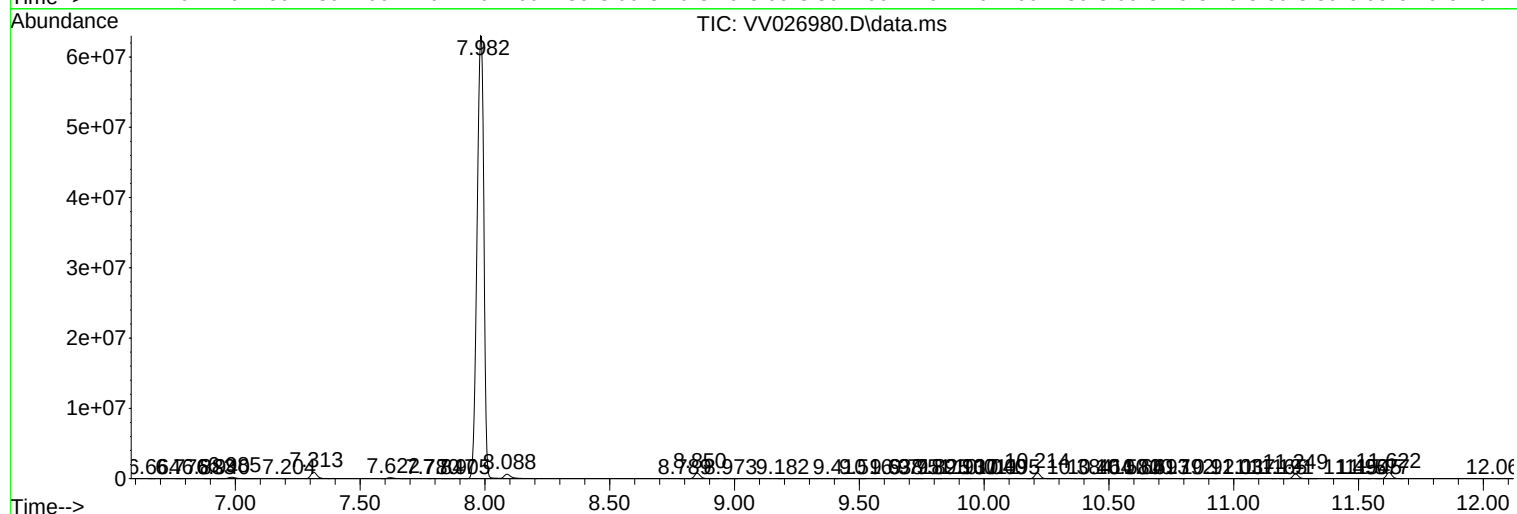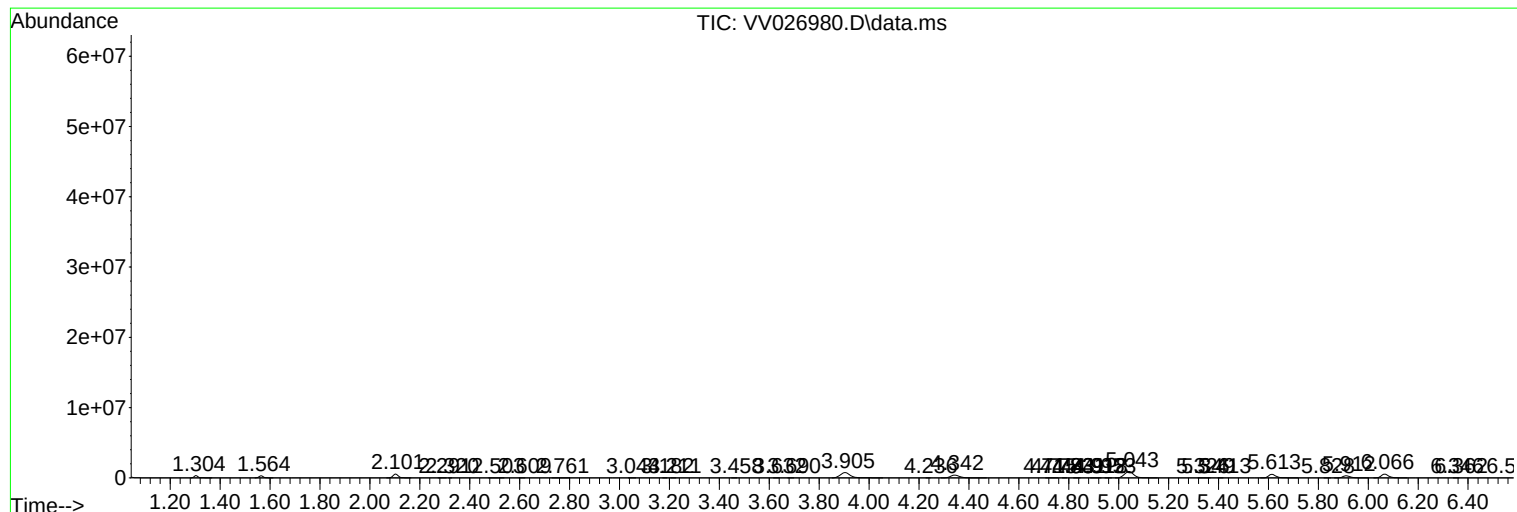

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026980.D
Acq On : 27 Jul 2022 03:21
Operator : SY/MD
Sample : N3880-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026980.D
Acq On : 27 Jul 2022 03:21
Operator : SY/MD
Sample : N3880-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
