

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026981.D
 Acq On : 27 Jul 2022 03:45
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	355941	370619	8.51%	1.487%
2	1.564	155	163	176	rBV	303093	340908	7.82%	1.368%
3	2.105	320	331	345	rBV	604817	869484	19.96%	3.488%
4	2.288	384	388	398	rVB4	1406	1808	0.04%	0.007%
5	2.561	471	473	479	rVB5	367	322	0.01%	0.001%
6	2.590	480	482	487	rBV2	372	310	0.01%	0.001%
7	2.715	514	521	524	rBV6	548	713	0.02%	0.003%
8	2.764	527	536	547	rVB5	4808	9239	0.21%	0.037%
9	2.815	547	552	558	rVB4	513	565	0.01%	0.002%
10	2.957	591	596	607	rBV3	508	636	0.01%	0.003%
11	3.008	608	612	615	rBV4	363	312	0.01%	0.001%
12	3.031	617	619	623	rVV2	681	431	0.01%	0.002%
13	3.532	770	775	782	rVB3	340	513	0.01%	0.002%
14	3.905	874	891	935	rBV2	1180339	3153580	72.38%	12.652%
15	4.246	995	997	1001	rVB2	690	429	0.01%	0.002%
16	4.268	1001	1004	1007	rBV3	614	474	0.01%	0.002%
17	4.342	1010	1027	1054	rBV	407266	1011017	23.21%	4.056%
18	4.609	1108	1110	1113	rVB3	657	376	0.01%	0.002%
19	4.809	1165	1172	1174	rBV4	525	572	0.01%	0.002%
20	4.889	1194	1197	1202	rBV5	383	357	0.01%	0.001%
21	5.043	1227	1245	1283	rBV2	962950	2492756	57.22%	10.001%
22	5.307	1324	1327	1332	rVB3	376	314	0.01%	0.001%
23	5.410	1357	1359	1364	rVB2	394	284	0.01%	0.001%
24	5.500	1381	1387	1391	rBV5	820	1050	0.02%	0.004%
25	5.561	1404	1406	1410	rVB3	629	445	0.01%	0.002%
26	5.612	1410	1422	1459	rBV	574308	1182650	27.14%	4.745%
27	5.789	1475	1477	1479	rVB2	1057	478	0.01%	0.002%
28	5.844	1491	1494	1498	rVB4	799	548	0.01%	0.002%
29	5.863	1498	1500	1502	rBV3	542	287	0.01%	0.001%
30	5.911	1502	1515	1544	rVV	342367	707121	16.23%	2.837%
31	6.066	1549	1563	1592	rBV	555132	1131885	25.98%	4.541%
32	6.194	1601	1603	1604	rBV2	719	352	0.01%	0.001%
33	6.336	1645	1647	1650	rBV2	365	284	0.01%	0.001%
34	6.371	1655	1658	1661	rBV2	432	379	0.01%	0.002%
35	6.477	1688	1691	1696	rVB2	314	276	0.01%	0.001%
36	6.654	1742	1746	1749	rBV3	593	578	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026981.D
 Acq On : 27 Jul 2022 03:45
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.744	1770	1774	1778	rVB2	733	448	0.01%	0.002%
38	6.799	1788	1791	1793	rBV	357	290	0.01%	0.001%
39	6.982	1834	1848	1885	rBV	208987	400169	9.18%	1.605%
40	7.214	1916	1920	1926	rBV6	555	555	0.01%	0.002%
41	7.313	1939	1951	1969	rBV	1065781	1840396	42.24%	7.384%
42	7.529	2016	2018	2024	rVB5	1074	851	0.02%	0.003%
43	7.619	2035	2046	2070	rBV	150545	270374	6.21%	1.085%
44	7.815	2105	2107	2110	rVB2	596	294	0.01%	0.001%
45	7.847	2110	2117	2121	rVB5	794	936	0.02%	0.004%
46	7.873	2121	2125	2129	rVB2	580	405	0.01%	0.002%
47	7.972	2137	2156	2182	rBV	2617282	4356796	100.00%	17.479%
48	8.088	2182	2192	2228	rVB	575611	1107037	25.41%	4.441%
49	8.542	2330	2333	2335	rBV2	407	315	0.01%	0.001%
50	8.738	2389	2394	2397	rVB3	407	386	0.01%	0.002%
51	8.792	2405	2411	2414	rBV4	761	775	0.02%	0.003%
52	8.850	2417	2429	2454	rBV	916835	1485740	34.10%	5.961%
53	9.152	2518	2523	2528	rBV6	1150	1269	0.03%	0.005%
54	9.259	2552	2556	2558	rBV3	670	364	0.01%	0.001%
55	9.342	2578	2582	2585	rBV3	363	269	0.01%	0.001%
56	9.410	2599	2603	2608	rBV3	654	515	0.01%	0.002%
57	9.554	2642	2648	2653	rBV6	907	1192	0.03%	0.005%
58	9.760	2710	2712	2718	rVB2	555	390	0.01%	0.002%
59	9.799	2718	2724	2728	rBV4	431	373	0.01%	0.001%
60	9.934	2763	2766	2770	rBV4	644	634	0.01%	0.003%
61	10.027	2792	2795	2800	rVB2	541	425	0.01%	0.002%
62	10.120	2821	2824	2829	rBV4	341	327	0.01%	0.001%
63	10.214	2839	2853	2878	rBV	829822	1294078	29.70%	5.192%
64	10.381	2897	2905	2916	rVB3	7217	11237	0.26%	0.045%
65	10.545	2953	2956	2962	rVB3	691	603	0.01%	0.002%
66	10.667	2991	2994	3000	rBV4	335	294	0.01%	0.001%
67	10.722	3006	3011	3018	rVV3	550	420	0.01%	0.002%
68	10.860	3051	3054	3058	rVB4	522	364	0.01%	0.001%
69	10.914	3069	3071	3073	rBV	458	303	0.01%	0.001%
70	11.175	3149	3152	3157	rBV3	401	416	0.01%	0.002%
71	11.246	3162	3174	3198	rBV	811852	1259717	28.91%	5.054%
72	11.445	3232	3236	3238	rBV3	437	350	0.01%	0.001%
73	11.484	3246	3248	3254	rVB4	778	694	0.02%	0.003%
74	11.512	3254	3257	3259	rBV2	473	379	0.01%	0.002%
75	11.541	3259	3266	3275	rVV5	3000	4995	0.11%	0.020%
76	11.622	3279	3291	3318	rBV	1016514	1587208	36.43%	6.368%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026981.D
 Acq On : 27 Jul 2022 03:45
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.815	3348	3351	3354	rVB3	606	332	0.01%	0.001%
78	11.866	3363	3367	3371	rVB3	469	452	0.01%	0.002%
79	11.889	3371	3374	3376	rBV3	443	308	0.01%	0.001%
80	11.905	3376	3379	3383	rVB3	608	367	0.01%	0.001%
81	12.111	3441	3443	3451	rVB3	401	370	0.01%	0.001%
82	12.230	3477	3480	3483	rBV	465	380	0.01%	0.002%
83	12.966	3706	3709	3715	rVB	436	353	0.01%	0.001%
84	13.040	3728	3732	3733	rBV2	445	293	0.01%	0.001%
85	13.278	3798	3806	3808	rBV5	516	665	0.02%	0.003%
86	13.303	3813	3814	3819	rBV3	546	341	0.01%	0.001%
87	13.355	3827	3830	3832	rBV2	457	280	0.01%	0.001%
88	13.406	3844	3846	3851	rVB2	444	350	0.01%	0.001%
89	13.435	3851	3855	3858	rBV	425	465	0.01%	0.002%
90	13.635	3914	3917	3919	rBV	342	287	0.01%	0.001%
91	13.853	3981	3985	3987	rBV4	372	370	0.01%	0.001%
92	13.895	3995	3998	4001	rBV	591	386	0.01%	0.002%
93	14.020	4033	4037	4040	rBV3	647	444	0.01%	0.002%
94	14.069	4050	4052	4058	rVB3	326	302	0.01%	0.001%
95	14.101	4058	4062	4068	rBV3	550	764	0.02%	0.003%
96	14.236	4098	4104	4105	rBV2	618	527	0.01%	0.002%
97	14.316	4127	4129	4134	rBV2	374	299	0.01%	0.001%
98	14.599	4215	4217	4220	rBV2	539	310	0.01%	0.001%
99	14.715	4251	4253	4256	rBV2	580	408	0.01%	0.002%
100	15.233	4409	4414	4419	rBV6	874	1329	0.03%	0.005%




Sum of corrected areas: 24925317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026981.D
Acq On : 27 Jul 2022 03:45
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

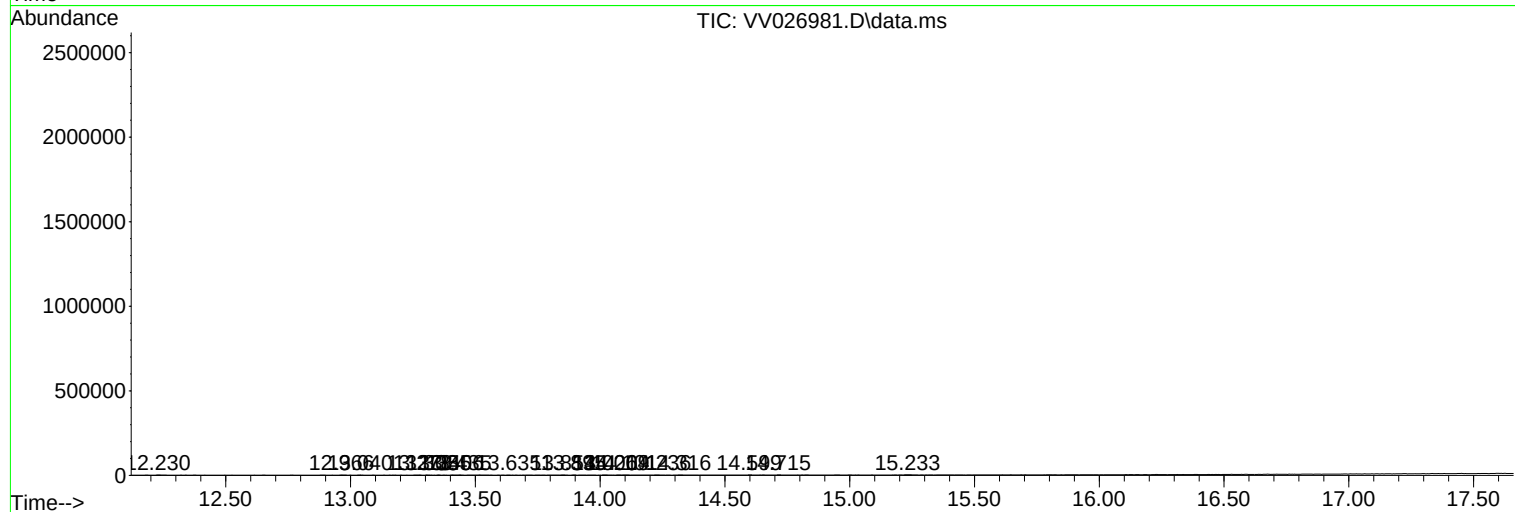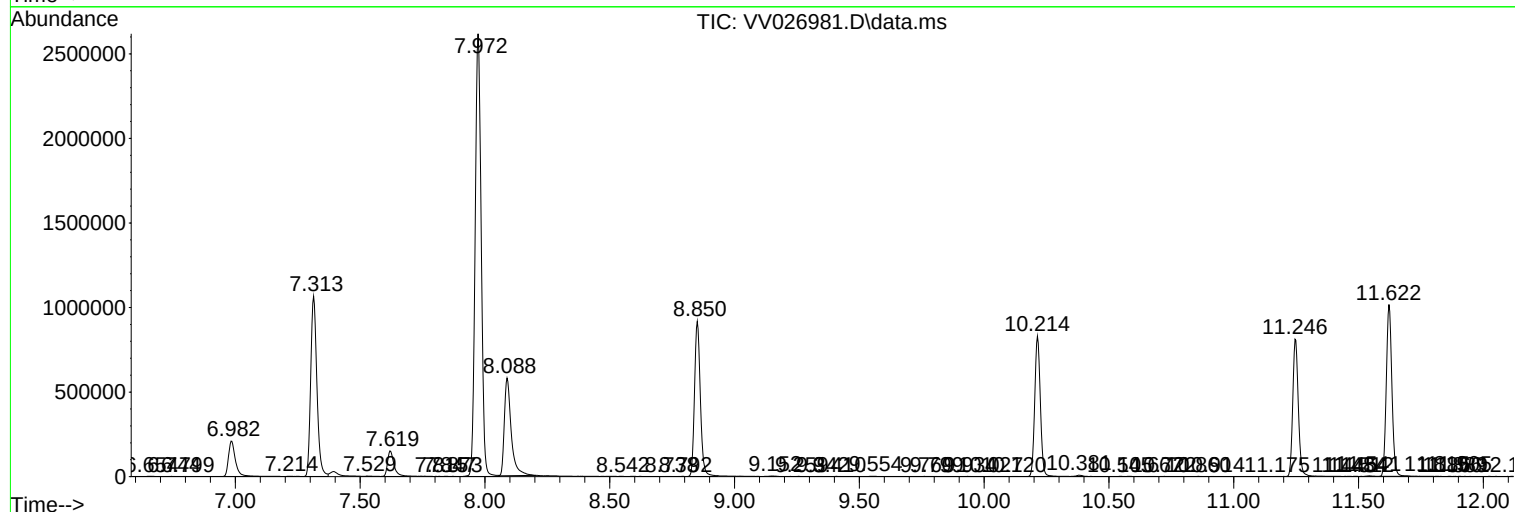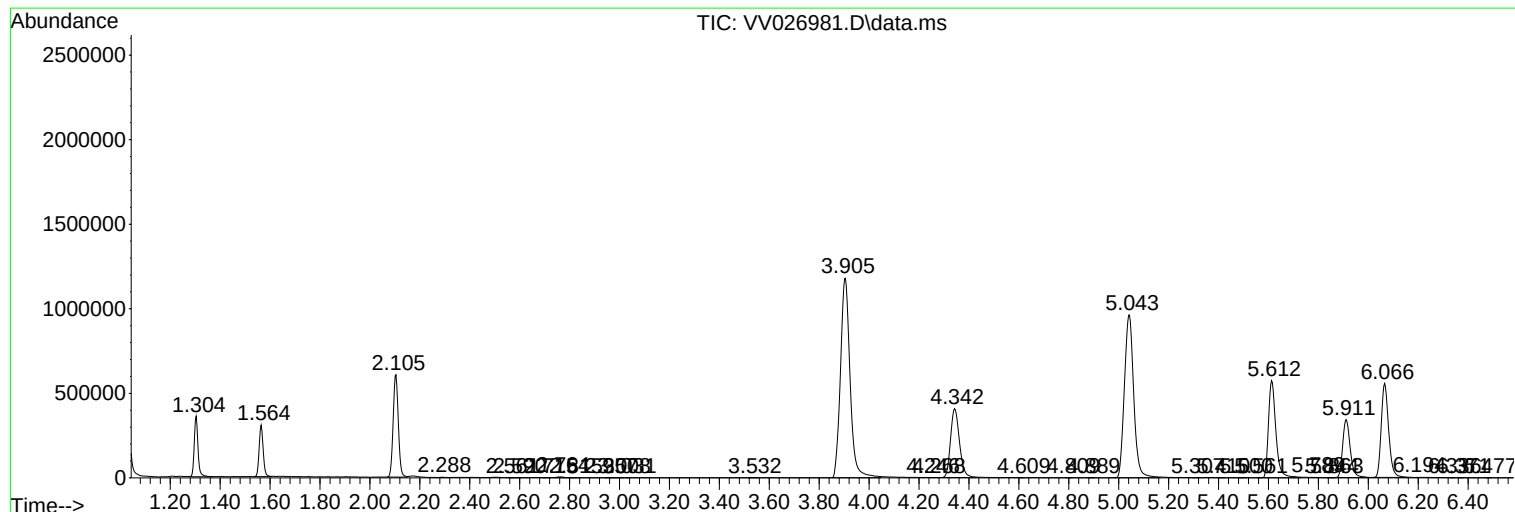

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026981.D
Acq On : 27 Jul 2022 03:45
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026981.D
Acq On : 27 Jul 2022 03:45
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc