

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026982.D
 Acq On : 27 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3880-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	106	rVB	362811	373559	3.83%	0.876%
2	1.565	155	163	176	rBV	300536	338960	3.48%	0.795%
3	2.105	320	331	347	rBV	579184	835808	8.57%	1.959%
4	2.294	384	390	398	rVB2	1335	1634	0.02%	0.004%
5	2.507	448	456	466	rVB4	4516	7335	0.08%	0.017%
6	2.561	470	473	480	rVB5	718	788	0.01%	0.002%
7	2.616	487	490	495	rBV3	521	458	0.00%	0.001%
8	2.690	512	513	519	rVB4	512	328	0.00%	0.001%
9	2.757	527	534	548	rVB5	5686	10523	0.11%	0.025%
10	2.960	595	597	602	rVV3	281	233	0.00%	0.001%
11	3.124	645	648	651	rVB	479	296	0.00%	0.001%
12	3.163	657	660	663	rBV2	331	217	0.00%	0.001%
13	3.182	663	666	670	rBV2	446	321	0.00%	0.001%
14	3.246	684	686	691	rVB3	342	274	0.00%	0.001%
15	3.281	691	697	698	rBV	597	477	0.00%	0.001%
16	3.468	749	755	758	rBV2	295	308	0.00%	0.001%
17	3.577	786	789	794	rVB2	461	411	0.00%	0.001%
18	3.902	872	890	945	rBV	4000295	9748296	100.00%	22.853%
19	4.343	1011	1027	1066	rVB	399878	988092	10.14%	2.316%
20	4.558	1092	1094	1097	rVB3	690	379	0.00%	0.001%
21	4.609	1108	1110	1111	rBV	431	237	0.00%	0.001%
22	4.690	1129	1135	1141	rBV5	514	716	0.01%	0.002%
23	4.744	1149	1152	1157	rVB5	665	611	0.01%	0.001%
24	4.770	1157	1160	1162	rVB2	671	372	0.00%	0.001%
25	4.796	1162	1168	1174	rBV4	658	924	0.01%	0.002%
26	4.828	1174	1178	1180	rBV2	452	316	0.00%	0.001%
27	5.040	1226	1244	1279	rBV2	934887	2419453	24.82%	5.672%
28	5.256	1309	1311	1315	rVB3	860	539	0.01%	0.001%
29	5.490	1382	1384	1387	rBV2	362	265	0.00%	0.001%
30	5.526	1392	1395	1397	rBV2	633	307	0.00%	0.001%
31	5.613	1410	1422	1450	rBV	537642	1105475	11.34%	2.592%
32	5.860	1497	1499	1500	rBV2	688	338	0.00%	0.001%
33	5.908	1500	1514	1549	rVV	4187314	8072365	82.81%	18.924%
34	6.066	1551	1563	1589	rVB	552298	1121781	11.51%	2.630%
35	6.362	1653	1655	1657	rBV3	755	344	0.00%	0.001%
36	6.426	1673	1675	1676	rBV2	652	217	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026982.D
 Acq On : 27 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3880-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.468	1684	1688	1689	rBV2	370	244	0.00%	0.001%
38	6.539	1706	1710	1713	rBV2	740	496	0.01%	0.001%
39	6.654	1744	1746	1749	rVV3	441	243	0.00%	0.001%
40	6.680	1749	1754	1757	rVV3	453	477	0.00%	0.001%
41	6.722	1762	1767	1770	rBV4	535	552	0.01%	0.001%
42	6.915	1825	1827	1833	rVB2	481	440	0.00%	0.001%
43	6.982	1833	1848	1880	rBV	205814	389340	3.99%	0.913%
44	7.214	1917	1920	1924	rBV3	401	379	0.00%	0.001%
45	7.313	1939	1951	1977	rBV	970522	1713879	17.58%	4.018%
46	7.619	2036	2046	2070	rBV	146207	261278	2.68%	0.613%
47	7.821	2106	2109	2112	rVB2	553	402	0.00%	0.001%
48	7.863	2121	2122	2126	rVB2	552	234	0.00%	0.001%
49	7.886	2126	2129	2131	rBV	557	399	0.00%	0.001%
50	7.973	2137	2156	2182	rBV	5484970	8975697	92.07%	21.041%
51	8.088	2183	2192	2223	rVB	565997	1090341	11.18%	2.556%
52	8.635	2360	2362	2367	rVB4	518	398	0.00%	0.001%
53	8.850	2417	2429	2461	rBV	828544	1354748	13.90%	3.176%
54	9.146	2516	2521	2522	rBV4	675	631	0.01%	0.001%
55	9.326	2574	2577	2579	rBV2	320	258	0.00%	0.001%
56	9.391	2594	2597	2599	rVB3	408	219	0.00%	0.001%
57	9.542	2641	2644	2645	rBV	466	244	0.00%	0.001%
58	9.863	2741	2744	2746	rBV2	402	268	0.00%	0.001%
59	9.899	2749	2755	2757	rVB2	414	390	0.00%	0.001%
60	9.931	2761	2765	2767	rBV2	389	313	0.00%	0.001%
61	10.117	2820	2823	2827	rVB2	456	328	0.00%	0.001%
62	10.146	2828	2832	2833	rBV	346	248	0.00%	0.001%
63	10.214	2841	2853	2874	rBV	804435	1270057	13.03%	2.977%
64	10.381	2896	2905	2916	rVB3	5092	8344	0.09%	0.020%
65	10.513	2938	2946	2949	rBV4	368	486	0.00%	0.001%
66	10.580	2963	2967	2969	rBV3	695	600	0.01%	0.001%
67	10.657	2988	2991	2994	rVV2	316	254	0.00%	0.001%
68	10.850	3046	3051	3056	rBV5	1154	1012	0.01%	0.002%
69	10.918	3068	3072	3074	rBV3	449	330	0.00%	0.001%
70	10.976	3085	3090	3093	rVV2	293	271	0.00%	0.001%
71	11.185	3153	3155	3158	rBV3	323	256	0.00%	0.001%
72	11.246	3163	3174	3203	rBV	707544	1104582	11.33%	2.589%
73	11.516	3255	3258	3263	rVB2	471	416	0.00%	0.001%
74	11.545	3263	3267	3272	rBV4	677	793	0.01%	0.002%
75	11.622	3279	3291	3317	rBV	920029	1435070	14.72%	3.364%
76	11.950	3390	3393	3396	rVV3	275	208	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026982.D
 Acq On : 27 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3880-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.037	3417	3420	3424	rBV3	468	377	0.00%	0.001%
78	12.085	3431	3435	3439	rBV2	388	414	0.00%	0.001%
79	12.397	3530	3532	3538	rVB4	311	269	0.00%	0.001%
80	12.654	3609	3612	3616	rBV3	590	396	0.00%	0.001%
81	12.734	3631	3637	3641	rBV4	415	520	0.01%	0.001%
82	12.754	3641	3643	3648	rVV3	433	306	0.00%	0.001%
83	12.866	3674	3678	3680	rBV2	586	311	0.00%	0.001%
84	12.940	3698	3701	3702	rBV2	423	254	0.00%	0.001%
85	13.069	3738	3741	3743	rBV3	333	243	0.00%	0.001%
86	13.181	3774	3776	3779	rBV	419	219	0.00%	0.001%
87	13.249	3795	3797	3799	rBV	475	271	0.00%	0.001%
88	13.419	3845	3850	3853	rBV3	508	511	0.01%	0.001%
89	13.786	3961	3964	3970	rBV4	512	596	0.01%	0.001%
90	13.876	3989	3992	3995	rBV2	509	460	0.00%	0.001%
91	13.924	4004	4007	4014	rVB3	522	496	0.01%	0.001%
92	14.056	4045	4048	4051	rBV2	495	364	0.00%	0.001%
93	14.072	4051	4053	4056	rVB2	591	302	0.00%	0.001%
94	14.165	4078	4082	4085	rBV3	465	424	0.00%	0.001%
95	14.522	4191	4193	4197	rBV2	435	332	0.00%	0.001%
96	14.773	4268	4271	4275	rBV4	679	411	0.00%	0.001%
97	14.905	4310	4312	4314	rBV2	651	325	0.00%	0.001%
98	15.030	4348	4351	4352	rBV3	680	398	0.00%	0.001%
99	15.217	4407	4409	4413	rBV4	608	515	0.01%	0.001%
100	15.422	4470	4473	4474	rBV	647	361	0.00%	0.001%




Sum of corrected areas: 42657157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026982.D
Acq On : 27 Jul 2022 04:10
Operator : SY/MD
Sample : N3880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

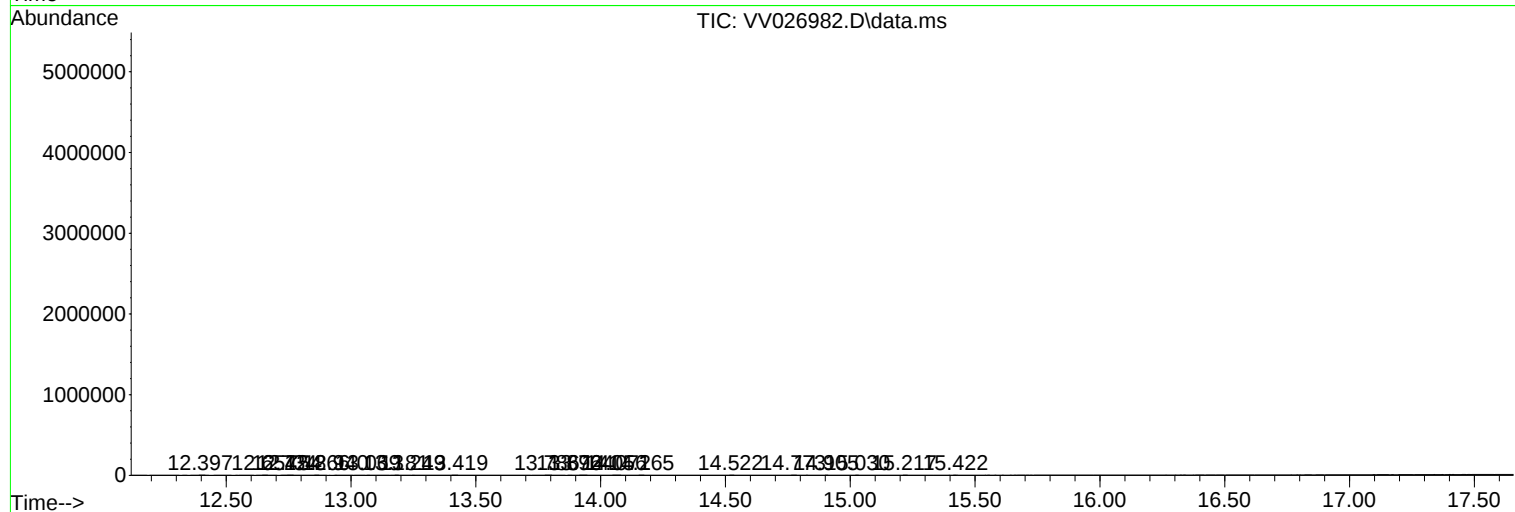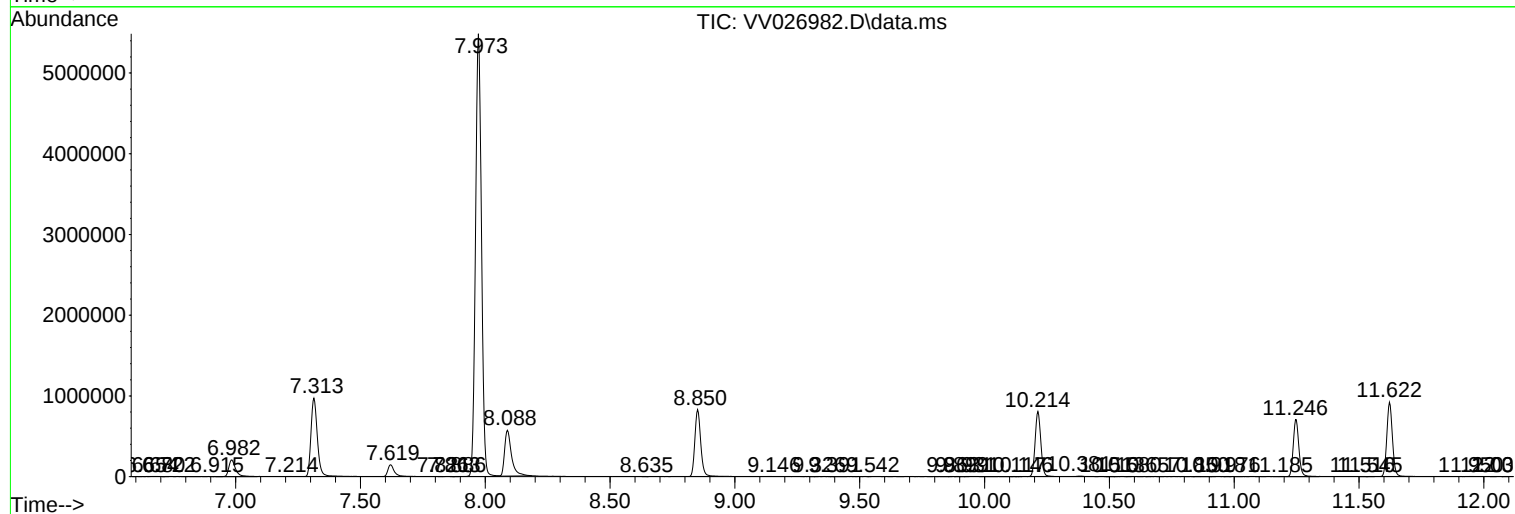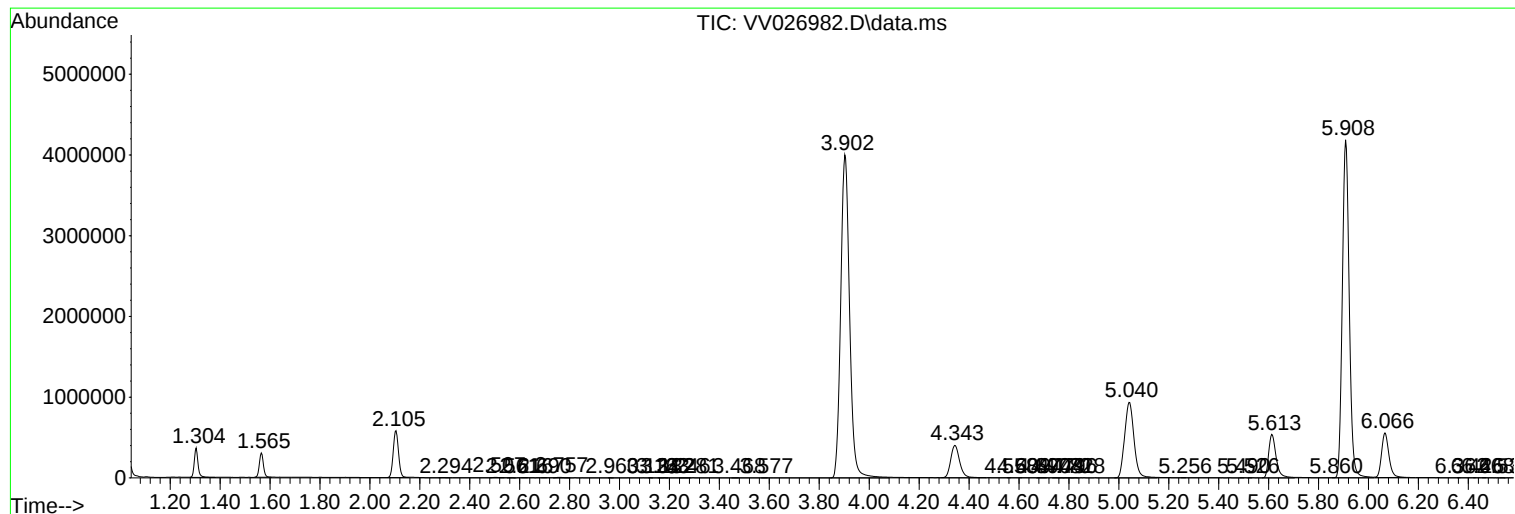

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026982.D
Acq On : 27 Jul 2022 04:10
Operator : SY/MD
Sample : N3880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026982.D
Acq On : 27 Jul 2022 04:10
Operator : SY/MD
Sample : N3880-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc