

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026983.D
 Acq On : 27 Jul 2022 04:34
 Operator : SY/MD
 Sample : N3880-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	356140	368882	0.18%	0.166%
2	1.564	155	163	177	rBV	303835	343196	0.17%	0.155%
3	2.105	320	331	346	rBV	614432	878240	0.43%	0.396%
4	2.507	447	456	466	rVB4	4723	8264	0.00%	0.004%
5	2.654	496	502	505	rBV3	317	423	0.00%	0.000%
6	2.761	525	535	548	rBV2	7001	12824	0.01%	0.006%
7	2.847	558	562	567	rBV2	371	440	0.00%	0.000%
8	2.979	600	603	605	rBV3	364	241	0.00%	0.000%
9	3.060	624	628	632	rVB3	327	225	0.00%	0.000%
10	3.088	632	637	640	rBV2	374	399	0.00%	0.000%
11	3.133	648	651	654	rBV2	363	243	0.00%	0.000%
12	3.571	785	787	790	rVB	402	223	0.00%	0.000%
13	3.719	826	833	838	rBV3	502	714	0.00%	0.000%
14	3.751	839	843	847	rVB2	311	260	0.00%	0.000%
15	3.902	874	890	939	rBV2	479888	1465747	0.73%	0.661%
16	4.342	1010	1027	1067	rBV	418345	1098807	0.54%	0.495%
17	4.593	1103	1105	1110	rVB2	724	497	0.00%	0.000%
18	4.722	1143	1145	1149	rVB2	489	223	0.00%	0.000%
19	4.777	1157	1162	1165	rVB2	387	336	0.00%	0.000%
20	4.796	1165	1168	1170	rBV3	367	275	0.00%	0.000%
21	4.957	1216	1218	1224	rVB3	516	412	0.00%	0.000%
22	5.040	1224	1244	1286	rBV2	973144	2519117	1.25%	1.135%
23	5.278	1316	1318	1321	rBV2	498	334	0.00%	0.000%
24	5.291	1321	1322	1327	rVB2	691	393	0.00%	0.000%
25	5.477	1376	1380	1383	rBV2	243	222	0.00%	0.000%
26	5.551	1397	1403	1405	rBV5	466	404	0.00%	0.000%
27	5.612	1409	1422	1456	rBV	580806	1189362	0.59%	0.536%
28	5.838	1489	1492	1495	rVB2	640	384	0.00%	0.000%
29	5.854	1495	1497	1500	rBV2	989	671	0.00%	0.000%
30	5.912	1501	1515	1545	rBV	583574	1169993	0.58%	0.527%
31	6.066	1550	1563	1594	rVB	562064	1145812	0.57%	0.516%
32	6.339	1644	1648	1651	rVB3	614	389	0.00%	0.000%
33	6.362	1651	1655	1657	rBV2	308	223	0.00%	0.000%
34	6.513	1690	1702	1720	rBV2	9685	18667	0.01%	0.008%
35	6.622	1733	1736	1739	rVB4	395	276	0.00%	0.000%
36	6.648	1739	1744	1745	rBV2	560	328	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026983.D
 Acq On : 27 Jul 2022 04:34
 Operator : SY/MD
 Sample : N3880-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.670	1749	1751	1753	rVV3	558	385	0.00%	0.000%
38	6.690	1755	1757	1761	rVB5	463	267	0.00%	0.000%
39	6.786	1782	1787	1791	rVB4	368	397	0.00%	0.000%
40	6.934	1831	1833	1838	rVB3	320	237	0.00%	0.000%
41	6.982	1838	1848	1874	rBV	209206	396885	0.20%	0.179%
42	7.210	1917	1919	1923	rVB2	1014	708	0.00%	0.000%
43	7.233	1923	1926	1928	rBV3	363	217	0.00%	0.000%
44	7.313	1936	1951	1974	rBV	1094118	1894160	0.94%	0.854%
45	7.513	2010	2013	2019	rVB3	1347	1000	0.00%	0.000%
46	7.619	2036	2046	2072	rVV	149945	270280	0.13%	0.122%
47	7.847	2114	2117	2119	rBV3	476	355	0.00%	0.000%
48	7.995	2135	2163	2183	rBV4	86586061	202162402	100.00%	91.125%
49	8.088	2184	2192	2229	rVB	643384	1315035	0.65%	0.593%
50	8.850	2417	2429	2454	rBV	896109	1443926	0.71%	0.651%
51	9.101	2505	2507	2510	rBV3	690	420	0.00%	0.000%
52	9.291	2563	2566	2569	rBV	580	528	0.00%	0.000%
53	9.452	2613	2616	2619	rBV2	450	260	0.00%	0.000%
54	9.783	2717	2719	2726	rBV3	311	271	0.00%	0.000%
55	9.892	2751	2753	2759	rBV2	307	269	0.00%	0.000%
56	10.091	2811	2815	2819	rVB3	424	321	0.00%	0.000%
57	10.117	2819	2823	2828	rBV4	392	409	0.00%	0.000%
58	10.146	2828	2832	2834	rBV2	564	335	0.00%	0.000%
59	10.214	2840	2853	2873	rBV	808730	1242751	0.61%	0.560%
60	10.387	2898	2907	2917	rVB4	4622	7089	0.00%	0.003%
61	10.542	2952	2955	2959	rBV4	435	313	0.00%	0.000%
62	10.580	2965	2967	2972	rVB2	863	461	0.00%	0.000%
63	10.641	2982	2986	2989	rBV2	288	312	0.00%	0.000%
64	10.725	3004	3012	3016	rBV4	464	639	0.00%	0.000%
65	10.763	3021	3024	3031	rVV4	321	366	0.00%	0.000%
66	10.853	3049	3052	3057	rVB4	815	699	0.00%	0.000%
67	10.879	3057	3060	3064	rBV3	460	363	0.00%	0.000%
68	11.030	3102	3107	3112	rBV2	667	659	0.00%	0.000%
69	11.059	3114	3116	3119	rVV3	335	221	0.00%	0.000%
70	11.143	3139	3142	3147	rVV3	307	345	0.00%	0.000%
71	11.249	3163	3175	3196	rBV	822206	1284960	0.64%	0.579%
72	11.474	3241	3245	3250	rBV5	524	578	0.00%	0.000%
73	11.622	3277	3291	3317	rBV	1027768	1585430	0.78%	0.715%
74	11.796	3343	3345	3347	rBV2	493	257	0.00%	0.000%
75	12.088	3434	3436	3440	rVB3	696	376	0.00%	0.000%
76	12.310	3503	3505	3509	rVB2	576	308	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026983.D
 Acq On : 27 Jul 2022 04:34
 Operator : SY/MD
 Sample : N3880-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.342	3509	3515	3518	rBV2	571	594	0.00%	0.000%
78	12.361	3518	3521	3523	rVB2	558	309	0.00%	0.000%
79	12.377	3523	3526	3531	rBV3	378	367	0.00%	0.000%
80	12.503	3561	3565	3567	rBV4	334	245	0.00%	0.000%
81	12.580	3586	3589	3590	rBV3	371	220	0.00%	0.000%
82	12.741	3637	3639	3645	rVB3	376	289	0.00%	0.000%
83	12.783	3649	3652	3655	rBV2	341	230	0.00%	0.000%
84	12.956	3703	3706	3712	rVB2	443	460	0.00%	0.000%
85	13.001	3717	3720	3727	rVB4	567	542	0.00%	0.000%
86	13.390	3835	3841	3844	rBV2	586	651	0.00%	0.000%
87	13.673	3926	3929	3934	rVB2	714	640	0.00%	0.000%
88	13.709	3937	3940	3942	rBV2	422	270	0.00%	0.000%
89	13.750	3949	3953	3954	rBV2	479	280	0.00%	0.000%
90	13.821	3973	3975	3979	rVB3	532	379	0.00%	0.000%
91	13.850	3979	3984	3988	rBV3	720	630	0.00%	0.000%
92	13.873	3988	3991	3992	rBV2	468	315	0.00%	0.000%
93	14.059	4046	4049	4052	rBV3	415	318	0.00%	0.000%
94	14.101	4059	4062	4065	rBV	323	259	0.00%	0.000%
95	14.159	4077	4080	4082	rBV4	660	435	0.00%	0.000%
96	14.721	4250	4255	4259	rBV5	744	897	0.00%	0.000%
97	14.853	4293	4296	4301	rBV4	524	471	0.00%	0.000%
98	14.879	4301	4304	4305	rBV2	610	328	0.00%	0.000%
99	14.959	4326	4329	4333	rBV3	665	570	0.00%	0.000%
100	15.049	4355	4357	4359	rVB3	717	343	0.00%	0.000%




Sum of corrected areas: 221852682

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026983.D
Acq On : 27 Jul 2022 04:34
Operator : SY/MD
Sample : N3880-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

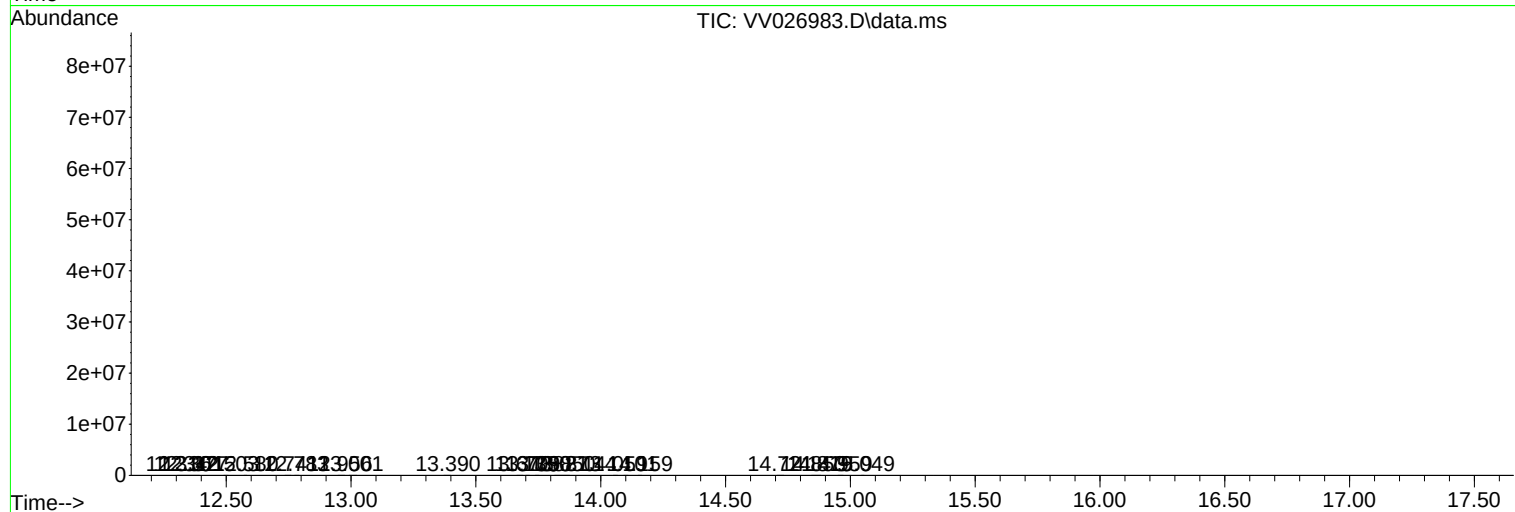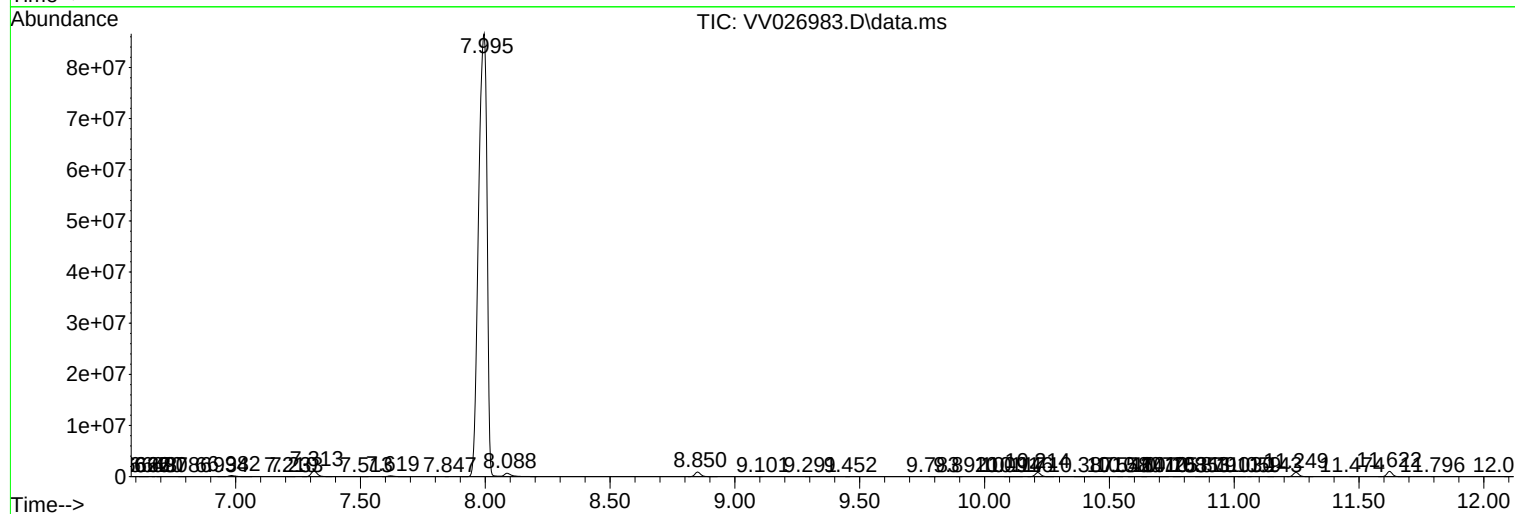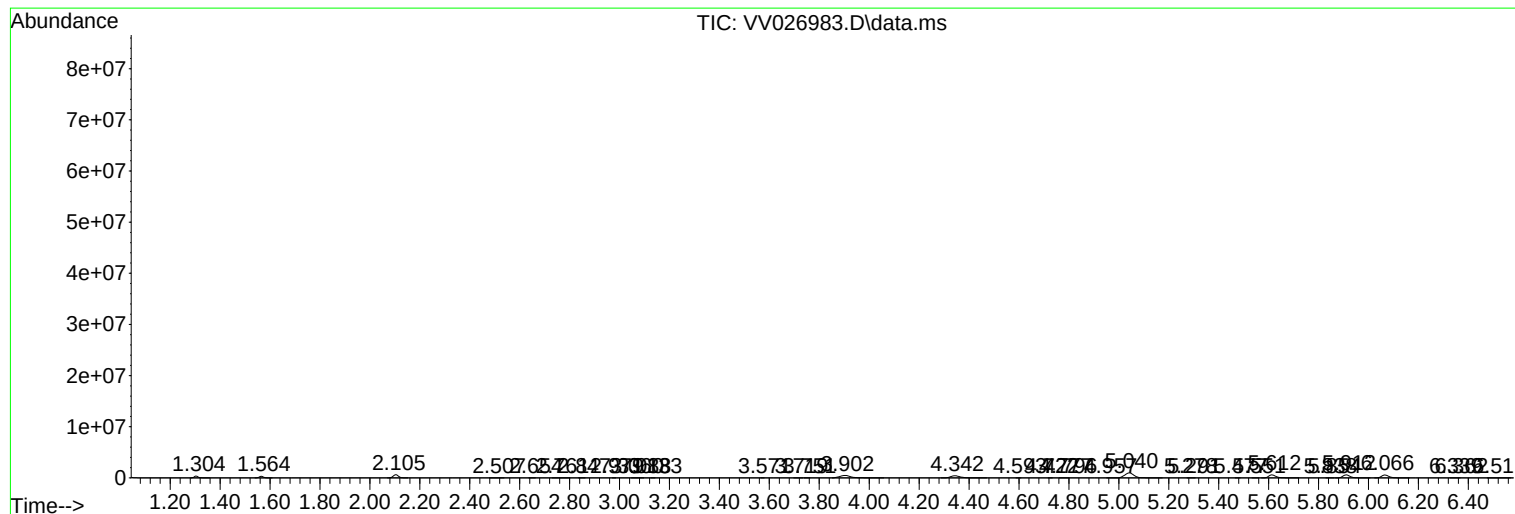

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026983.D
Acq On : 27 Jul 2022 04:34
Operator : SY/MD
Sample : N3880-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026983.D
Acq On : 27 Jul 2022 04:34
Operator : SY/MD
Sample : N3880-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DEBUG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc