

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026984.D
 Acq On : 27 Jul 2022 04:58
 Operator : SY/MD
 Sample : N3880-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	325448	334253	0.20%	0.182%
2	1.564	155	163	175	rBV	284381	321065	0.19%	0.175%
3	2.105	320	331	346	rBV	526535	756582	0.46%	0.413%
4	2.503	447	455	471	rVB3	8109	14200	0.01%	0.008%
5	2.761	527	535	550	rVB3	6411	11419	0.01%	0.006%
6	2.857	562	565	572	rBV3	413	428	0.00%	0.000%
7	2.889	572	575	577	rBV3	318	220	0.00%	0.000%
8	2.953	593	595	598	rBV	316	193	0.00%	0.000%
9	3.085	633	636	642	rBV3	218	198	0.00%	0.000%
10	3.169	657	662	665	rBV2	542	445	0.00%	0.000%
11	3.198	667	671	673	rBV2	422	328	0.00%	0.000%
12	3.252	685	688	692	rVB3	296	251	0.00%	0.000%
13	3.278	692	696	700	rBV2	327	275	0.00%	0.000%
14	3.359	717	721	725	rVB3	289	259	0.00%	0.000%
15	3.384	725	729	735	rVB2	377	345	0.00%	0.000%
16	3.574	785	788	792	rVB3	284	290	0.00%	0.000%
17	3.603	792	797	800	rBV2	378	435	0.00%	0.000%
18	3.902	874	890	943	rBV4	468642	1419368	0.86%	0.775%
19	4.342	1010	1027	1060	rBV	390806	1027675	0.62%	0.561%
20	4.613	1107	1111	1115	rVB4	475	374	0.00%	0.000%
21	4.822	1171	1176	1177	rBV	432	236	0.00%	0.000%
22	4.908	1200	1203	1206	rBV3	385	244	0.00%	0.000%
23	4.947	1212	1215	1217	rVB3	364	226	0.00%	0.000%
24	4.969	1217	1222	1225	rBV2	405	347	0.00%	0.000%
25	5.040	1225	1244	1291	rBV2	887067	2321785	1.40%	1.268%
26	5.314	1326	1329	1334	rBV4	949	733	0.00%	0.000%
27	5.381	1348	1350	1353	rVB2	391	198	0.00%	0.000%
28	5.420	1359	1362	1367	rVB4	375	312	0.00%	0.000%
29	5.555	1401	1404	1408	rBV2	258	251	0.00%	0.000%
30	5.613	1409	1422	1459	rBV	512003	1060231	0.64%	0.579%
31	5.912	1501	1515	1543	rBV	513415	1029209	0.62%	0.562%
32	6.066	1550	1563	1585	rBV	529971	1071039	0.65%	0.585%
33	6.342	1645	1649	1650	rBV3	421	307	0.00%	0.000%
34	6.352	1650	1652	1657	rVB2	810	428	0.00%	0.000%
35	6.403	1664	1668	1669	rBV3	605	243	0.00%	0.000%
36	6.429	1673	1676	1680	rVB4	466	413	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026984.D
 Acq On : 27 Jul 2022 04:58
 Operator : SY/MD
 Sample : N3880-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.513	1692	1702	1717	rBV2	8416	17502	0.01%	0.010%
38	6.567	1717	1719	1722	rVB3	662	271	0.00%	0.000%
39	6.603	1727	1730	1737	rVB2	450	362	0.00%	0.000%
40	6.670	1748	1751	1756	rVB3	464	402	0.00%	0.000%
41	6.825	1794	1799	1802	rVB2	321	294	0.00%	0.000%
42	6.847	1804	1806	1811	rVB2	322	200	0.00%	0.000%
43	6.928	1825	1831	1835	rVB4	739	577	0.00%	0.000%
44	6.985	1838	1849	1871	rBV	194543	366228	0.22%	0.200%
45	7.204	1913	1917	1922	rBV3	485	492	0.00%	0.000%
46	7.313	1939	1951	1973	rBV	917680	1590624	0.96%	0.868%
47	7.622	2037	2047	2074	rBV	139524	253732	0.15%	0.139%
48	7.989	2136	2161	2183	rBV4	78582369	165521076	100.00%	90.372%
49	8.088	2184	2192	2226	rVB	606781	1217804	0.74%	0.665%
50	8.850	2417	2429	2456	rBV	756713	1244532	0.75%	0.679%
51	9.172	2527	2529	2532	rBV3	659	376	0.00%	0.000%
52	9.751	2706	2709	2715	rBV4	317	322	0.00%	0.000%
53	9.783	2716	2719	2723	rVV4	367	323	0.00%	0.000%
54	9.850	2738	2740	2742	rBV3	325	197	0.00%	0.000%
55	10.014	2788	2791	2796	rVB2	430	337	0.00%	0.000%
56	10.037	2796	2798	2802	rBV4	326	239	0.00%	0.000%
57	10.214	2839	2853	2874	rBV	753576	1182246	0.71%	0.645%
58	10.384	2899	2906	2919	rVB4	4336	7354	0.00%	0.004%
59	10.551	2952	2958	2960	rBV3	708	734	0.00%	0.000%
60	10.580	2964	2967	2970	rBV3	437	373	0.00%	0.000%
61	10.722	3008	3011	3014	rBV	568	350	0.00%	0.000%
62	10.770	3022	3026	3028	rBV2	304	247	0.00%	0.000%
63	10.792	3031	3033	3039	rBV2	433	303	0.00%	0.000%
64	10.853	3049	3052	3056	rBV2	648	452	0.00%	0.000%
65	10.966	3084	3087	3089	rVB3	432	273	0.00%	0.000%
66	10.985	3089	3093	3098	rBV4	393	356	0.00%	0.000%
67	11.011	3098	3101	3105	rBV2	195	196	0.00%	0.000%
68	11.136	3135	3140	3142	rBV3	415	302	0.00%	0.000%
69	11.246	3163	3174	3200	rBV	671067	1038273	0.63%	0.567%
70	11.622	3278	3291	3311	rBV	839307	1320518	0.80%	0.721%
71	11.837	3355	3358	3359	rBV	468	342	0.00%	0.000%
72	11.870	3365	3368	3371	rVB4	484	239	0.00%	0.000%
73	11.908	3376	3380	3383	rBV2	327	312	0.00%	0.000%
74	12.124	3443	3447	3452	rBV3	367	453	0.00%	0.000%
75	12.255	3485	3488	3492	rVB3	847	681	0.00%	0.000%
76	12.445	3544	3547	3550	rVB2	457	285	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026984.D
 Acq On : 27 Jul 2022 04:58
 Operator : SY/MD
 Sample : N3880-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.487	3556	3560	3561	rBV2	469	297	0.00%	0.000%
78	12.503	3561	3565	3568	rBV4	280	273	0.00%	0.000%
79	12.654	3608	3612	3615	rBV2	345	304	0.00%	0.000%
80	12.857	3671	3675	3677	rBV3	398	312	0.00%	0.000%
81	12.905	3687	3690	3691	rBV	364	200	0.00%	0.000%
82	13.082	3741	3745	3748	rBV2	461	314	0.00%	0.000%
83	13.278	3801	3806	3813	rVB5	881	1007	0.00%	0.001%
84	13.329	3819	3822	3826	rBV3	672	522	0.00%	0.000%
85	13.586	3897	3902	3906	rBV2	557	578	0.00%	0.000%
86	13.628	3910	3915	3918	rBV2	508	571	0.00%	0.000%
87	13.725	3941	3945	3947	rBV3	300	252	0.00%	0.000%
88	13.873	3989	3991	3993	rVB2	732	229	0.00%	0.000%
89	14.085	4054	4057	4063	rVB3	547	420	0.00%	0.000%
90	14.123	4067	4069	4072	rVB2	546	252	0.00%	0.000%
91	14.162	4078	4081	4082	rBV	457	223	0.00%	0.000%
92	14.172	4082	4084	4087	rVV3	366	260	0.00%	0.000%
93	14.387	4149	4151	4153	rVB2	544	222	0.00%	0.000%
94	14.648	4230	4232	4235	rBV	464	233	0.00%	0.000%
95	14.673	4236	4240	4244	rVV5	686	627	0.00%	0.000%
96	14.744	4259	4262	4265	rBV	486	401	0.00%	0.000%
97	14.876	4301	4303	4306	rBV2	481	279	0.00%	0.000%
98	15.127	4375	4381	4384	rBV6	776	947	0.00%	0.001%
99	15.246	4416	4418	4420	rBV3	646	290	0.00%	0.000%
100	15.914	4624	4626	4629	rBV3	988	441	0.00%	0.000%




Sum of corrected areas: 183154438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026984.D
Acq On : 27 Jul 2022 04:58
Operator : SY/MD
Sample : N3880-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

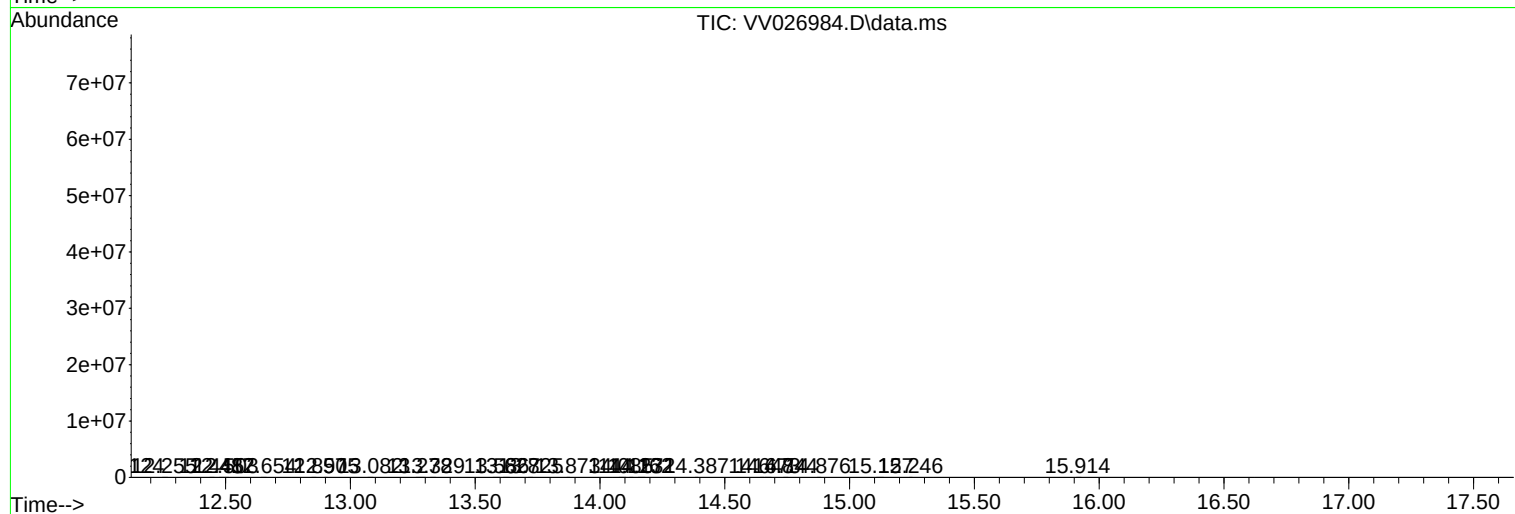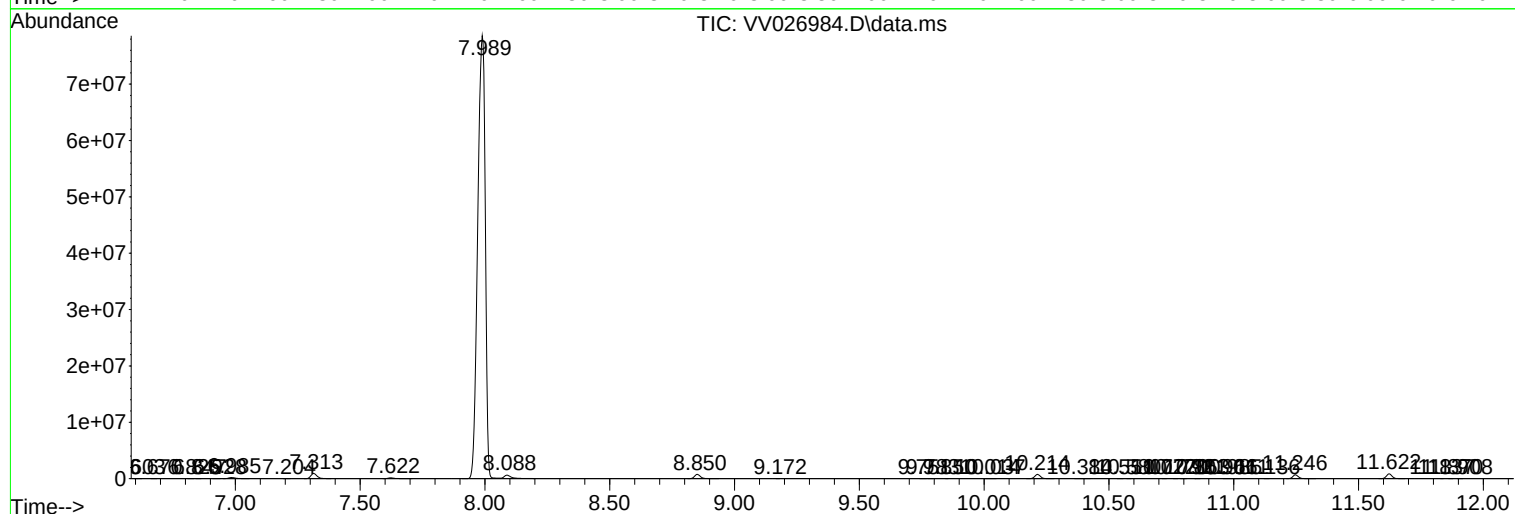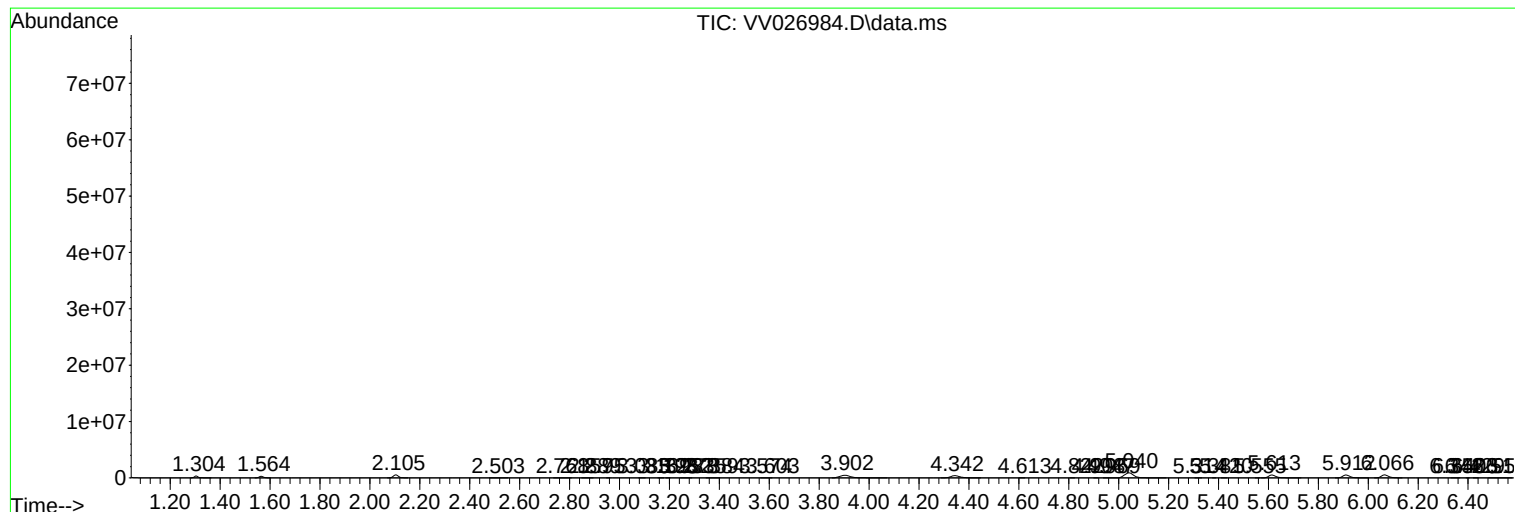

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026984.D
Acq On : 27 Jul 2022 04:58
Operator : SY/MD
Sample : N3880-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026984.D
Acq On : 27 Jul 2022 04:58
Operator : SY/MD
Sample : N3880-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc