

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026985.D
 Acq On : 27 Jul 2022 05:23
 Operator : SY/MD
 Sample : N3880-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.069	6	9	32	rVB	60649	69061	0.06%	0.051%
2	1.201	45	50	56	rBV2	11434	12766	0.01%	0.009%
3	1.304	75	82	102	rVB	354422	367257	0.31%	0.272%
4	1.564	155	163	178	rBV	295830	338053	0.29%	0.251%
5	2.105	320	331	345	rBV	600100	859774	0.73%	0.637%
6	2.416	426	428	432	rBV	483	355	0.00%	0.000%
7	2.500	448	454	464	rVB6	2801	4827	0.00%	0.004%
8	2.555	469	471	476	rBV2	273	297	0.00%	0.000%
9	2.674	505	508	513	rVB3	488	291	0.00%	0.000%
10	2.725	521	524	528	rBV2	539	478	0.00%	0.000%
11	2.754	528	533	536	rBV3	1521	1526	0.00%	0.001%
12	2.921	581	585	590	rBV4	286	289	0.00%	0.000%
13	3.166	658	661	664	rBV3	616	525	0.00%	0.000%
14	3.442	742	747	750	rBV2	374	400	0.00%	0.000%
15	3.519	768	771	777	rVB4	432	509	0.00%	0.000%
16	3.548	777	780	785	rBV	501	447	0.00%	0.000%
17	3.892	874	887	929	rBV3	185543	689650	0.59%	0.511%
18	4.275	1001	1006	1009	rBV3	566	497	0.00%	0.000%
19	4.342	1009	1027	1068	rBV	406335	1029793	0.88%	0.763%
20	4.613	1109	1111	1118	rVB4	500	403	0.00%	0.000%
21	4.719	1141	1144	1147	rBV3	425	345	0.00%	0.000%
22	4.912	1200	1204	1207	rBV3	380	346	0.00%	0.000%
23	4.941	1207	1213	1217	rVV3	542	543	0.00%	0.000%
24	5.043	1227	1245	1281	rBV2	948570	2452341	2.09%	1.817%
25	5.387	1349	1352	1356	rBV2	483	366	0.00%	0.000%
26	5.490	1375	1384	1387	rBV4	903	908	0.00%	0.001%
27	5.555	1401	1404	1406	rBV3	554	341	0.00%	0.000%
28	5.613	1410	1422	1458	rBV	568628	1165007	0.99%	0.863%
29	5.912	1502	1515	1544	rBV3	207012	431243	0.37%	0.320%
30	6.066	1549	1563	1592	rBV	546757	1120779	0.96%	0.831%
31	6.474	1684	1690	1693	rVB3	428	319	0.00%	0.000%
32	6.535	1705	1709	1715	rVB3	557	536	0.00%	0.000%
33	6.625	1733	1737	1741	rBV4	317	386	0.00%	0.000%
34	6.648	1741	1744	1746	rBV2	547	361	0.00%	0.000%
35	6.693	1756	1758	1762	rVB2	584	344	0.00%	0.000%
36	6.741	1770	1773	1775	rBV	496	293	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026985.D
 Acq On : 27 Jul 2022 05:23
 Operator : SY/MD
 Sample : N3880-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.892	1817	1820	1826	rVB3	331	296	0.00%	0.000%
38	6.985	1836	1849	1871	rBV	204254	386326	0.33%	0.286%
39	7.120	1888	1891	1896	rVB2	771	574	0.00%	0.000%
40	7.204	1912	1917	1919	rBV5	614	584	0.00%	0.000%
41	7.256	1931	1933	1937	rVB4	780	463	0.00%	0.000%
42	7.313	1937	1951	1976	rBV	1050310	1839063	1.57%	1.363%
43	7.619	2036	2046	2079	rBV	146571	270604	0.23%	0.201%
44	7.825	2108	2110	2114	rVB2	503	302	0.00%	0.000%
45	7.847	2114	2117	2119	rBV2	516	408	0.00%	0.000%
46	7.982	2137	2159	2183	rBV	62384729	117136566	100.00%	86.811%
47	8.088	2184	2192	2229	rVB	622810	1235461	1.05%	0.916%
48	8.622	2355	2358	2363	rVB6	1164	997	0.00%	0.001%
49	8.735	2392	2393	2397	rBV3	576	362	0.00%	0.000%
50	8.786	2405	2409	2411	rBV3	548	514	0.00%	0.000%
51	8.850	2417	2429	2457	rBV	878128	1418799	1.21%	1.051%
52	9.104	2505	2508	2509	rBV2	690	406	0.00%	0.000%
53	9.153	2519	2523	2532	rVB9	1544	2249	0.00%	0.002%
54	9.403	2598	2601	2606	rVB4	511	442	0.00%	0.000%
55	9.455	2614	2617	2618	rBV	1022	490	0.00%	0.000%
56	9.509	2629	2634	2635	rBV2	592	340	0.00%	0.000%
57	9.542	2639	2644	2646	rBV3	723	627	0.00%	0.000%
58	9.702	2691	2694	2697	rVV3	720	546	0.00%	0.000%
59	9.805	2721	2726	2734	rBV5	1141	1450	0.00%	0.001%
60	9.876	2744	2748	2750	rBV3	422	289	0.00%	0.000%
61	9.931	2760	2765	2767	rBV3	494	502	0.00%	0.000%
62	9.944	2767	2769	2776	rVB3	802	521	0.00%	0.000%
63	10.011	2787	2790	2796	rVB3	327	298	0.00%	0.000%
64	10.133	2825	2828	2831	rVB2	560	336	0.00%	0.000%
65	10.214	2841	2853	2874	rBV	802407	1249645	1.07%	0.926%
66	10.384	2899	2906	2916	rVB5	4203	6398	0.01%	0.005%
67	10.635	2981	2984	2987	rVV2	463	308	0.00%	0.000%
68	10.693	2998	3002	3006	rBV	407	430	0.00%	0.000%
69	10.728	3008	3013	3021	rVB5	1572	2180	0.00%	0.002%
70	10.921	3068	3073	3074	rBV2	623	535	0.00%	0.000%
71	11.165	3144	3149	3151	rBV3	408	385	0.00%	0.000%
72	11.197	3156	3159	3162	rBV2	392	316	0.00%	0.000%
73	11.246	3163	3174	3199	rBV	803571	1254260	1.07%	0.930%
74	11.435	3230	3233	3235	rBV	619	402	0.00%	0.000%
75	11.567	3270	3274	3277	rVB4	629	460	0.00%	0.000%
76	11.622	3278	3291	3323	rBV	999521	1553358	1.33%	1.151%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026985.D
 Acq On : 27 Jul 2022 05:23
 Operator : SY/MD
 Sample : N3880-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.947	3385	3392	3395	rBV3	656	839	0.00%	0.001%
78	11.982	3399	3403	3405	rBV2	375	302	0.00%	0.000%
79	12.352	3515	3518	3522	rVB2	404	312	0.00%	0.000%
80	12.596	3592	3594	3600	rVB3	459	375	0.00%	0.000%
81	12.850	3668	3673	3678	rBV3	558	703	0.00%	0.001%
82	12.947	3695	3703	3706	rBV2	767	703	0.00%	0.001%
83	12.969	3706	3710	3713	rVV4	640	586	0.00%	0.000%
84	13.004	3717	3721	3725	rVV3	375	380	0.00%	0.000%
85	13.361	3829	3832	3835	rVB4	629	382	0.00%	0.000%
86	13.416	3847	3849	3855	rVB	521	483	0.00%	0.000%
87	13.448	3855	3859	3864	rBV4	408	494	0.00%	0.000%
88	13.509	3875	3878	3880	rBV2	900	639	0.00%	0.000%
89	14.014	4033	4035	4044	rVB4	608	696	0.00%	0.001%
90	14.056	4045	4048	4053	rBV4	498	596	0.00%	0.000%
91	14.599	4215	4217	4219	rBV2	589	344	0.00%	0.000%
92	14.683	4240	4243	4244	rBV2	581	327	0.00%	0.000%
93	14.721	4252	4255	4259	rVB3	785	527	0.00%	0.000%
94	14.744	4259	4262	4266	rBV3	407	458	0.00%	0.000%
95	14.918	4314	4316	4321	rBV2	571	472	0.00%	0.000%
96	15.091	4367	4370	4373	rBV2	741	515	0.00%	0.000%
97	15.139	4382	4385	4387	rBV4	774	503	0.00%	0.000%
98	15.281	4427	4429	4435	rVB4	1268	748	0.00%	0.001%
99	15.332	4442	4445	4450	rBV4	888	832	0.00%	0.001%
100	15.564	4515	4517	4521	rBV5	861	574	0.00%	0.000%




Sum of corrected areas: 134932938

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026985.D
Acq On : 27 Jul 2022 05:23
Operator : SY/MD
Sample : N3880-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

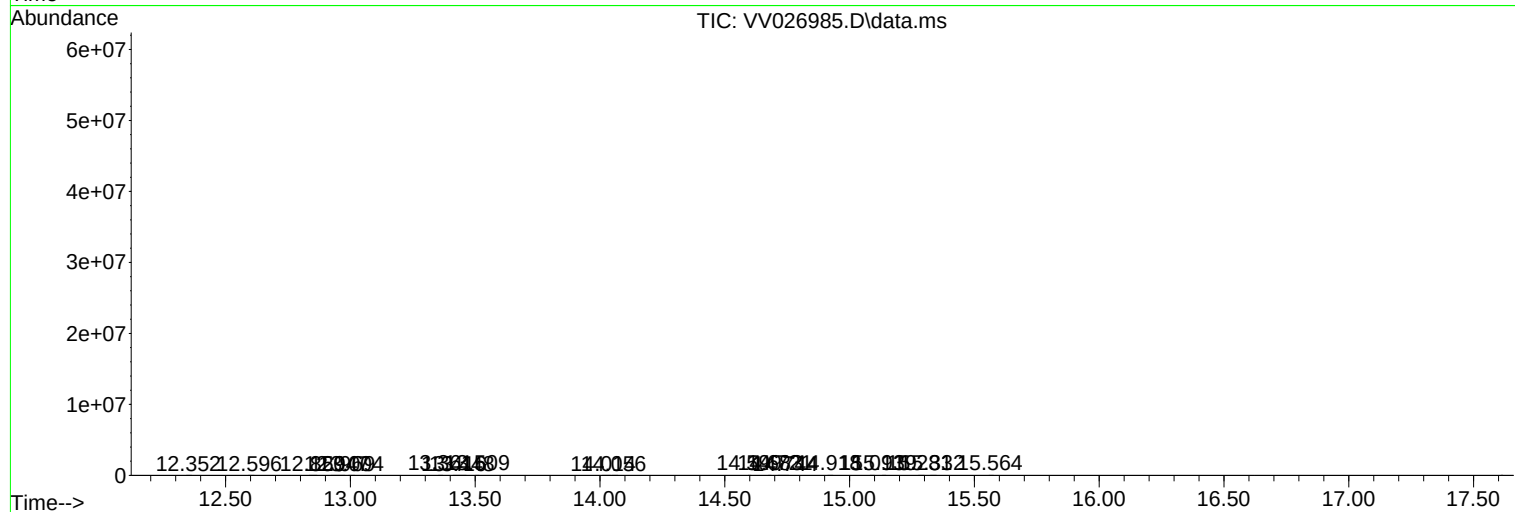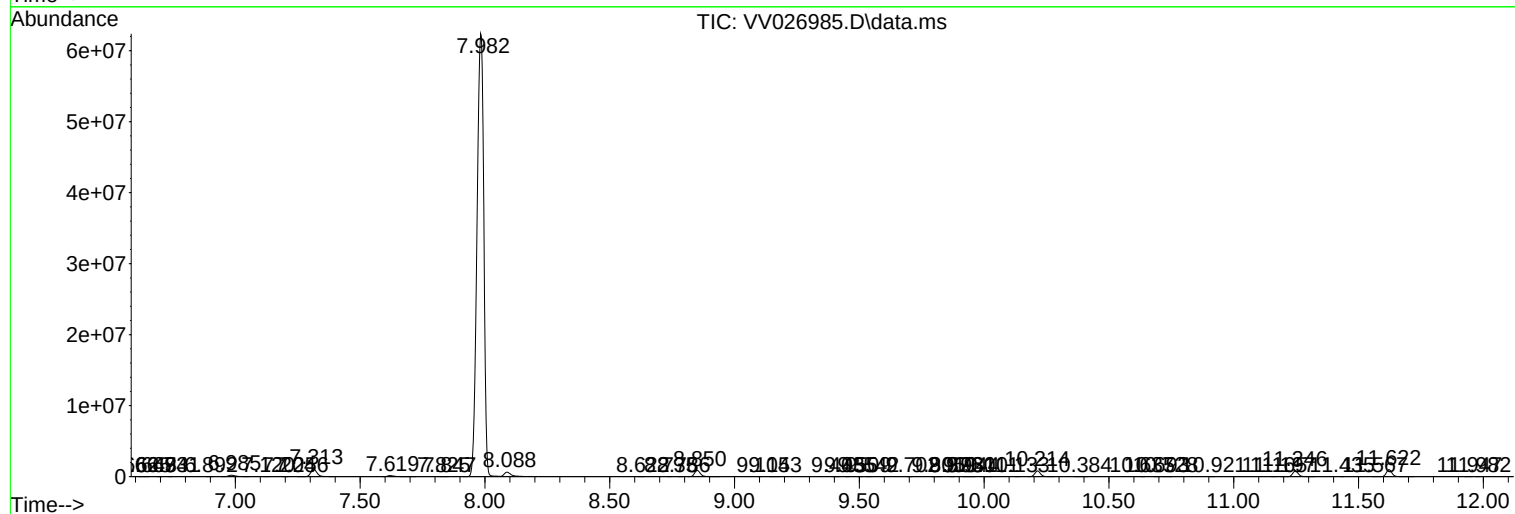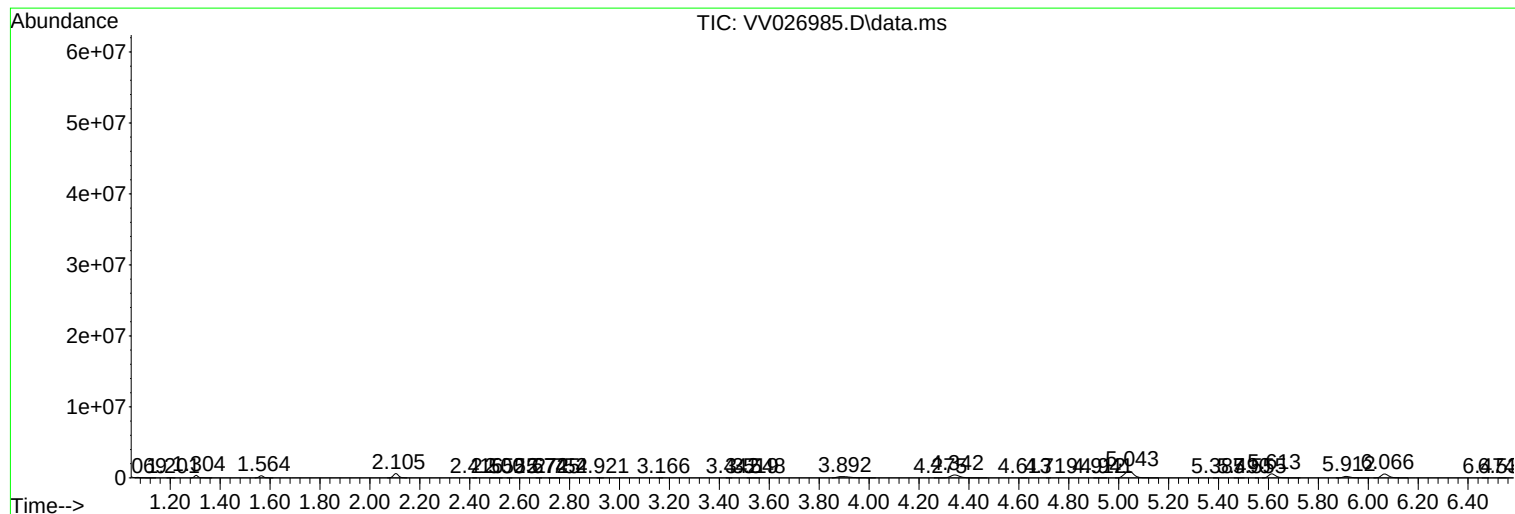

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026985.D
Acq On : 27 Jul 2022 05:23
Operator : SY/MD
Sample : N3880-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG3









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.069	2.96 ug/L	69061	1,4-Difluorobenzene	5.612

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,1,1,3,3,3-Hexafluoropropan-2-o...	331	C6HF12NO	053517-77-4	4		
2	Propargylamine, N-trifluoroacetyl-	151	C5H4F3NO	014719-21-2	4		
3	Neral	152	C10H16O	000106-26-3	3		
4	Fluoroform	70	CHF3	000075-46-7	3		
5	Fluoroform	70	CHF3	000075-46-7	3		

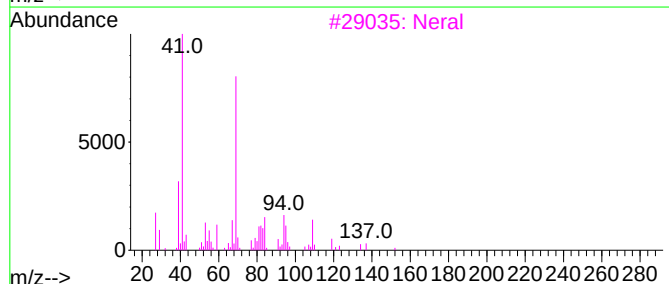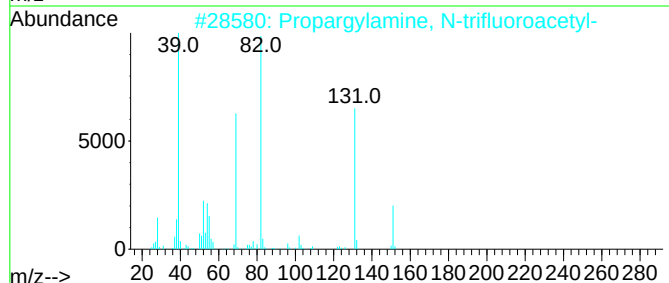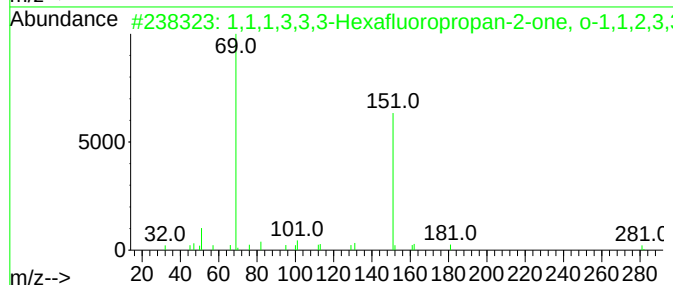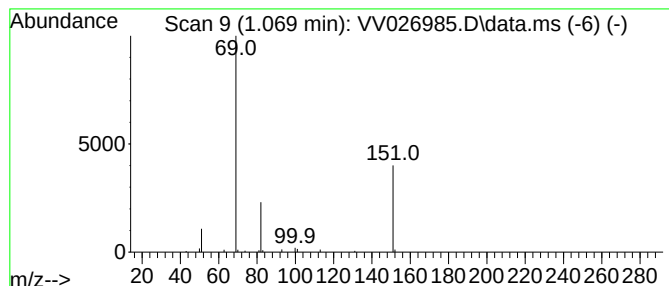

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026985.D
Acq On : 27 Jul 2022 05:23
Operator : SY/MD
Sample : N3880-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DEBUG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.069	3.0	ug/L	69061	1	5.612	1165010	50.0