

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026986.D
 Acq On : 27 Jul 2022 05:47
 Operator : SY/MD
 Sample : N3880-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	343751	359381	0.26%	0.225%
2	1.564	155	163	176	rBV	293284	331980	0.24%	0.208%
3	2.105	320	331	346	rBV	584920	840613	0.60%	0.527%
4	2.294	385	390	395	rVB5	1146	1258	0.00%	0.001%
5	2.507	449	456	464	rVB7	4367	7572	0.01%	0.005%
6	2.609	485	488	489	rBV2	452	255	0.00%	0.000%
7	2.761	527	535	548	rVB6	4180	7968	0.01%	0.005%
8	2.857	558	565	568	rBV4	282	395	0.00%	0.000%
9	3.053	622	626	628	rBV3	605	514	0.00%	0.000%
10	3.195	665	670	675	rBV3	278	320	0.00%	0.000%
11	3.265	689	692	697	rVB4	466	383	0.00%	0.000%
12	3.391	727	731	737	rVB	382	415	0.00%	0.000%
13	3.433	737	744	750	rBV3	264	463	0.00%	0.000%
14	3.494	760	763	767	rVB3	291	237	0.00%	0.000%
15	3.539	774	777	779	rBV	323	232	0.00%	0.000%
16	3.564	782	785	789	rVB2	380	329	0.00%	0.000%
17	3.587	789	792	797	rBV3	377	382	0.00%	0.000%
18	3.658	808	814	817	rVB2	353	300	0.00%	0.000%
19	3.728	831	836	838	rBV2	405	373	0.00%	0.000%
20	3.902	874	890	936	rBV2	330692	1090294	0.78%	0.683%
21	4.162	969	971	975	rBV4	888	585	0.00%	0.000%
22	4.342	1010	1027	1058	rVV	406367	1018738	0.73%	0.639%
23	4.873	1187	1192	1198	rVB3	383	416	0.00%	0.000%
24	4.915	1198	1205	1207	rBV2	478	411	0.00%	0.000%
25	4.969	1220	1222	1225	rBV3	285	230	0.00%	0.000%
26	5.043	1228	1245	1285	rBV2	936552	2420267	1.73%	1.517%
27	5.429	1363	1365	1368	rBV3	417	232	0.00%	0.000%
28	5.484	1379	1382	1386	rBV3	350	273	0.00%	0.000%
29	5.612	1410	1422	1455	rBV	557489	1154389	0.82%	0.724%
30	5.908	1501	1514	1550	rBV	1120956	2243360	1.60%	1.406%
31	6.066	1550	1563	1591	rVB	542405	1113237	0.80%	0.698%
32	6.288	1628	1632	1636	rVB4	546	509	0.00%	0.000%
33	6.349	1649	1651	1657	rVB4	652	743	0.00%	0.000%
34	6.397	1662	1666	1669	rBV3	494	550	0.00%	0.000%
35	6.439	1673	1679	1680	rBV3	457	436	0.00%	0.000%
36	6.513	1697	1702	1705	rBV4	862	802	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026986.D
 Acq On : 27 Jul 2022 05:47
 Operator : SY/MD
 Sample : N3880-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.741	1770	1773	1776	rBV2	485	275	0.00%	0.000%
38	6.764	1776	1780	1782	rBV3	496	271	0.00%	0.000%
39	6.982	1838	1848	1876	rBV	203201	384096	0.27%	0.241%
40	7.124	1890	1892	1893	rBV	565	261	0.00%	0.000%
41	7.207	1913	1918	1920	rBV4	789	656	0.00%	0.000%
42	7.313	1938	1951	1971	rBV	1025936	1784701	1.27%	1.119%
43	7.622	2036	2047	2067	rBV	143281	260172	0.19%	0.163%
44	7.799	2100	2102	2105	rBV	365	236	0.00%	0.000%
45	7.850	2116	2118	2126	rVB6	1185	1222	0.00%	0.001%
46	7.886	2127	2129	2132	rVB2	582	329	0.00%	0.000%
47	7.985	2132	2160	2183	rBV2	70945340	140006845	100.00%	87.759%
48	8.088	2184	2192	2225	rVB	621225	1209404	0.86%	0.758%
49	8.702	2381	2383	2385	rVB2	582	281	0.00%	0.000%
50	8.812	2414	2417	2418	rBV3	486	300	0.00%	0.000%
51	8.850	2418	2429	2456	rVV	844120	1382701	0.99%	0.867%
52	9.120	2510	2513	2514	rBV2	413	235	0.00%	0.000%
53	9.143	2515	2520	2521	rBV3	1036	910	0.00%	0.001%
54	9.468	2619	2621	2622	rBV	522	257	0.00%	0.000%
55	9.548	2643	2646	2647	rBV2	492	332	0.00%	0.000%
56	9.783	2716	2719	2725	rVB2	402	356	0.00%	0.000%
57	9.937	2759	2767	2778	rVV3	2507	3343	0.00%	0.002%
58	10.011	2787	2790	2793	rBV2	461	314	0.00%	0.000%
59	10.214	2840	2853	2878	rBV	775827	1215390	0.87%	0.762%
60	10.384	2897	2906	2916	rVB2	4512	6935	0.00%	0.004%
61	10.542	2951	2955	2962	rBV4	517	583	0.00%	0.000%
62	10.590	2963	2970	2973	rVV6	520	675	0.00%	0.000%
63	10.609	2973	2976	2980	rVB2	313	258	0.00%	0.000%
64	10.699	3001	3004	3008	rVB2	416	316	0.00%	0.000%
65	10.754	3015	3021	3026	rBV3	479	600	0.00%	0.000%
66	10.783	3026	3030	3034	rBV2	414	343	0.00%	0.000%
67	10.853	3048	3052	3056	rVV5	896	757	0.00%	0.000%
68	10.882	3058	3061	3065	rVB3	528	305	0.00%	0.000%
69	11.075	3117	3121	3123	rVB2	337	233	0.00%	0.000%
70	11.197	3155	3159	3162	rBV3	692	484	0.00%	0.000%
71	11.249	3162	3175	3195	rBV	769999	1186575	0.85%	0.744%
72	11.535	3260	3264	3266	rBV3	470	384	0.00%	0.000%
73	11.622	3279	3291	3318	rVV	942286	1475460	1.05%	0.925%
74	12.143	3450	3453	3456	rBV	335	262	0.00%	0.000%
75	12.207	3469	3473	3474	rBV	639	332	0.00%	0.000%
76	12.307	3501	3504	3509	rBV3	627	486	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026986.D
 Acq On : 27 Jul 2022 05:47
 Operator : SY/MD
 Sample : N3880-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.439	3542	3545	3547	rBV3	466	294	0.00%	0.000%
78	12.558	3579	3582	3586	rVB3	450	391	0.00%	0.000%
79	12.580	3586	3589	3597	rVB4	363	430	0.00%	0.000%
80	12.619	3597	3601	3604	rBV3	420	410	0.00%	0.000%
81	12.773	3647	3649	3652	rBV	445	259	0.00%	0.000%
82	12.844	3667	3671	3672	rBV2	404	269	0.00%	0.000%
83	12.876	3678	3681	3686	rBV3	309	335	0.00%	0.000%
84	13.024	3723	3727	3732	rBV4	395	398	0.00%	0.000%
85	13.149	3763	3766	3767	rBV	388	245	0.00%	0.000%
86	13.210	3781	3785	3786	rBV3	431	300	0.00%	0.000%
87	13.422	3847	3851	3852	rBV2	456	273	0.00%	0.000%
88	13.702	3935	3938	3939	rBV3	370	246	0.00%	0.000%
89	13.776	3958	3961	3964	rBV2	422	306	0.00%	0.000%
90	13.911	4000	4003	4007	rBV3	391	376	0.00%	0.000%
91	14.082	4054	4056	4060	rBV2	319	239	0.00%	0.000%
92	14.220	4097	4099	4102	rVB2	493	234	0.00%	0.000%
93	14.287	4117	4120	4123	rBV2	512	353	0.00%	0.000%
94	14.365	4142	4144	4147	rVB	509	229	0.00%	0.000%
95	14.471	4175	4177	4180	rVB2	897	472	0.00%	0.000%
96	14.516	4187	4191	4195	rVV3	631	466	0.00%	0.000%
97	14.670	4234	4239	4241	rBV3	799	709	0.00%	0.000%
98	14.686	4241	4244	4246	rBV	504	266	0.00%	0.000%
99	15.223	4409	4411	4415	rBV3	769	561	0.00%	0.000%
100	15.696	4555	4558	4562	rBV4	985	714	0.00%	0.000%




Sum of corrected areas: 159535492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026986.D
Acq On : 27 Jul 2022 05:47
Operator : SY/MD
Sample : N3880-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

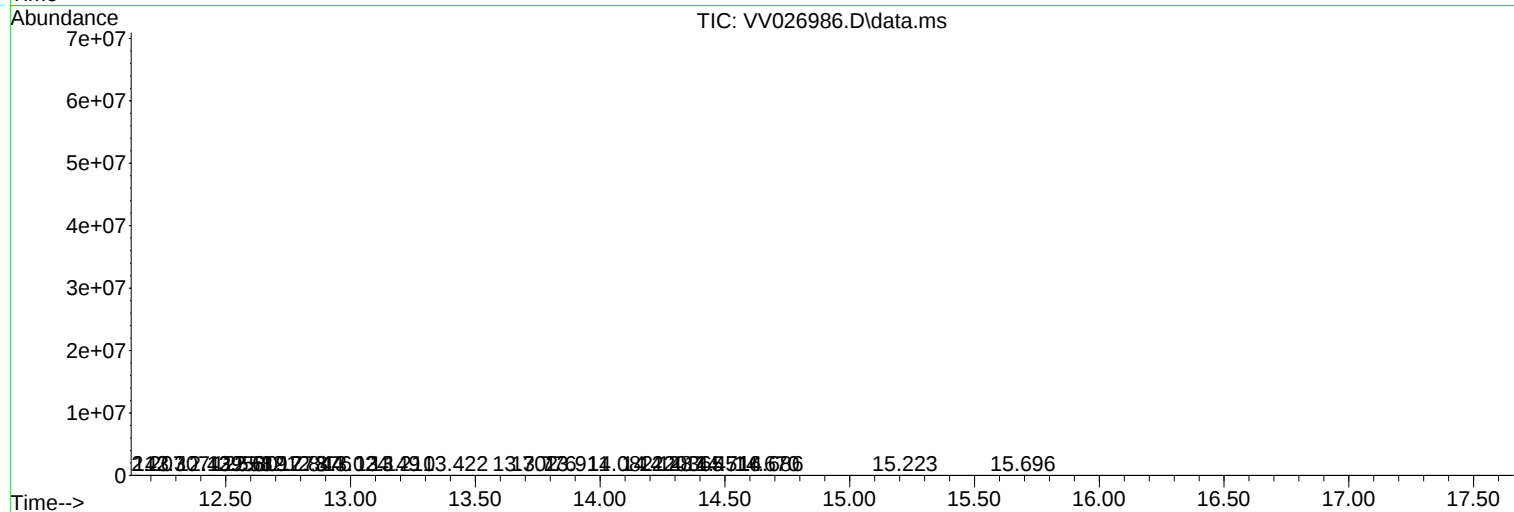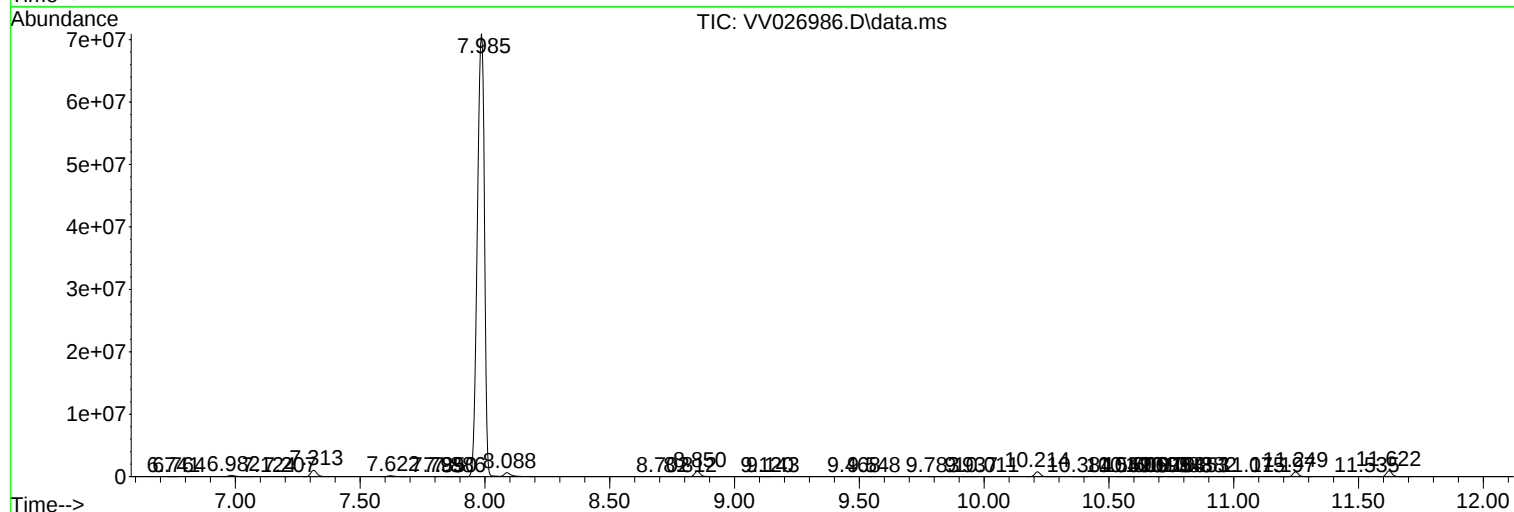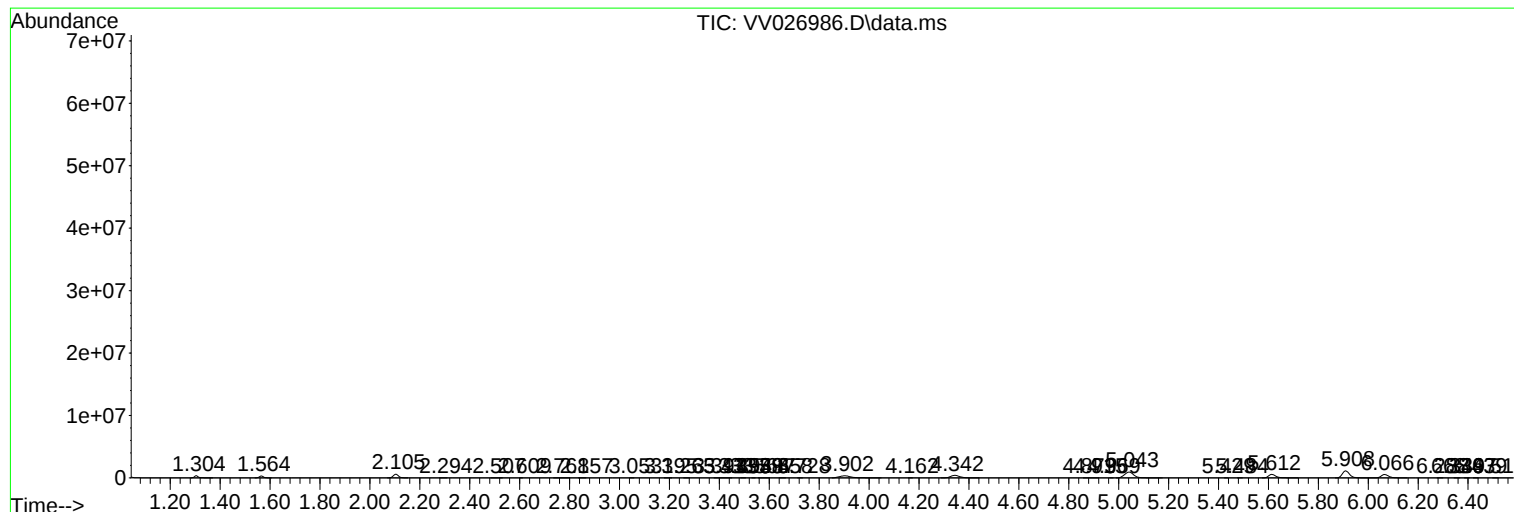

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026986.D
Acq On : 27 Jul 2022 05:47
Operator : SY/MD
Sample : N3880-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026986.D
Acq On : 27 Jul 2022 05:47
Operator : SY/MD
Sample : N3880-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
