

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026987.D
 Acq On : 27 Jul 2022 06:12
 Operator : SY/MD
 Sample : N3880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	352923	359948	4.65%	1.386%
2	1.565	156	163	178	rBV	289981	325321	4.20%	1.252%
3	2.105	321	331	346	rBV	595430	848876	10.96%	3.268%
4	2.610	484	488	492	rBV2	569	573	0.01%	0.002%
5	2.680	507	510	513	rBV4	577	415	0.01%	0.002%
6	2.757	528	534	544	rVB7	2367	3963	0.05%	0.015%
7	2.947	591	593	596	rBV	459	272	0.00%	0.001%
8	3.073	629	632	636	rVB4	390	327	0.00%	0.001%
9	3.134	647	651	654	rVB3	313	303	0.00%	0.001%
10	3.156	654	658	665	rBV3	331	402	0.01%	0.002%
11	3.188	665	668	669	rBV2	390	231	0.00%	0.001%
12	3.355	718	720	725	rVB	418	193	0.00%	0.001%
13	3.378	725	727	730	rBV2	157	111	0.00%	0.000%
14	3.391	730	731	732	rBV	332	83	0.00%	0.000%
15	3.442	744	747	750	rBV3	410	278	0.00%	0.001%
16	3.471	750	756	759	rVB3	354	410	0.01%	0.002%
17	3.494	759	763	765	rBV2	310	223	0.00%	0.001%
18	3.519	768	771	773	rVB2	230	133	0.00%	0.001%
19	3.561	781	784	786	rBV	183	110	0.00%	0.000%
20	3.581	786	790	792	rBV2	162	129	0.00%	0.000%
21	3.593	792	794	795	rBV2	162	51	0.00%	0.000%
22	3.638	807	808	809	rBV2	167	59	0.00%	0.000%
23	3.677	817	820	823	rBV2	311	203	0.00%	0.001%
24	3.719	831	833	836	rBV2	238	121	0.00%	0.000%
25	3.777	849	851	852	rVB	196	54	0.00%	0.000%
26	3.793	852	856	858	rVB	293	200	0.00%	0.001%
27	3.806	858	860	863	rBV	449	165	0.00%	0.001%
28	3.822	863	865	867	rBV	155	100	0.00%	0.000%
29	3.902	874	890	939	rBV2	317288	1058946	13.67%	4.077%
30	4.343	1011	1027	1063	rBV	400788	999444	12.90%	3.848%
31	4.658	1123	1125	1127	rBV	390	207	0.00%	0.001%
32	4.671	1127	1129	1131	rVV3	467	319	0.00%	0.001%
33	4.699	1135	1138	1141	rVV	376	257	0.00%	0.001%
34	4.719	1142	1144	1150	rVB3	593	403	0.01%	0.002%
35	4.863	1187	1189	1191	rBV	234	131	0.00%	0.001%
36	4.921	1205	1207	1210	rVB	299	142	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026987.D
 Acq On : 27 Jul 2022 06:12
 Operator : SY/MD
 Sample : N3880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	4.941	1210	1213	1217	rBV	282	299	0.00%	0.001%
38	5.040	1227	1244	1285	rBV2	941384	2436456	31.45%	9.380%
39	5.355	1340	1342	1346	rVB3	395	236	0.00%	0.001%
40	5.410	1356	1359	1362	rBV	306	215	0.00%	0.001%
41	5.449	1369	1371	1373	rBV2	332	143	0.00%	0.001%
42	5.461	1373	1375	1378	rVB2	380	215	0.00%	0.001%
43	5.490	1381	1384	1386	rBV	346	193	0.00%	0.001%
44	5.529	1394	1396	1399	rBV2	511	379	0.00%	0.001%
45	5.613	1410	1422	1453	rBV	555978	1141641	14.74%	4.395%
46	5.860	1496	1499	1501	rBV4	851	594	0.01%	0.002%
47	5.912	1502	1515	1539	rBV	406057	825619	10.66%	3.178%
48	6.066	1551	1563	1592	rVB	538698	1098048	14.17%	4.227%
49	6.294	1632	1634	1640	rBV4	548	443	0.01%	0.002%
50	6.333	1645	1646	1647	rBV	289	68	0.00%	0.000%
51	6.388	1660	1663	1665	rBV2	146	118	0.00%	0.000%
52	6.400	1665	1667	1670	rVV2	248	154	0.00%	0.001%
53	6.455	1682	1684	1688	rVB3	299	120	0.00%	0.000%
54	6.490	1691	1695	1698	rBV3	366	263	0.00%	0.001%
55	6.526	1705	1706	1708	rBV	186	66	0.00%	0.000%
56	6.561	1714	1717	1718	rBV2	325	162	0.00%	0.001%
57	6.619	1731	1735	1737	rBV3	562	450	0.01%	0.002%
58	6.648	1742	1744	1746	rBV2	526	227	0.00%	0.001%
59	6.751	1773	1776	1778	rVB2	349	187	0.00%	0.001%
60	6.789	1782	1788	1791	rBV	487	367	0.00%	0.001%
61	6.802	1791	1792	1797	rBV2	270	142	0.00%	0.001%
62	6.841	1802	1804	1805	rBV	294	78	0.00%	0.000%
63	6.860	1805	1810	1815	rVB3	313	345	0.00%	0.001%
64	6.883	1815	1817	1820	rVB3	267	124	0.00%	0.000%
65	6.912	1822	1826	1828	rBV3	264	192	0.00%	0.001%
66	6.944	1833	1836	1838	rBV3	230	151	0.00%	0.001%
67	6.986	1838	1849	1882	rBV	196399	376073	4.85%	1.448%
68	7.314	1936	1951	1987	rBV	1024144	1812550	23.40%	6.978%
69	7.619	2036	2046	2068	rBV	143379	256164	3.31%	0.986%
70	7.805	2102	2104	2108	rBV3	657	213	0.00%	0.001%
71	7.844	2112	2116	2118	rBV3	752	617	0.01%	0.002%
72	7.973	2139	2156	2181	rBV	4684866	7747320	100.00%	29.826%
73	8.088	2183	2192	2227	rVB	584595	1145690	14.79%	4.411%
74	8.703	2376	2383	2387	rBV4	893	977	0.01%	0.004%
75	8.773	2403	2405	2407	rBV	539	154	0.00%	0.001%
76	8.850	2417	2429	2457	rBV	892082	1462406	18.88%	5.630%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026987.D
 Acq On : 27 Jul 2022 06:12
 Operator : SY/MD
 Sample : N3880-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.259	2554	2556	2558	rBV2	265	76	0.00%	0.000%
78	9.346	2580	2583	2584	rBV2	402	184	0.00%	0.001%
79	9.420	2604	2606	2610	rBV3	231	208	0.00%	0.001%
80	9.481	2623	2625	2627	rVB	295	77	0.00%	0.000%
81	9.548	2642	2646	2648	rBV2	630	498	0.01%	0.002%
82	9.574	2652	2654	2658	rBV4	530	395	0.01%	0.002%
83	9.838	2734	2736	2737	rBV	139	33	0.00%	0.000%
84	9.892	2748	2753	2755	rBV3	300	276	0.00%	0.001%
85	9.921	2759	2762	2764	rBV2	619	423	0.01%	0.002%
86	10.053	2801	2803	2806	rBV	751	209	0.00%	0.001%
87	10.214	2841	2853	2879	rBV	823633	1284411	16.58%	4.945%
88	10.384	2899	2906	2916	rVB2	4202	6040	0.08%	0.023%
89	10.426	2916	2919	2924	rVB3	490	399	0.01%	0.002%
90	10.474	2932	2934	2935	rBV2	278	111	0.00%	0.000%
91	10.542	2952	2955	2957	rBV2	341	208	0.00%	0.001%
92	10.664	2991	2993	2994	rBV2	279	104	0.00%	0.000%
93	10.854	3047	3052	3054	rBV3	683	558	0.01%	0.002%
94	11.143	3140	3142	3146	rBV2	297	146	0.00%	0.001%
95	11.246	3163	3174	3199	rBV	785903	1224331	15.80%	4.713%
96	11.513	3255	3257	3260	rVB2	564	274	0.00%	0.001%
97	11.622	3279	3291	3310	rBV	958315	1542576	19.91%	5.939%
98	13.992	4026	4028	4031	rBV3	676	418	0.01%	0.002%
99	14.114	4064	4066	4071	rVB2	561	278	0.00%	0.001%




Sum of corrected areas: 25975195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026987.D
Acq On : 27 Jul 2022 06:12
Operator : SY/MD
Sample : N3880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

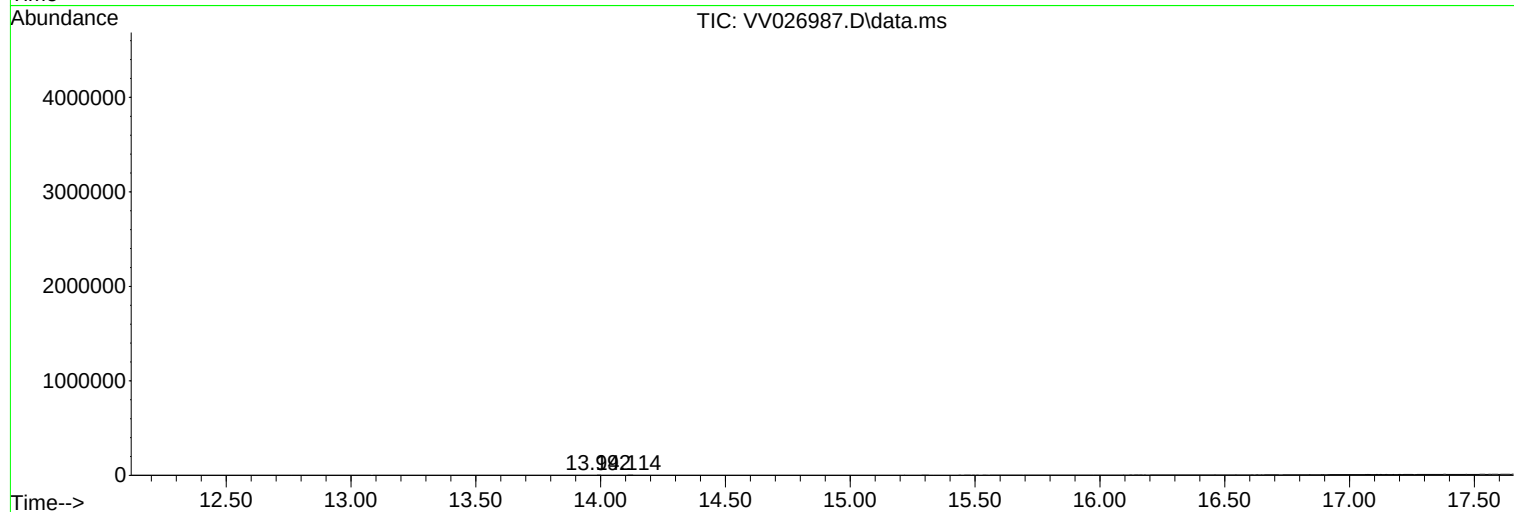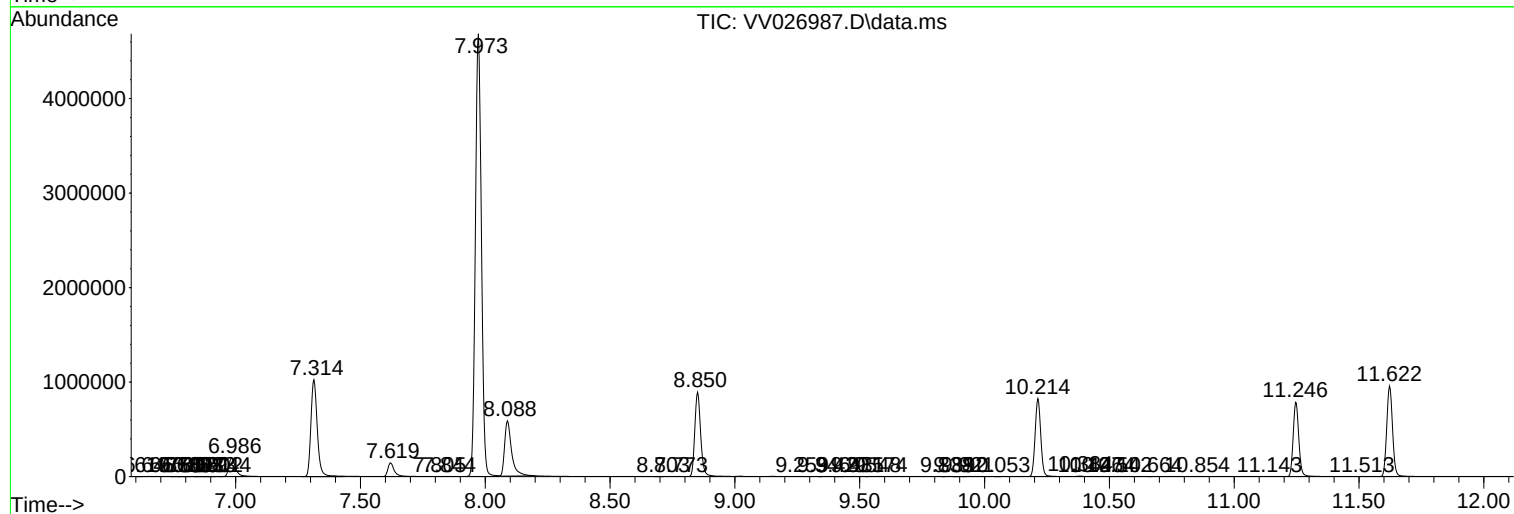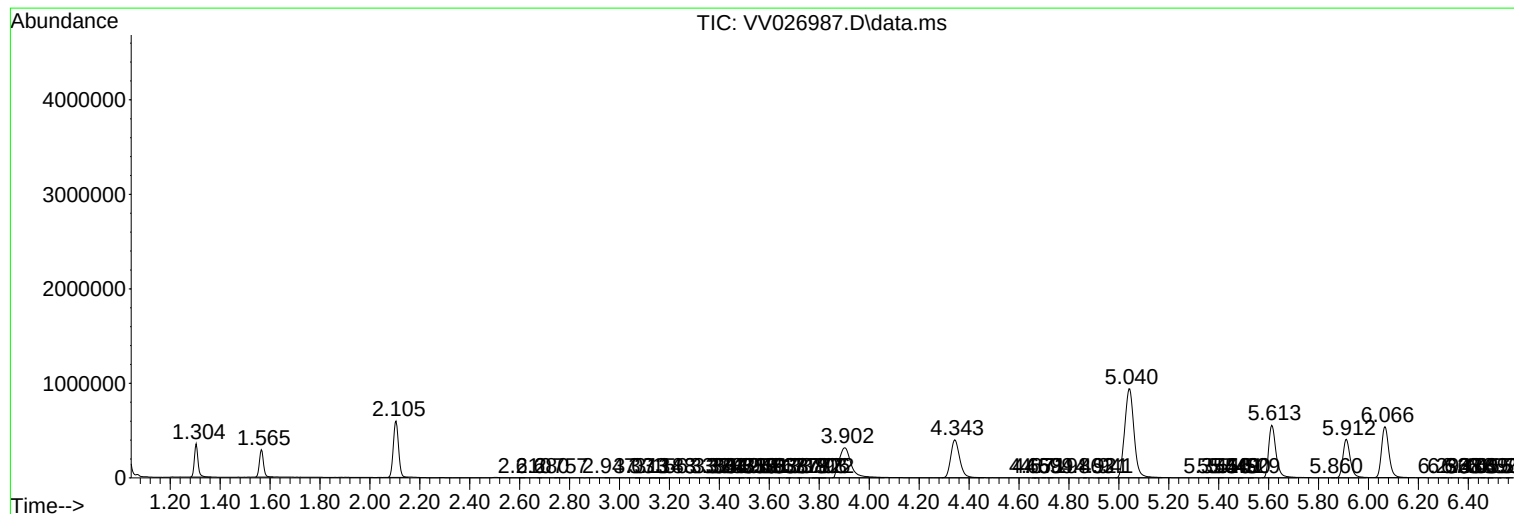

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026987.D
Acq On : 27 Jul 2022 06:12
Operator : SY/MD
Sample : N3880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026987.D
Acq On : 27 Jul 2022 06:12
Operator : SY/MD
Sample : N3880-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
