

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026989.D
 Acq On : 27 Jul 2022 07:00
 Operator : SY/MD
 Sample : N3880-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	244437	254413	0.59%	0.440%
2	1.564	156	163	177	rBV	220144	248669	0.58%	0.430%
3	2.104	320	331	348	rBV	412942	594570	1.38%	1.029%
4	2.506	447	456	464	rVB8	2228	4118	0.01%	0.007%
5	2.767	532	537	542	rVB4	1198	1298	0.00%	0.002%
6	2.966	596	599	603	rBV4	403	288	0.00%	0.000%
7	3.047	623	624	631	rVB2	735	536	0.00%	0.001%
8	3.082	631	635	636	rBV	343	222	0.00%	0.000%
9	3.239	680	684	688	rBV2	511	407	0.00%	0.001%
10	3.352	715	719	726	rBV3	291	222	0.00%	0.000%
11	3.744	838	841	844	rBV2	469	460	0.00%	0.001%
12	3.812	857	862	864	rBV2	276	255	0.00%	0.000%
13	3.899	875	889	943	rBV2	216467	786952	1.83%	1.361%
14	4.265	999	1003	1008	rBV5	430	505	0.00%	0.001%
15	4.342	1012	1027	1065	rVV	333587	840689	1.95%	1.454%
16	4.516	1079	1081	1082	rBV2	633	235	0.00%	0.000%
17	4.603	1106	1108	1113	rVB3	422	328	0.00%	0.001%
18	4.667	1126	1128	1130	rBV2	447	249	0.00%	0.000%
19	4.747	1150	1153	1156	rBV2	280	210	0.00%	0.000%
20	4.809	1168	1172	1176	rVB2	284	220	0.00%	0.000%
21	4.931	1205	1210	1212	rBV2	647	431	0.00%	0.001%
22	5.043	1227	1245	1280	rBV2	779057	2041019	4.75%	3.531%
23	5.358	1337	1343	1345	rBV3	442	412	0.00%	0.001%
24	5.436	1364	1367	1372	rVB	694	447	0.00%	0.001%
25	5.487	1379	1383	1386	rBV3	596	643	0.00%	0.001%
26	5.503	1386	1388	1392	rVV	574	403	0.00%	0.001%
27	5.612	1411	1422	1453	rBV	427678	888080	2.06%	1.536%
28	5.911	1502	1515	1545	rBV2	242564	506250	1.18%	0.876%
29	6.066	1549	1563	1594	rBV	462924	950513	2.21%	1.644%
30	6.368	1655	1657	1660	rVV3	545	332	0.00%	0.001%
31	6.413	1667	1671	1674	rVV4	556	462	0.00%	0.001%
32	6.468	1684	1688	1690	rVB2	422	223	0.00%	0.000%
33	6.516	1699	1703	1708	rBV3	295	291	0.00%	0.001%
34	6.577	1719	1722	1725	rVB2	446	262	0.00%	0.000%
35	6.593	1725	1727	1734	rBV3	290	258	0.00%	0.000%
36	6.651	1738	1745	1746	rBV3	588	443	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026989.D
 Acq On : 27 Jul 2022 07:00
 Operator : SY/MD
 Sample : N3880-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.718	1764	1766	1771	rVB4	509	366	0.00%	0.001%
38	6.741	1771	1773	1780	rBV3	350	364	0.00%	0.001%
39	6.818	1790	1797	1799	rBV	506	545	0.00%	0.001%
40	6.985	1838	1849	1873	rBV	168922	319033	0.74%	0.552%
41	7.136	1894	1896	1901	rVB3	744	457	0.00%	0.001%
42	7.313	1939	1951	1984	rBV	802763	1425316	3.31%	2.466%
43	7.622	2035	2047	2070	rBV	123348	225467	0.52%	0.390%
44	7.767	2090	2092	2095	rVB2	625	334	0.00%	0.001%
45	7.879	2125	2127	2130	rBV	332	246	0.00%	0.000%
46	7.976	2136	2157	2183	rBV	26131318	43013534	100.00%	74.410%
47	8.088	2183	2192	2229	rVB	565499	1114693	2.59%	1.928%
48	8.403	2288	2290	2293	rBV4	663	310	0.00%	0.001%
49	8.458	2306	2307	2315	rVB5	1130	1038	0.00%	0.002%
50	8.580	2342	2345	2347	rBV2	432	259	0.00%	0.000%
51	8.609	2349	2354	2357	rBV5	516	515	0.00%	0.001%
52	8.725	2388	2390	2391	rBV	436	215	0.00%	0.000%
53	8.850	2417	2429	2452	rBV	723587	1172050	2.72%	2.028%
54	9.095	2502	2505	2508	rBV3	433	256	0.00%	0.000%
55	9.152	2516	2523	2528	rBV4	3013	3669	0.01%	0.006%
56	9.233	2544	2548	2554	rBV2	539	574	0.00%	0.001%
57	9.291	2563	2566	2570	rBV3	389	346	0.00%	0.001%
58	9.313	2570	2573	2575	rVV2	444	272	0.00%	0.000%
59	9.352	2581	2585	2588	rVB3	380	314	0.00%	0.001%
60	9.371	2588	2591	2594	rVB3	361	260	0.00%	0.000%
61	9.390	2594	2597	2599	rBV3	453	243	0.00%	0.000%
62	9.406	2599	2602	2605	rBV3	523	432	0.00%	0.001%
63	9.554	2643	2648	2651	rBV3	1100	855	0.00%	0.001%
64	9.625	2669	2670	2675	rVB3	401	247	0.00%	0.000%
65	9.828	2731	2733	2738	rVB3	335	236	0.00%	0.000%
66	9.937	2764	2767	2772	rVB3	449	283	0.00%	0.000%
67	10.033	2794	2797	2801	rVV2	320	283	0.00%	0.000%
68	10.149	2831	2833	2838	rBV2	299	260	0.00%	0.000%
69	10.213	2841	2853	2876	rVV	733419	1145830	2.66%	1.982%
70	10.381	2898	2905	2913	rVB5	3384	4999	0.01%	0.009%
71	10.493	2938	2940	2945	rVB2	414	242	0.00%	0.000%
72	10.516	2945	2947	2950	rBV2	257	216	0.00%	0.000%
73	10.541	2951	2955	2958	rBV2	1000	744	0.00%	0.001%
74	10.914	3065	3071	3073	rBV4	953	985	0.00%	0.002%
75	10.992	3093	3095	3100	rVV2	287	215	0.00%	0.000%
76	11.098	3126	3128	3132	rBV2	350	276	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026989.D
 Acq On : 27 Jul 2022 07:00
 Operator : SY/MD
 Sample : N3880-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3201	rBV	616250	971041	2.26%	1.680%
78	11.480	3245	3247	3254	rVB5	280	277	0.00%	0.000%
79	11.622	3277	3291	3313	rBV	791691	1262903	2.94%	2.185%
80	11.824	3352	3354	3357	rVB3	633	259	0.00%	0.000%
81	11.914	3380	3382	3392	rVB6	715	837	0.00%	0.001%
82	11.959	3392	3396	3398	rBV2	494	430	0.00%	0.001%
83	12.217	3473	3476	3480	rBV3	328	294	0.00%	0.001%
84	12.249	3481	3486	3492	rVV2	729	872	0.00%	0.002%
85	12.805	3657	3659	3662	rBV2	354	236	0.00%	0.000%
86	12.889	3679	3685	3689	rBV2	629	759	0.00%	0.001%
87	13.001	3718	3720	3726	rBV3	298	239	0.00%	0.000%
88	13.033	3727	3730	3735	rBV4	312	263	0.00%	0.000%
89	13.348	3826	3828	3832	rBV3	457	277	0.00%	0.000%
90	13.397	3839	3843	3847	rVB2	541	454	0.00%	0.001%
91	13.461	3860	3863	3866	rBV2	571	356	0.00%	0.001%
92	13.683	3930	3932	3937	rBV3	447	348	0.00%	0.001%
93	13.805	3966	3970	3972	rBV2	490	347	0.00%	0.001%
94	13.905	3998	4001	4008	rBV4	521	492	0.00%	0.001%
95	14.319	4128	4130	4133	rBV2	445	352	0.00%	0.001%
96	14.792	4275	4277	4279	rBV	613	360	0.00%	0.001%
97	14.882	4301	4305	4309	rBV3	717	596	0.00%	0.001%
98	15.216	4407	4409	4413	rBV3	473	341	0.00%	0.001%
99	15.342	4446	4448	4452	rVB4	714	455	0.00%	0.001%
100	15.821	4594	4597	4602	rBV4	1257	1095	0.00%	0.002%




Sum of corrected areas: 57805977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026989.D
Acq On : 27 Jul 2022 07:00
Operator : SY/MD
Sample : N3880-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

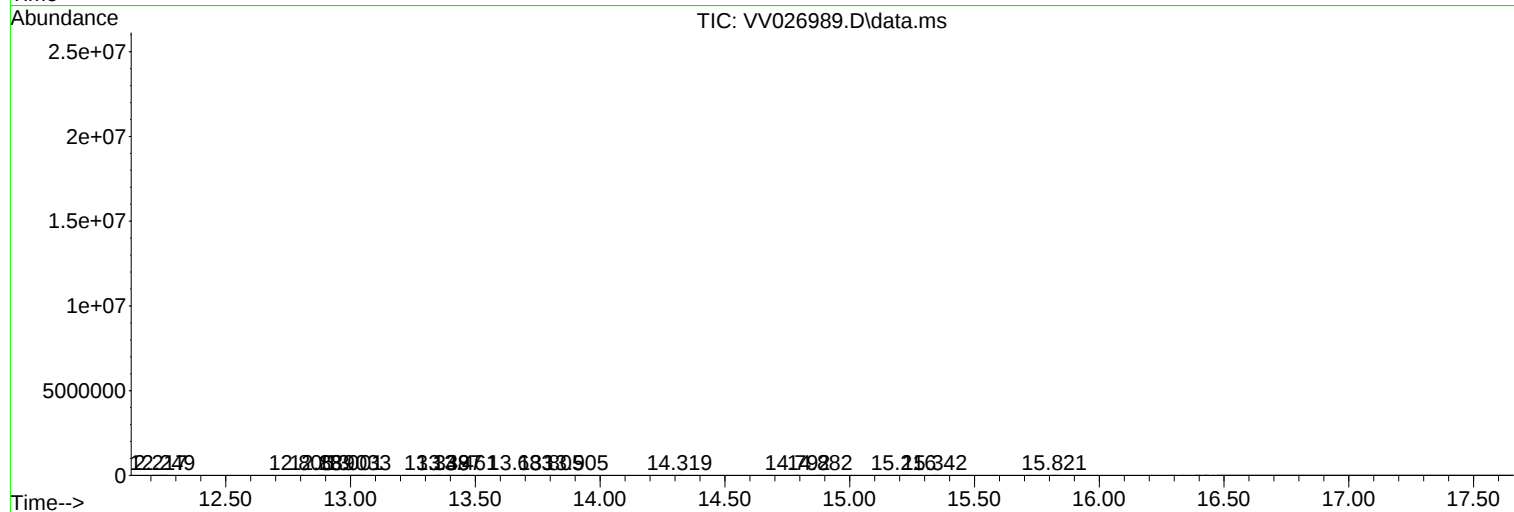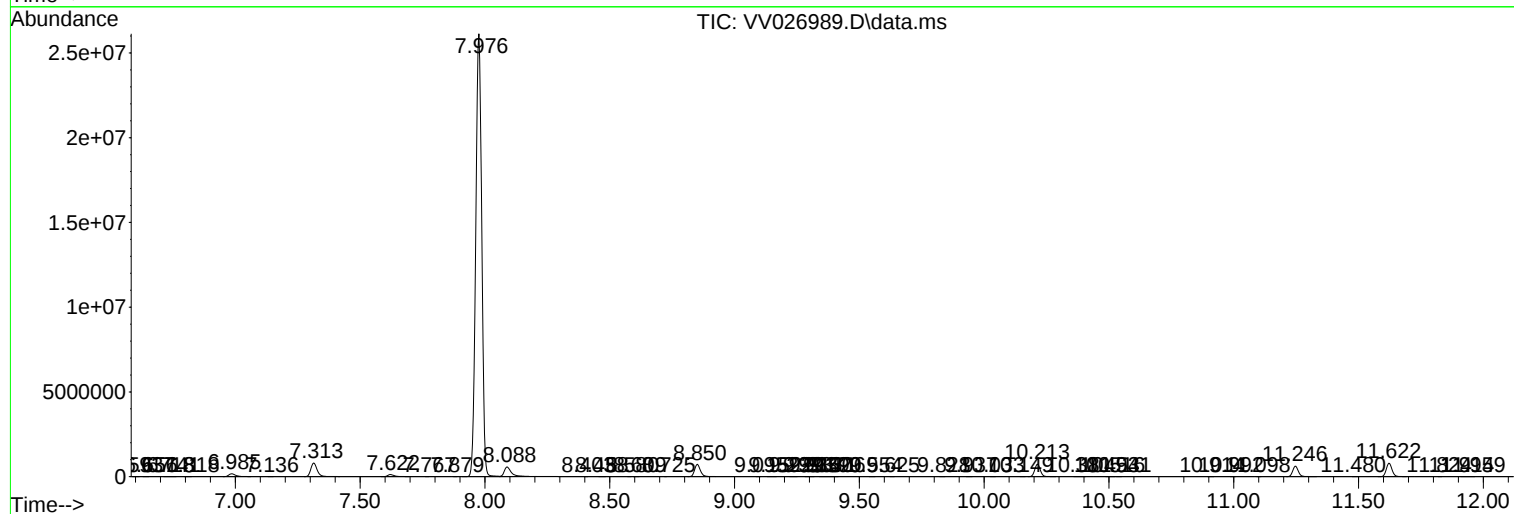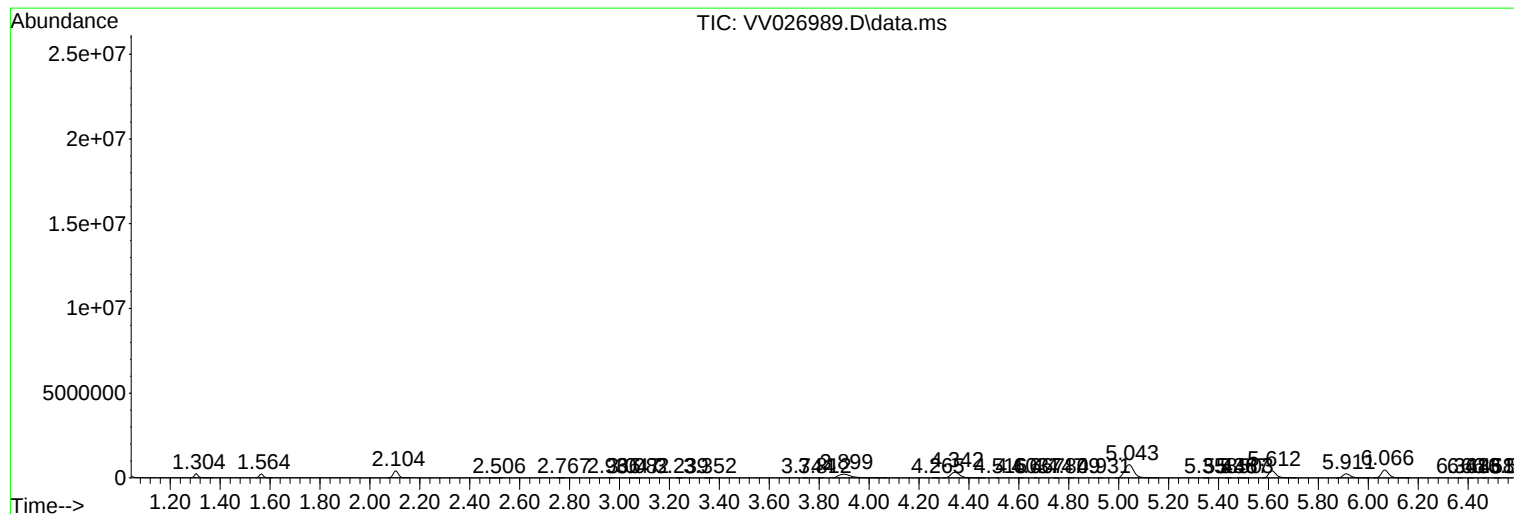

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026989.D
Acq On : 27 Jul 2022 07:00
Operator : SY/MD
Sample : N3880-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026989.D
Acq On : 27 Jul 2022 07:00
Operator : SY/MD
Sample : N3880-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc