

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026990.D
 Acq On : 27 Jul 2022 07:25
 Operator : SY/MD
 Sample : N3843-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV026990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	256320	265345	12.86%	1.719%
2	1.565	156	163	178	rBV	238221	268077	12.99%	1.737%
3	2.105	320	331	345	rBV	467650	672353	32.57%	4.357%
4	2.648	496	500	502	rBV2	342	276	0.01%	0.002%
5	3.118	644	646	650	rVB3	241	115	0.01%	0.001%
6	3.143	651	654	660	rVV	258	222	0.01%	0.001%
7	3.384	726	729	732	rBV2	387	293	0.01%	0.002%
8	3.458	748	752	753	rBV	332	229	0.01%	0.001%
9	3.638	803	808	813	rBV2	627	571	0.03%	0.004%
10	3.677	817	820	822	rBV3	344	239	0.01%	0.002%
11	3.806	858	860	862	rVB	204	85	0.00%	0.001%
12	3.818	862	864	869	rBV3	270	223	0.01%	0.001%
13	3.847	869	873	875	rBV	380	263	0.01%	0.002%
14	3.886	875	885	949	rBV	137229	492590	23.87%	3.192%
15	4.343	1012	1027	1071	rVB	349416	862377	41.78%	5.588%
16	4.806	1168	1171	1172	rBV2	288	182	0.01%	0.001%
17	4.870	1188	1191	1196	rVB3	472	410	0.02%	0.003%
18	4.896	1196	1199	1202	rBV2	298	163	0.01%	0.001%
19	4.918	1202	1206	1209	rBV2	241	217	0.01%	0.001%
20	4.966	1218	1221	1222	rBV2	213	124	0.01%	0.001%
21	5.043	1227	1245	1283	rBV2	791901	2064018	100.00%	13.374%
22	5.433	1364	1366	1369	rBV	382	206	0.01%	0.001%
23	5.532	1393	1397	1400	rBV3	407	358	0.02%	0.002%
24	5.555	1402	1404	1407	rVB	548	277	0.01%	0.002%
25	5.613	1407	1422	1453	rBV	563308	1155965	56.01%	7.490%
26	5.912	1504	1515	1535	rVB5	12633	30485	1.48%	0.198%
27	6.005	1541	1544	1546	rBV2	235	166	0.01%	0.001%
28	6.018	1546	1548	1549	rVV	373	154	0.01%	0.001%
29	6.066	1549	1563	1597	rVV	476745	974829	47.23%	6.317%
30	6.365	1653	1656	1658	rBV2	237	165	0.01%	0.001%
31	6.387	1661	1663	1665	rBV	279	161	0.01%	0.001%
32	6.436	1674	1678	1680	rBV3	331	230	0.01%	0.001%
33	6.465	1680	1687	1689	rBV3	401	413	0.02%	0.003%
34	6.523	1702	1705	1706	rBV	454	235	0.01%	0.002%
35	6.548	1710	1713	1714	rBV	176	94	0.00%	0.001%
36	6.584	1720	1724	1727	rBV2	550	415	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026990.D
 Acq On : 27 Jul 2022 07:25
 Operator : SY/MD
 Sample : N3843-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.658	1739	1747	1748	rBV4	660	781	0.04%	0.005%
38	6.712	1763	1764	1765	rBV	404	95	0.00%	0.001%
39	6.738	1770	1772	1773	rBV	228	112	0.01%	0.001%
40	6.786	1784	1787	1789	rBV	149	129	0.01%	0.001%
41	6.828	1797	1800	1801	rBV2	404	174	0.01%	0.001%
42	6.863	1810	1811	1814	rBV2	332	212	0.01%	0.001%
43	6.892	1818	1820	1822	rVB2	332	166	0.01%	0.001%
44	6.908	1822	1825	1826	rBV	261	115	0.01%	0.001%
45	6.986	1835	1849	1881	rBV	195306	372310	18.04%	2.412%
46	7.313	1939	1951	1987	rBV	830978	1486471	72.02%	9.632%
47	7.619	2037	2046	2078	rBV	140523	255412	12.37%	1.655%
48	7.802	2101	2103	2106	rVB2	746	260	0.01%	0.002%
49	7.934	2134	2144	2145	rBV4	2931	3071	0.15%	0.020%
50	7.973	2146	2156	2182	rVB	155218	269554	13.06%	1.747%
51	8.088	2182	2192	2237	rBV	504977	1014915	49.17%	6.576%
52	8.494	2315	2318	2321	rBV3	522	286	0.01%	0.002%
53	8.564	2337	2340	2342	rVB2	569	363	0.02%	0.002%
54	8.616	2353	2356	2359	rBV4	571	368	0.02%	0.002%
55	8.677	2373	2375	2381	rVB3	587	447	0.02%	0.003%
56	8.703	2381	2383	2388	rVB2	519	287	0.01%	0.002%
57	8.725	2388	2390	2393	rBV2	239	148	0.01%	0.001%
58	8.741	2393	2395	2398	rBV3	333	154	0.01%	0.001%
59	8.773	2403	2405	2407	rVB3	417	165	0.01%	0.001%
60	8.850	2417	2429	2453	rBV	889880	1456155	70.55%	9.436%
61	9.217	2540	2543	2544	rBV	403	246	0.01%	0.002%
62	9.278	2557	2562	2563	rBV	396	309	0.01%	0.002%
63	9.326	2574	2577	2578	rBV2	277	153	0.01%	0.001%
64	9.442	2610	2613	2614	rBV	477	248	0.01%	0.002%
65	9.548	2640	2646	2651	rBV3	513	678	0.03%	0.004%
66	9.645	2674	2676	2678	rBV	248	141	0.01%	0.001%
67	9.825	2729	2732	2735	rBV3	347	288	0.01%	0.002%
68	9.860	2740	2743	2746	rBV2	465	355	0.02%	0.002%
69	9.924	2758	2763	2765	rBV3	481	429	0.02%	0.003%
70	10.011	2788	2790	2794	rVB2	177	71	0.00%	0.000%
71	10.034	2794	2797	2799	rBV2	325	167	0.01%	0.001%
72	10.069	2806	2808	2811	rVB2	726	327	0.02%	0.002%
73	10.082	2811	2812	2814	rBV	175	74	0.00%	0.000%
74	10.153	2832	2834	2836	rBV	184	91	0.00%	0.001%
75	10.214	2841	2853	2879	rBV	743789	1175709	56.96%	7.618%
76	10.587	2966	2969	2970	rBV2	489	232	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026990.D
 Acq On : 27 Jul 2022 07:25
 Operator : SY/MD
 Sample : N3843-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.635	2982	2984	2985	rBV	182	67	0.00%	0.000%
78	10.677	2995	2997	2999	rBV2	202	111	0.01%	0.001%
79	10.796	3031	3034	3037	rBV3	518	355	0.02%	0.002%
80	10.850	3048	3051	3055	rVB3	759	671	0.03%	0.004%
81	10.956	3082	3084	3088	rBV2	651	238	0.01%	0.002%
82	10.985	3092	3093	3095	rVB	526	108	0.01%	0.001%
83	11.001	3095	3098	3099	rBV2	343	210	0.01%	0.001%
84	11.120	3132	3135	3138	rBV2	372	176	0.01%	0.001%
85	11.156	3144	3146	3149	rBV	215	156	0.01%	0.001%
86	11.178	3150	3153	3154	rBV2	352	191	0.01%	0.001%
87	11.246	3163	3174	3195	rBV	792728	1233734	59.77%	7.994%
88	11.535	3260	3264	3265	rBV3	1584	1073	0.05%	0.007%
89	11.622	3280	3291	3313	rBV	860900	1360808	65.93%	8.818%
90	14.014	4032	4035	4038	rBV3	681	582	0.03%	0.004%




Sum of corrected areas: 15432673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026990.D
Acq On : 27 Jul 2022 07:25
Operator : SY/MD
Sample : N3843-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

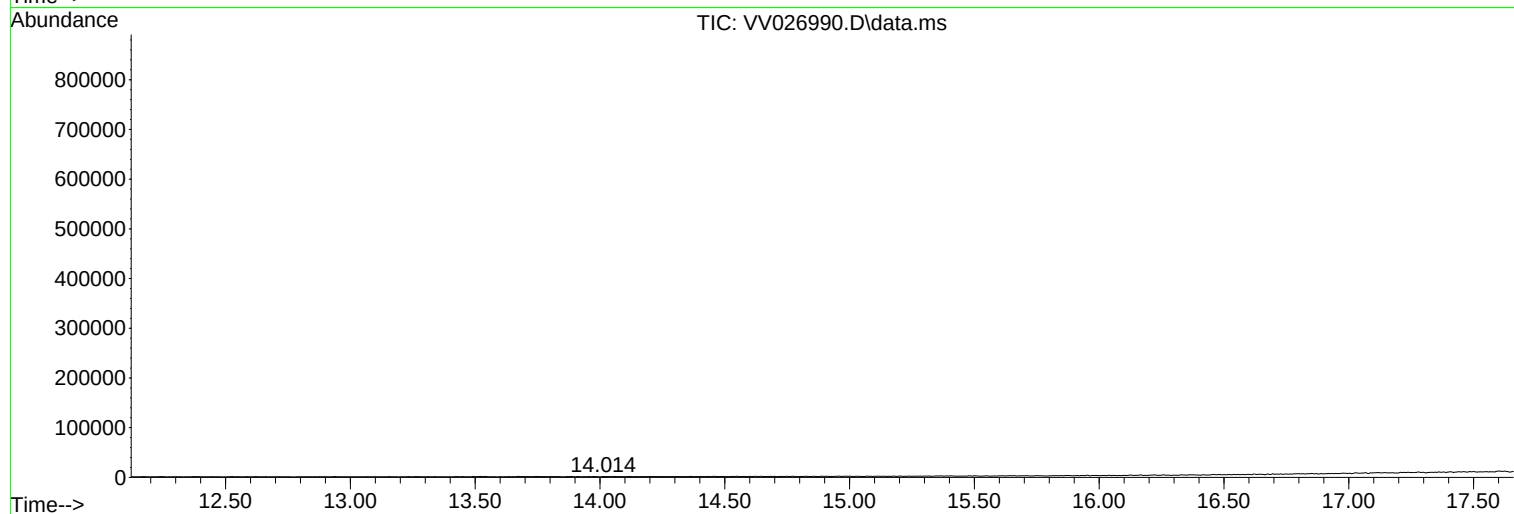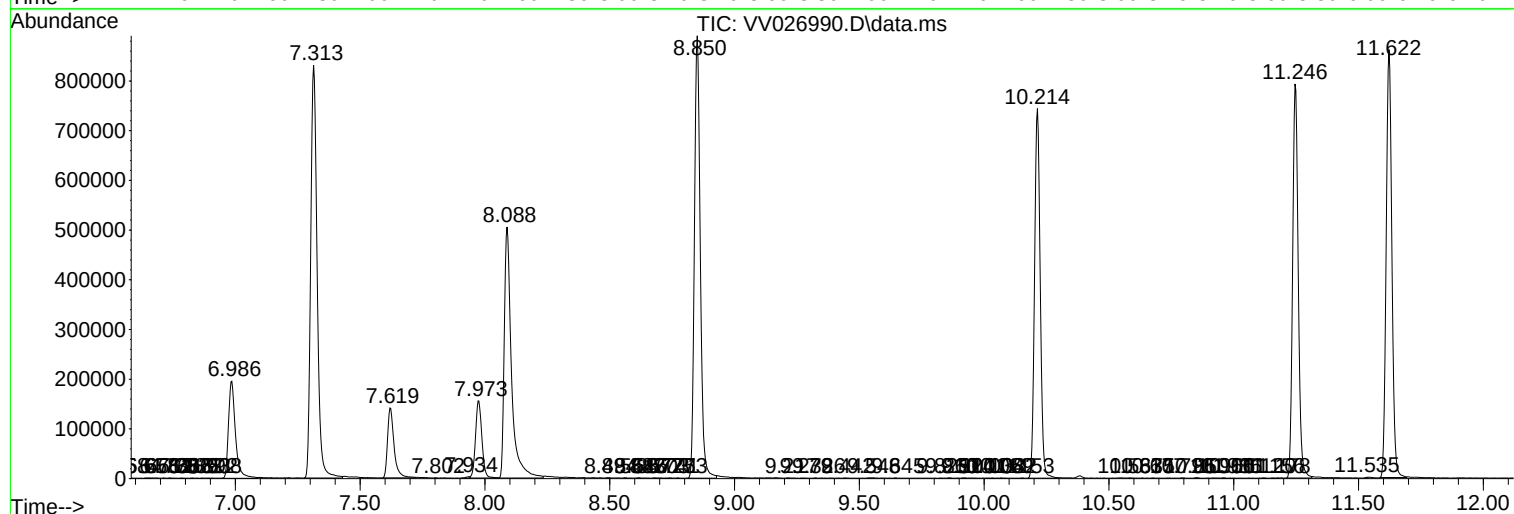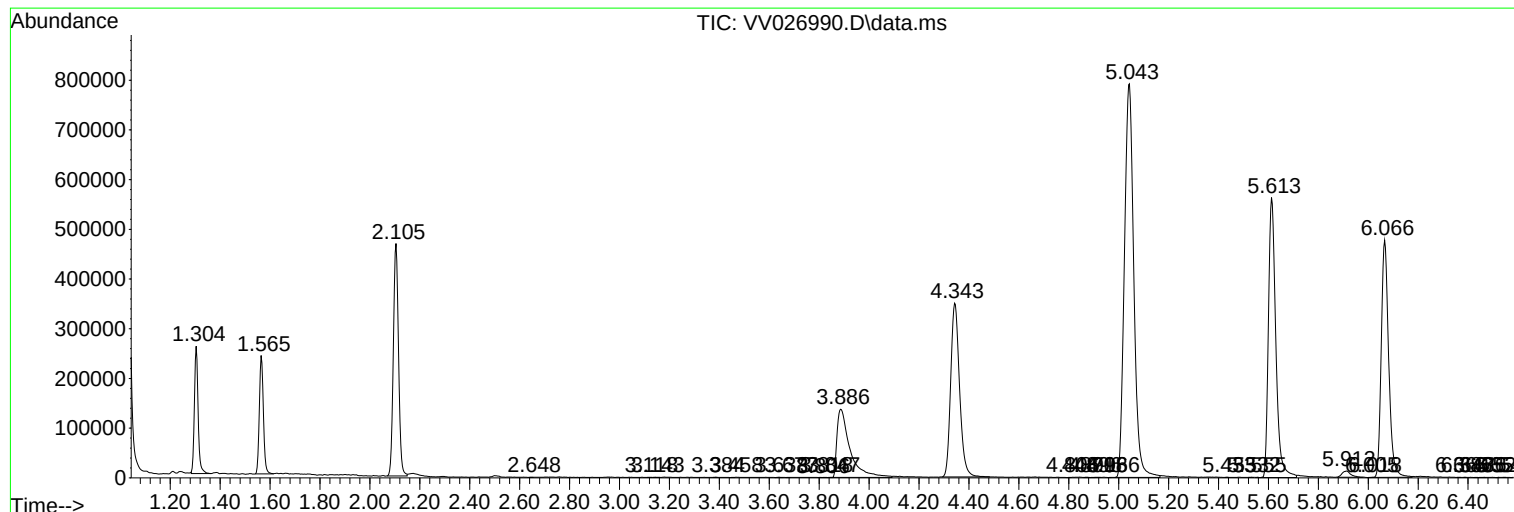

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026990.D
Acq On : 27 Jul 2022 07:25
Operator : SY/MD
Sample : N3843-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026990.D
Acq On : 27 Jul 2022 07:25
Operator : SY/MD
Sample : N3843-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc