

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026991.D
 Acq On : 27 Jul 2022 07:49
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	303396	315552	14.34%	1.965%
2	1.564	155	163	179	rBV	269117	307952	13.99%	1.918%
3	2.105	319	331	350	rBV	537137	774967	35.22%	4.827%
4	2.272	380	383	384	rBV4	752	471	0.02%	0.003%
5	2.507	446	456	466	rVB3	10029	16342	0.74%	0.102%
6	2.609	481	488	491	rBV5	1610	2265	0.10%	0.014%
7	2.709	515	519	524	rVB2	496	419	0.02%	0.003%
8	2.757	531	534	537	rBV3	1139	677	0.03%	0.004%
9	3.034	617	620	624	rBV2	266	253	0.01%	0.002%
10	3.314	704	707	713	rVB2	258	307	0.01%	0.002%
11	3.372	719	725	733	rVB3	383	570	0.03%	0.004%
12	3.410	733	737	742	rBV2	240	279	0.01%	0.002%
13	3.510	766	768	773	rVB3	374	255	0.01%	0.002%
14	3.539	773	777	780	rBV	302	298	0.01%	0.002%
15	3.671	814	818	820	rBV3	322	256	0.01%	0.002%
16	3.770	845	849	854	rVB3	402	432	0.02%	0.003%
17	3.799	854	858	861	rBV2	449	388	0.02%	0.002%
18	3.892	873	887	945	rBV2	160050	623086	28.32%	3.881%
19	4.162	969	971	973	rVB3	996	298	0.01%	0.002%
20	4.259	998	1001	1003	rBV2	488	337	0.02%	0.002%
21	4.343	1010	1027	1059	rBV	368379	915668	41.61%	5.703%
22	4.690	1130	1135	1141	rVB5	650	813	0.04%	0.005%
23	4.754	1149	1155	1156	rBV3	362	276	0.01%	0.002%
24	4.783	1162	1164	1168	rVB2	477	356	0.02%	0.002%
25	4.806	1168	1171	1173	rBV	399	280	0.01%	0.002%
26	4.822	1173	1176	1183	rVB5	672	794	0.04%	0.005%
27	4.870	1183	1191	1195	rBV4	505	668	0.03%	0.004%
28	4.931	1204	1210	1212	rBV2	678	572	0.03%	0.004%
29	5.043	1226	1245	1276	rBV2	850275	2200513	100.00%	13.706%
30	5.359	1342	1343	1349	rVB3	702	479	0.02%	0.003%
31	5.410	1355	1359	1361	rBV3	458	356	0.02%	0.002%
32	5.423	1361	1363	1368	rVB4	554	446	0.02%	0.003%
33	5.471	1372	1378	1379	rBV5	331	294	0.01%	0.002%
34	5.613	1409	1422	1464	rBV	554920	1153096	52.40%	7.182%
35	5.847	1491	1495	1498	rVV4	669	496	0.02%	0.003%
36	5.863	1498	1500	1502	rVV2	521	272	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072622\
 Data File : VW026991.D
 Acq On : 27 Jul 2022 07:49
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	5.908	1503	1514	1533	rVB5	15504	35205	1.60%	0.219%
38	6.066	1549	1563	1598	rBV	494923	1015756	46.16%	6.327%
39	6.301	1634	1636	1640	rVB3	716	384	0.02%	0.002%
40	6.371	1656	1658	1663	rVB2	424	314	0.01%	0.002%
41	6.580	1720	1723	1726	rVV	391	258	0.01%	0.002%
42	6.596	1726	1728	1736	rVB4	498	421	0.02%	0.003%
43	6.654	1741	1746	1749	rBV3	625	468	0.02%	0.003%
44	6.796	1784	1790	1791	rBV2	299	255	0.01%	0.002%
45	6.986	1837	1849	1870	rBV	203055	376244	17.10%	2.344%
46	7.313	1939	1951	1986	rBV	918867	1612843	73.29%	10.046%
47	7.619	2036	2046	2071	rBV	142407	262432	11.93%	1.635%
48	7.902	2131	2134	2136	rBV	562	306	0.01%	0.002%
49	7.931	2140	2143	2145	rBV2	616	453	0.02%	0.003%
50	7.976	2146	2157	2177	rVB	93190	161563	7.34%	1.006%
51	8.088	2181	2192	2227	rBV	499967	987339	44.87%	6.150%
52	8.420	2290	2295	2305	rVV8	1704	2761	0.13%	0.017%
53	8.461	2305	2308	2312	rVB3	962	695	0.03%	0.004%
54	8.532	2328	2330	2332	rBV	443	253	0.01%	0.002%
55	8.587	2342	2347	2351	rBV3	601	535	0.02%	0.003%
56	8.850	2417	2429	2458	rBV	891402	1456996	66.21%	9.075%
57	9.249	2549	2553	2557	rBV3	353	252	0.01%	0.002%
58	9.365	2586	2589	2592	rVB	369	253	0.01%	0.002%
59	9.506	2629	2633	2637	rBV2	366	274	0.01%	0.002%
60	9.635	2665	2673	2677	rBV3	375	632	0.03%	0.004%
61	9.680	2684	2687	2692	rVB2	523	452	0.02%	0.003%
62	9.741	2700	2706	2711	rBV3	234	260	0.01%	0.002%
63	9.860	2739	2743	2748	rVV3	465	503	0.02%	0.003%
64	9.947	2767	2770	2775	rVB4	372	260	0.01%	0.002%
65	10.214	2837	2853	2876	rBV	738460	1166615	53.02%	7.267%
66	10.371	2899	2902	2904	rBV2	648	481	0.02%	0.003%
67	10.416	2913	2916	2917	rBV2	572	295	0.01%	0.002%
68	10.554	2949	2959	2962	rVV3	594	866	0.04%	0.005%
69	10.587	2967	2969	2975	rVB3	484	330	0.01%	0.002%
70	10.809	3034	3038	3040	rBV3	327	264	0.01%	0.002%
71	11.008	3096	3100	3106	rVV2	364	399	0.02%	0.002%
72	11.046	3106	3112	3116	rVB3	460	496	0.02%	0.003%
73	11.085	3120	3124	3127	rBV3	300	358	0.02%	0.002%
74	11.246	3163	3174	3198	rBV	795360	1231674	55.97%	7.672%
75	11.622	3278	3291	3311	rBV	894155	1403324	63.77%	8.741%
76	11.818	3349	3352	3356	rVB4	518	353	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
 Data File : VV026991.D
 Acq On : 27 Jul 2022 07:49
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.908	3375	3380	3384	rVB	599	572	0.03%	0.004%
78	11.934	3385	3388	3394	rVB3	325	254	0.01%	0.002%
79	12.053	3422	3425	3429	rBV2	359	302	0.01%	0.002%
80	12.497	3560	3563	3571	rBV2	450	658	0.03%	0.004%
81	12.561	3579	3583	3586	rBV2	482	408	0.02%	0.003%
82	12.776	3645	3650	3655	rBV2	421	542	0.02%	0.003%
83	12.802	3655	3658	3661	rVV2	410	317	0.01%	0.002%
84	13.053	3733	3736	3740	rVB2	440	321	0.01%	0.002%
85	13.130	3759	3760	3764	rVB	818	297	0.01%	0.002%
86	13.207	3778	3784	3788	rBV2	465	489	0.02%	0.003%
87	13.226	3788	3790	3791	rVV2	498	261	0.01%	0.002%
88	13.410	3845	3847	3851	rBV3	476	347	0.02%	0.002%
89	13.442	3852	3857	3860	rVB2	682	646	0.03%	0.004%
90	13.461	3860	3863	3865	rBV2	422	293	0.01%	0.002%
91	13.525	3878	3883	3888	rBV3	867	1000	0.05%	0.006%
92	13.593	3901	3904	3906	rBV2	498	290	0.01%	0.002%
93	13.751	3951	3953	3959	rBV2	374	335	0.02%	0.002%
94	13.882	3991	3994	3997	rBV2	394	293	0.01%	0.002%
95	13.963	4014	4019	4024	rBV4	450	661	0.03%	0.004%
96	14.432	4163	4165	4168	rBV3	390	261	0.01%	0.002%
97	14.805	4279	4281	4284	rVB2	489	291	0.01%	0.002%
98	14.866	4297	4300	4304	rVB3	430	267	0.01%	0.002%
99	14.998	4338	4341	4344	rBV2	564	479	0.02%	0.003%
100	15.111	4374	4376	4380	rBV2	548	413	0.02%	0.003%

Sum of corrected areas: 16054602




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026991.D
Acq On : 27 Jul 2022 07:49
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

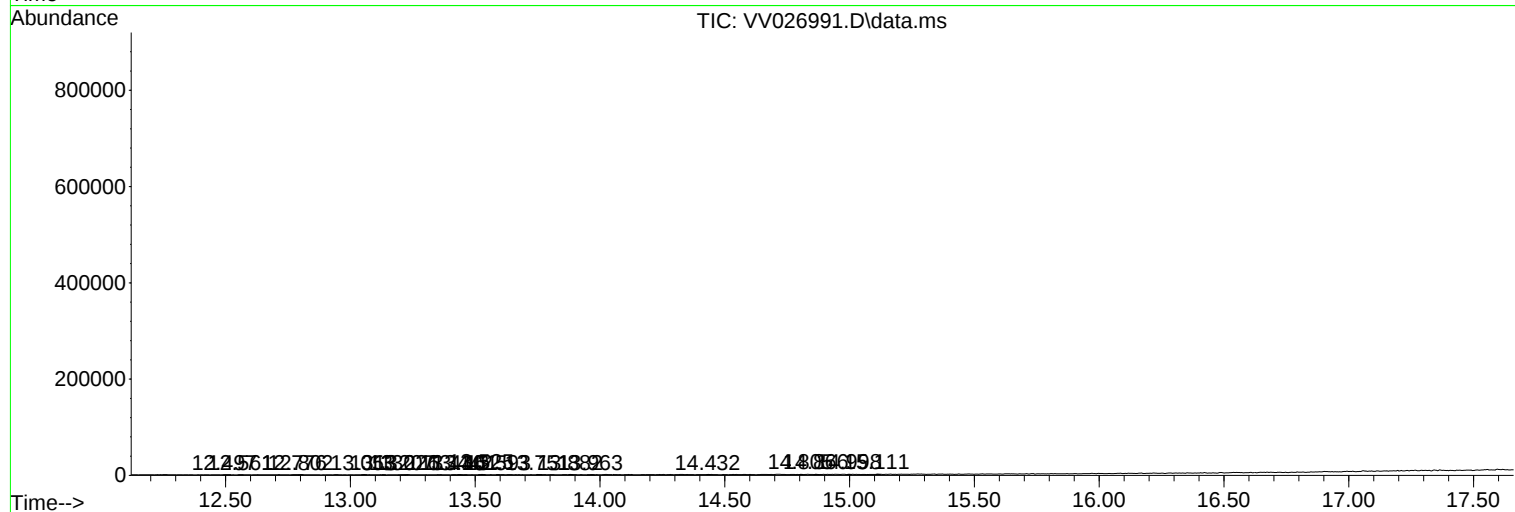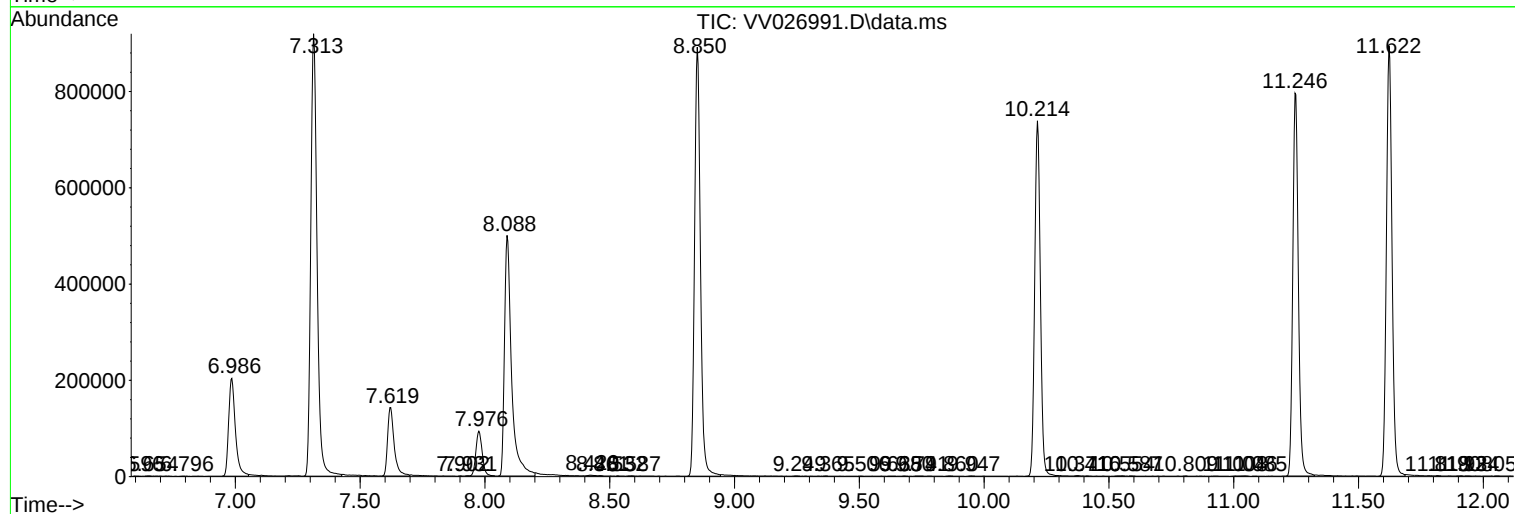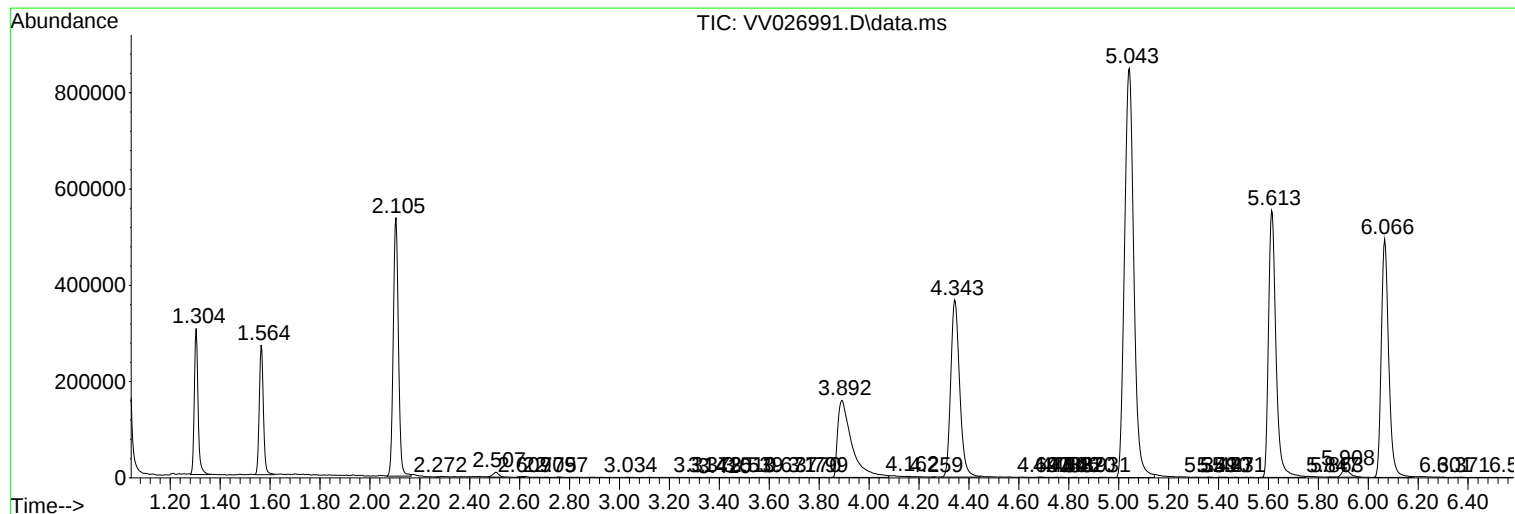

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026991.D
Acq On : 27 Jul 2022 07:49
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026991.D
Acq On : 27 Jul 2022 07:49
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc