
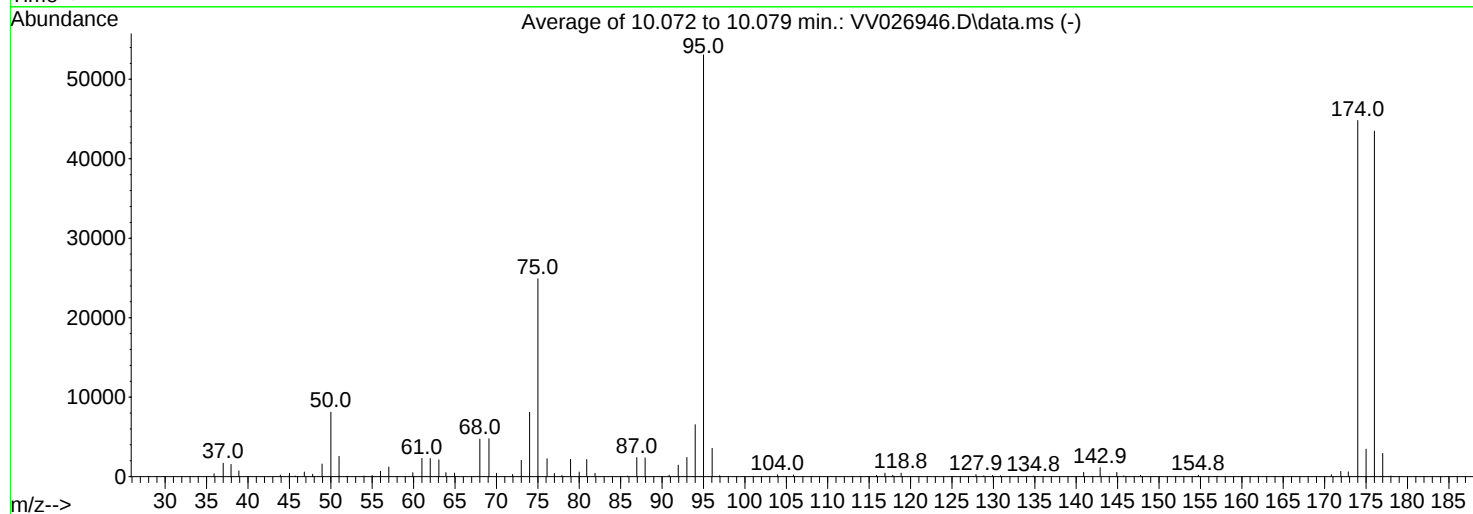


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072622\
Data File : VV026946.D
Acq On : 26 Jul 2022 11:01
Operator : SY/MD
Sample : BFB299
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB299

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis
Last Update : Thu Jul 28 02:51:09 2022

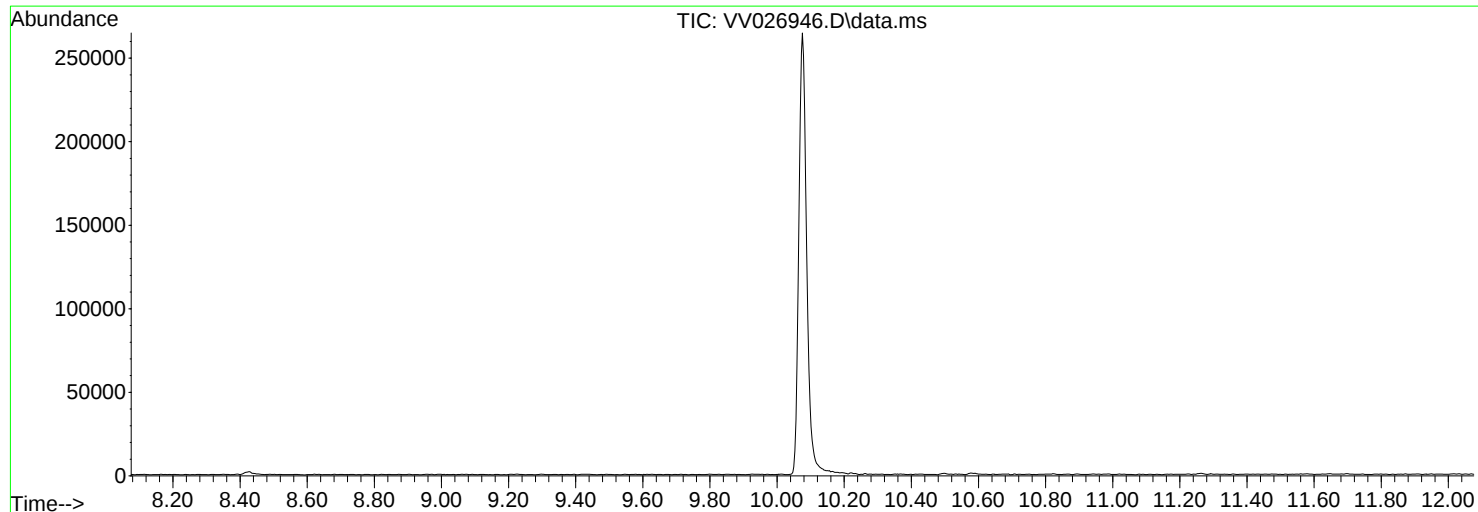

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	8114	PASS
75	95	30	80	46.9	24912	PASS
95	95	100	100	100.0	53072	PASS
96	95	5	9	6.7	3574	PASS
173	174	0.00	2	1.4	614	PASS
174	95	50	120	84.5	44824	PASS
175	174	5	9	7.7	3454	PASS
176	174	95	105	97.0	43485	PASS
177	176	5	10	6.7	2924	PASS

m/z	Abundance
39.90	380.0
43.90	470.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
35.90	382.0
37.00	1691.0
38.00	1563.0
38.90	804.0
39.90	428.0
43.90	642.0
45.00	428.0
46.80	653.0
47.80	244.0
48.90	1633.0
50.00	8367.0
51.00	2633.0
51.90	114.0
55.00	147.0
56.00	646.0
57.00	1252.0
59.90	500.0
61.00	2386.0
62.00	2215.0
63.10	2052.0
63.90	558.0
64.90	471.0
68.00	4751.0
69.10	4906.0
70.00	444.0
71.90	323.0
73.00	2033.0
74.00	8189.0
75.00	25328.0
76.10	2289.0
76.90	360.0
78.90	2010.0
80.00	533.0
80.90	2061.0
81.90	343.0
87.00	2427.0
87.90	2530.0
90.90	179.0
91.90	1454.0
93.00	2448.0
94.00	6386.0
95.00	52528.0
96.00	3595.0
96.90	104.0
103.90	199.0
105.90	265.0
115.90	144.0
116.90	444.0
117.90	201.0
118.80	463.0
127.90	305.0
128.80	117.0
129.90	147.0
130.80	118.0
140.90	532.0
142.90	1158.0
144.80	605.0
145.80	100.0
147.70	156.0
154.80	176.0
170.80	232.0
172.00	617.0
172.90	604.0
174.00	43232.0
175.00	3432.0
176.00	42128.0
177.00	2800.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
35.90	364.0
37.00	1760.0
38.00	1597.0
38.90	737.0
39.90	397.0
43.90	672.0
45.00	442.0
45.70	110.0
46.80	620.0
47.80	307.0
49.00	1654.0
50.00	8344.0
51.00	2661.0
54.00	119.0
55.00	125.0
56.00	707.0
57.00	1264.0
59.90	516.0
61.00	2372.0
62.00	2339.0
63.00	2180.0
63.90	536.0
65.00	466.0
68.00	4919.0
69.10	4929.0
70.00	448.0
72.00	272.0
73.00	2114.0
74.00	8373.0
75.00	25600.0
76.10	2308.0
77.00	432.0
77.90	223.0
78.90	2238.0
80.00	590.0
80.90	2220.0
81.90	429.0
85.80	103.0
87.00	2444.0
87.90	2371.0
90.90	205.0
92.00	1495.0
93.00	2544.0
94.00	6771.0
95.00	54912.0
96.00	3721.0
96.90	121.0
103.90	244.0
105.90	198.0
115.90	171.0
116.90	437.0
117.80	178.0
118.90	464.0
127.90	274.0
128.90	135.0
129.90	162.0
130.80	128.0
134.90	111.0
140.90	569.0
142.90	1191.0
144.90	558.0
145.80	108.0
147.80	157.0
154.80	208.0
156.70	106.0
170.80	257.0
172.00	695.0
172.80	632.0
174.00	46240.0
175.00	3626.0
176.00	44952.0
177.00	3067.0
178.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
35.90	359.0
37.00	1598.0
37.90	1511.0
38.90	650.0
39.90	361.0
44.00	673.0
45.00	403.0
45.70	135.0
46.80	485.0
47.80	345.0
49.00	1479.0
50.00	7630.0
51.00	2402.0
54.00	129.0
55.00	126.0
56.00	687.0
57.00	1142.0
59.90	465.0
61.00	2125.0
62.00	2261.0
63.00	2091.0
63.90	439.0
65.00	392.0
68.00	4533.0
69.10	4483.0
70.00	372.0
72.00	237.0
73.00	2010.0
74.00	7790.0
75.00	23808.0
76.10	2188.0
77.10	411.0
77.90	228.0
79.00	2273.0
80.00	632.0
80.90	2162.0
81.90	489.0
85.90	118.0
86.90	2334.0
88.00	2152.0
90.80	177.0
92.00	1433.0
93.00	2271.0
94.00	6493.0
95.00	51776.0
96.10	3406.0
97.00	133.0
104.00	278.0
104.70	101.0
105.70	138.0
115.90	183.0
116.90	430.0
117.90	180.0
118.90	419.0
127.90	229.0
128.90	119.0
129.90	168.0
130.90	140.0
134.80	140.0
140.90	517.0
142.90	1025.0
145.00	496.0
145.70	109.0
147.80	144.0
154.70	171.0
157.10	116.0
170.80	255.0
171.90	698.0
172.80	606.0
174.00	45000.0
175.00	3303.0
176.00	43376.0
177.00	2905.0
178.00	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299