

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031764.D
 Acq On : 26 Jul 2023 13:15
 Operator : SY/MD
 Sample : 03712-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 27 05:20:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	346289	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	356456	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	160882	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	141497	40.082	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.160%
7) Chloroethane-d5	1.532	69	138250	42.734	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.460%
11) 1,1-Dichloroethene-d2	2.060	65	66638	40.780	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.560%
21) 2-Butanone-d5	3.790	46	214680	87.884	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.880%
24) Chloroform-d	4.256	84	319156	43.974	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.940%
26) 1,2-Dichloroethane-d4	4.947	65	206000	45.617	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.240%
32) Benzene-d6	4.966	84	516390	45.749	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.500%
36) 1,2-Dichloropropane-d6	5.992	67	199585	47.072	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.140%
41) Toluene-d8	7.249	98	381439	40.316	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.640%
43) trans-1,3-Dichloroprop...	7.558	79	74744	41.013	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.020%
47) 2-Hexanone-d5	8.031	63	129630	81.529	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.530%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	241436	41.328	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.660%
66) 1,2-Dichlorobenzene-d4	11.567	152	171159	52.545	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.080%
Target Compounds						
13) Acetone	2.114	43	44523	19.042	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031764.D
Acq On : 26 Jul 2023 13:15
Operator : SY/MD
Sample : 03712-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 27 05:20:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

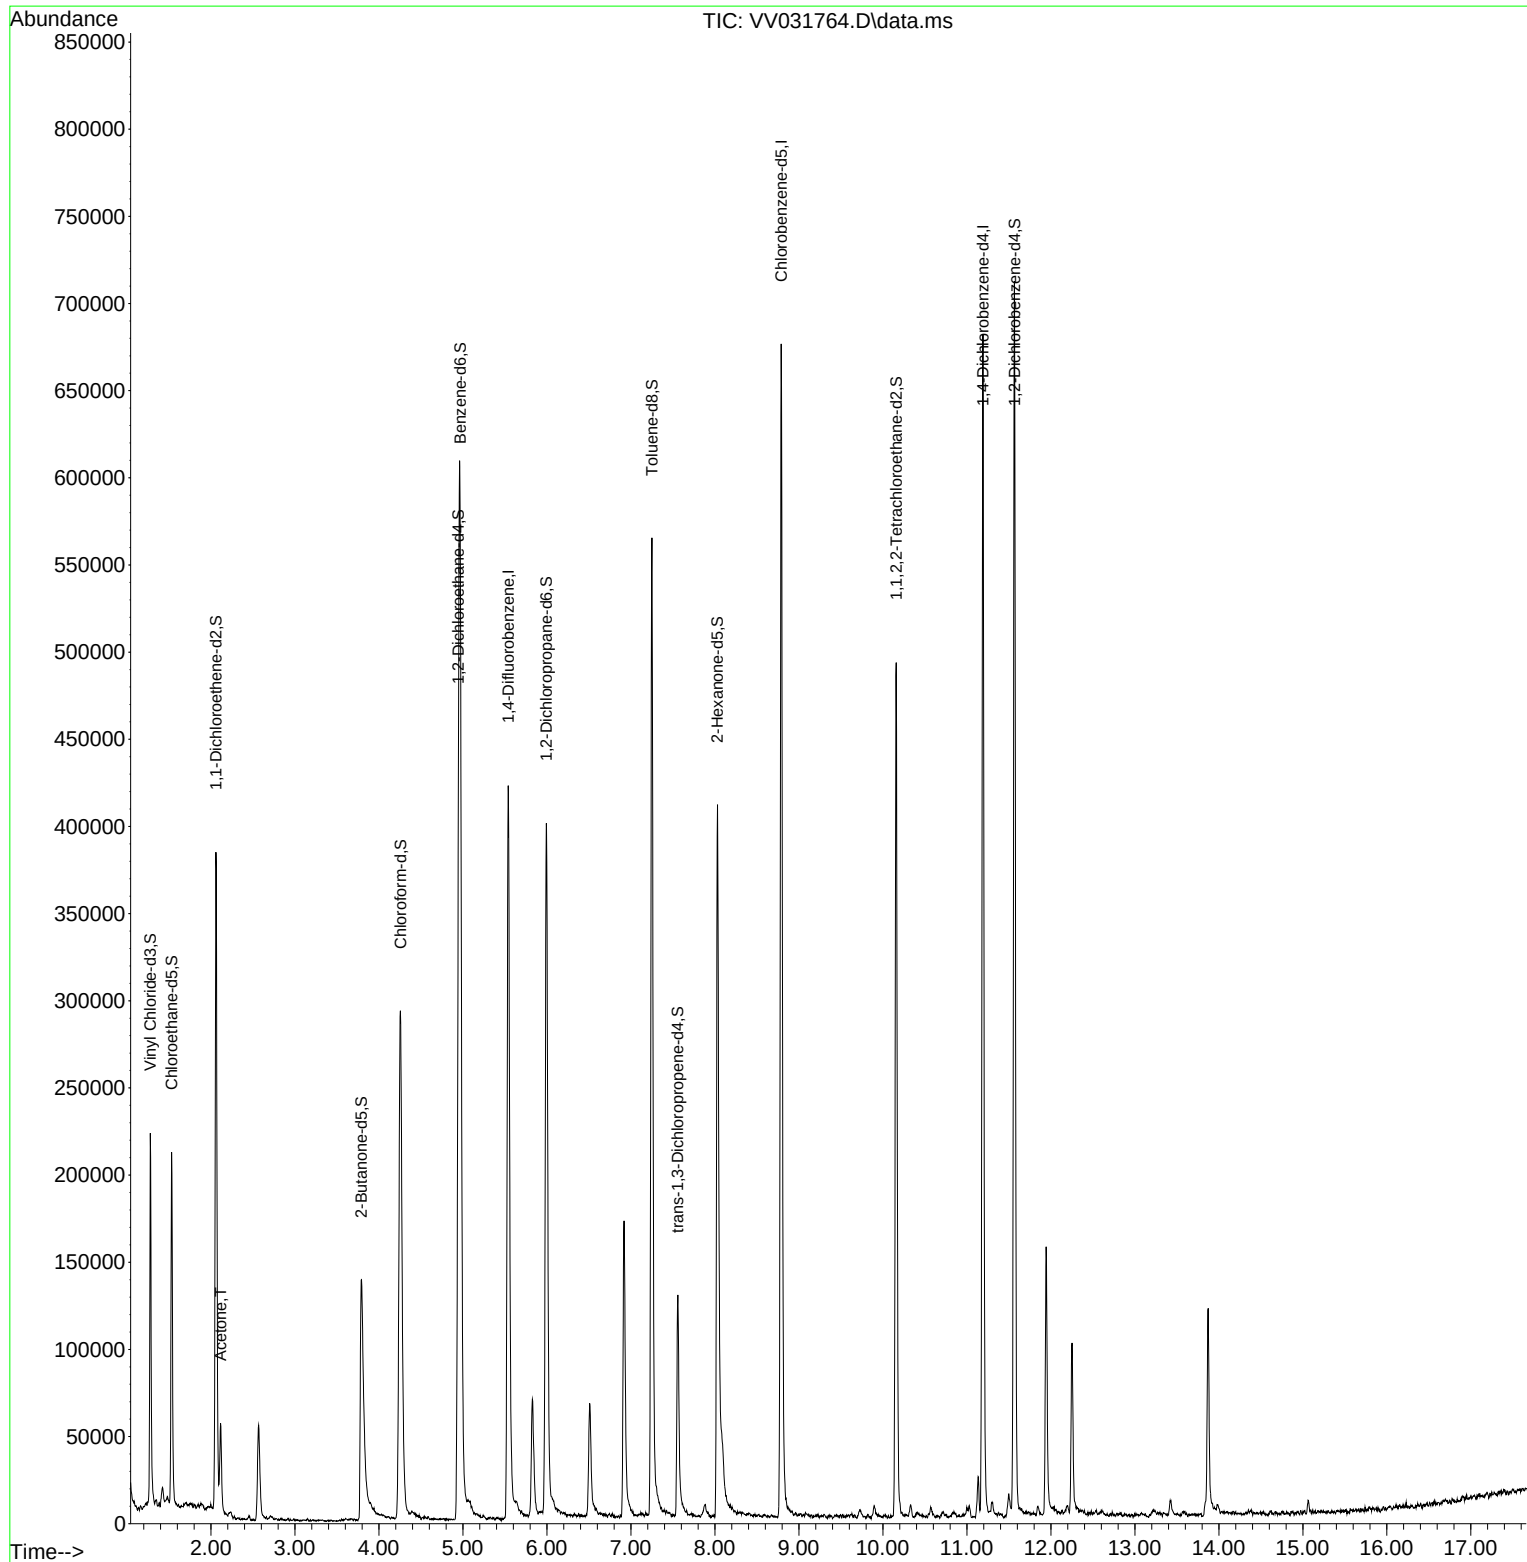

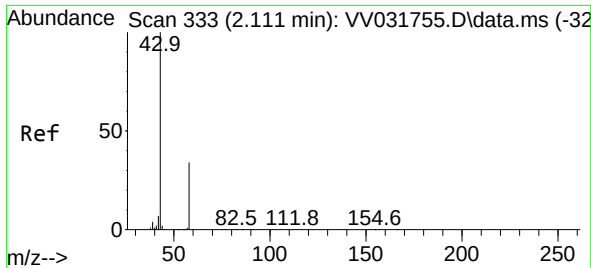

#13

Acetone

Concen: 19.042 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min


Lab File: VV031764.D

Acq: 26 Jul 2023 13:15

Instrument :

MSVOA_V

ClientSampleId :

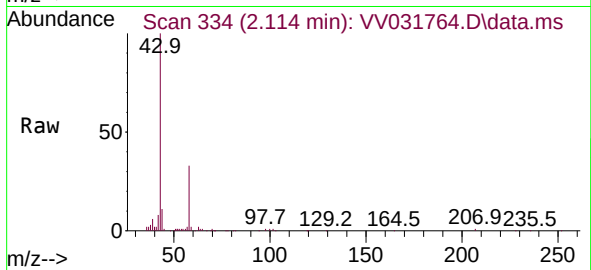

Tgt Ion: 43 Resp: 44523

Ion Ratio Lower Upper

43 100

58 35.5 0.0 72.0

