

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031768.D
 Acq On : 26 Jul 2023 14:49
 Operator : SY/MD
 Sample : 03754-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 27 05:21:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	320484	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	350761	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	155330	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	148719	45.520	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	91.040%	
7) Chloroethane-d5	1.532	69	141106	47.129	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.260%	
11) 1,1-Dichloroethene-d2	2.060	65	65629	43.397	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.800%	
21) 2-Butanone-d5	3.789	46	233352	103.220	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.220%	
24) Chloroform-d	4.256	84	320192	47.669	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.340%	
26) 1,2-Dichloroethane-d4	4.947	65	203760	48.754	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.500%	
32) Benzene-d6	4.966	84	506637	45.613	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.220%	
36) 1,2-Dichloropropane-d6	5.995	67	202124	48.445	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.880%	
41) Toluene-d8	7.249	98	384063	41.253	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.500%	
43) trans-1,3-Dichloroprop...	7.558	79	78439	43.739	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.480%	
47) 2-Hexanone-d5	8.030	63	138046	88.231	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	88.230%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	279683	48.652	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.300%	
66) 1,2-Dichlorobenzene-d4	11.567	152	168071	53.441	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.880%	
Target Compounds						
39) cis-1,3-Dichloropropene	6.924	75	4766	0.916	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031768.D
Acq On : 26 Jul 2023 14:49
Operator : SY/MD
Sample : 03754-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 27 05:21:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

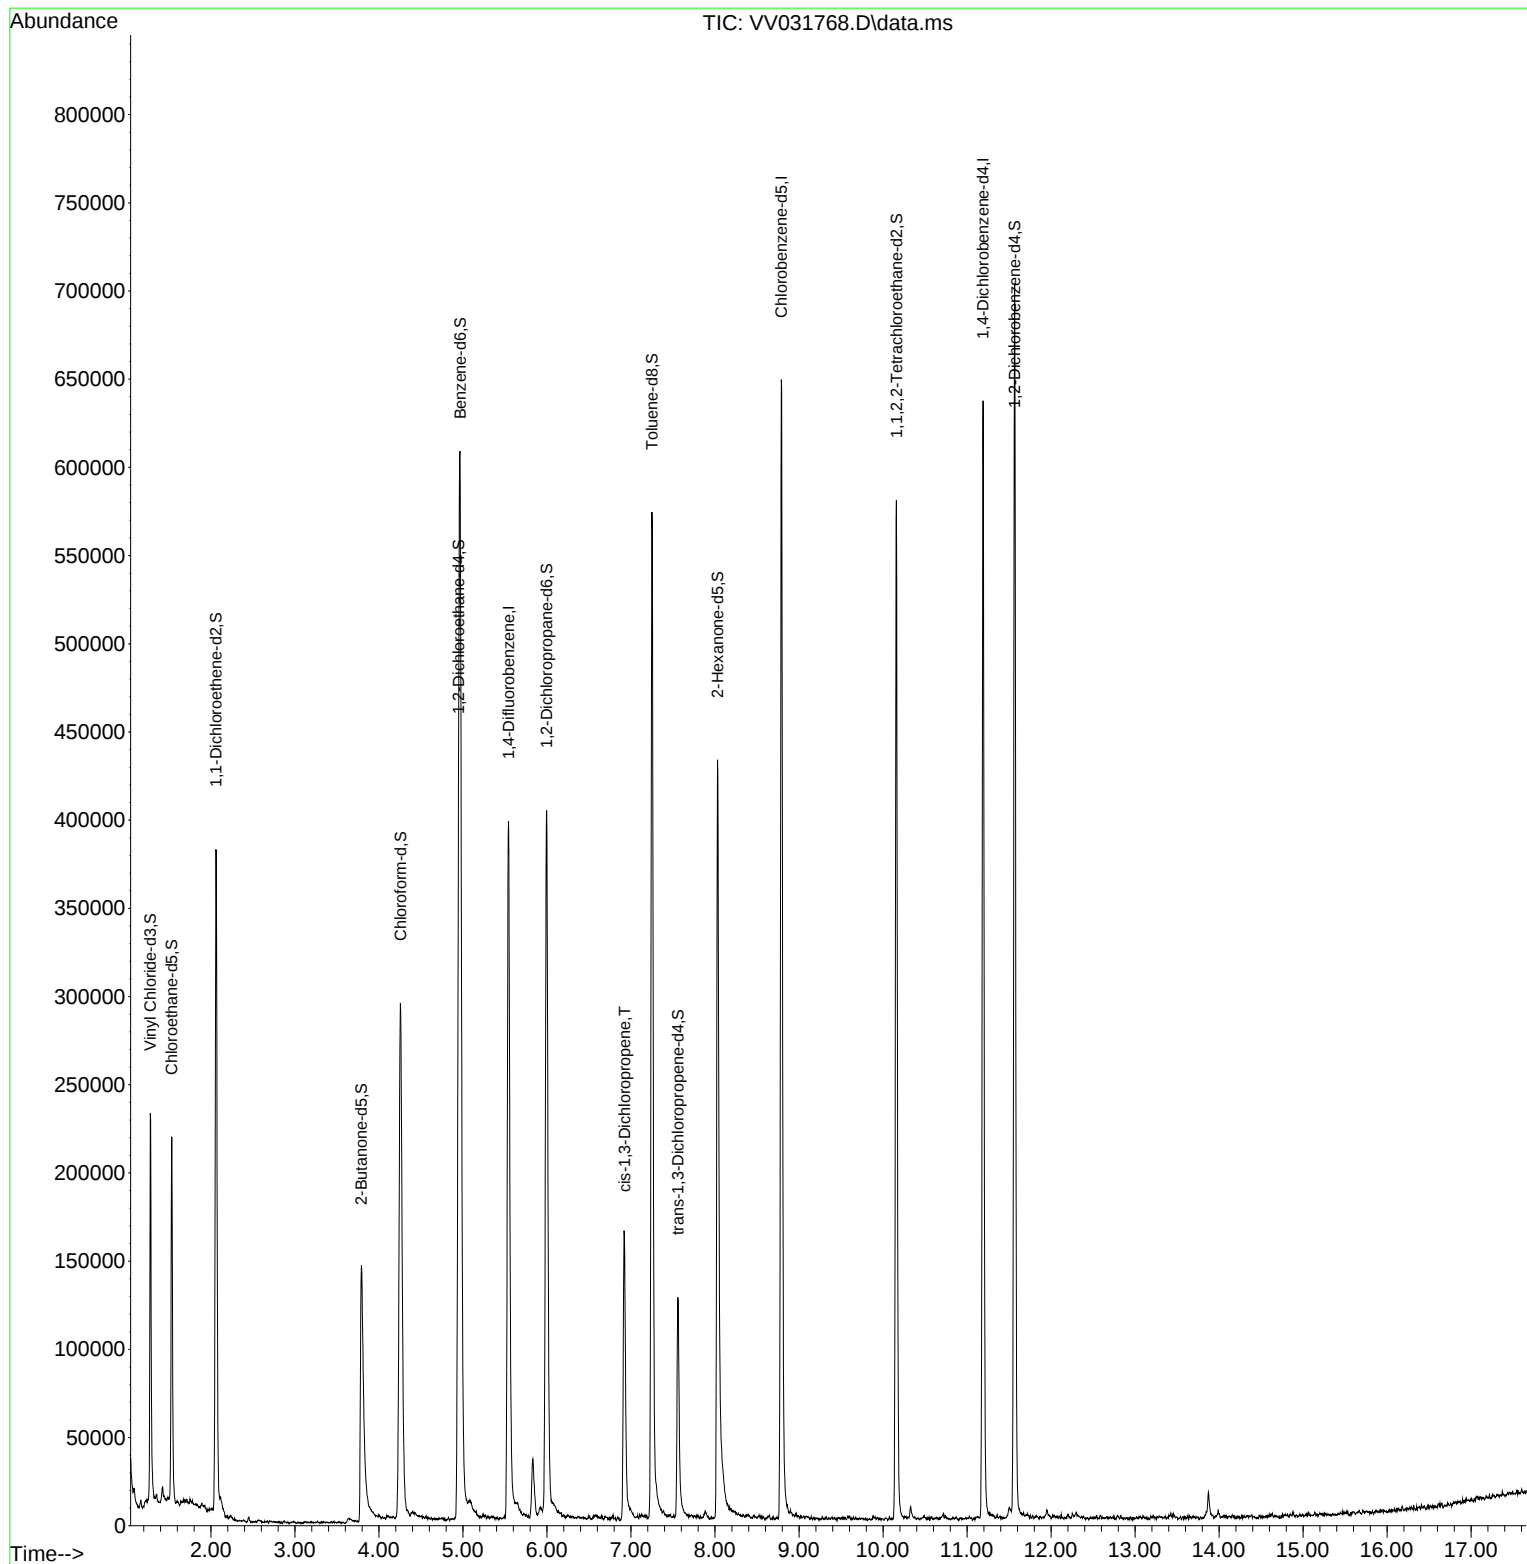

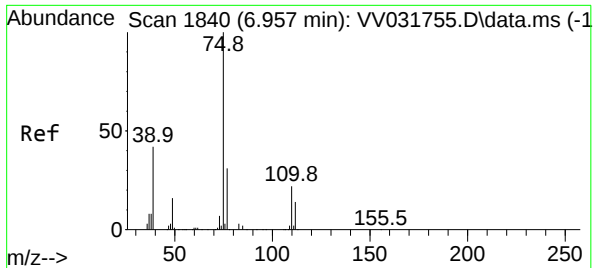

#39
 cis-1,3-Dichloropropene
 Concen: 0.916 ug/L
 RT: 6.924 min Scan# 11
 Delta R.T. -0.032 min
 Lab File: VV031768.D
 Acq: 26 Jul 2023 14:49

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4766
 Ion Ratio Lower Upper
 75 100
 77 37.1 22.1 41.1

