

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031772.D
 Acq On : 26 Jul 2023 16:23
 Operator : SY/MD
 Sample : 03712-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 27 05:22:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	302658	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	335587	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	154738	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	153670	49.805	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 99.620%			
7) Chloroethane-d5	1.532	69	144398	51.069	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 102.140%			
11) 1,1-Dichloroethene-d2	2.060	65	69393	48.588	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.180%			
21) 2-Butanone-d5	3.793	46	220649	103.349	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 103.350%			
24) Chloroform-d	4.256	84	318629	50.230	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.460%			
26) 1,2-Dichloroethane-d4	4.947	65	203842	51.646	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.300%			
32) Benzene-d6	4.966	84	501851	47.225	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 94.460%			
36) 1,2-Dichloropropane-d6	5.995	67	194596	48.749	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 97.500%			
41) Toluene-d8	7.249	98	381566	42.838	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 85.680%			
43) trans-1,3-Dichloroprop...	7.558	79	76264	44.449	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 88.900%			
47) 2-Hexanone-d5	8.030	63	137262	91.697	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 91.700%			
56) 1,1,2,2-Tetrachloroeth...	10.159	84	280130	50.933	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 101.860%			
66) 1,2-Dichlorobenzene-d4	11.567	152	177033	56.506	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 113.020%			
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	5.828	63	2176	0.621	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031772.D
Acq On : 26 Jul 2023 16:23
Operator : SY/MD
Sample : 03712-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 27 05:22:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

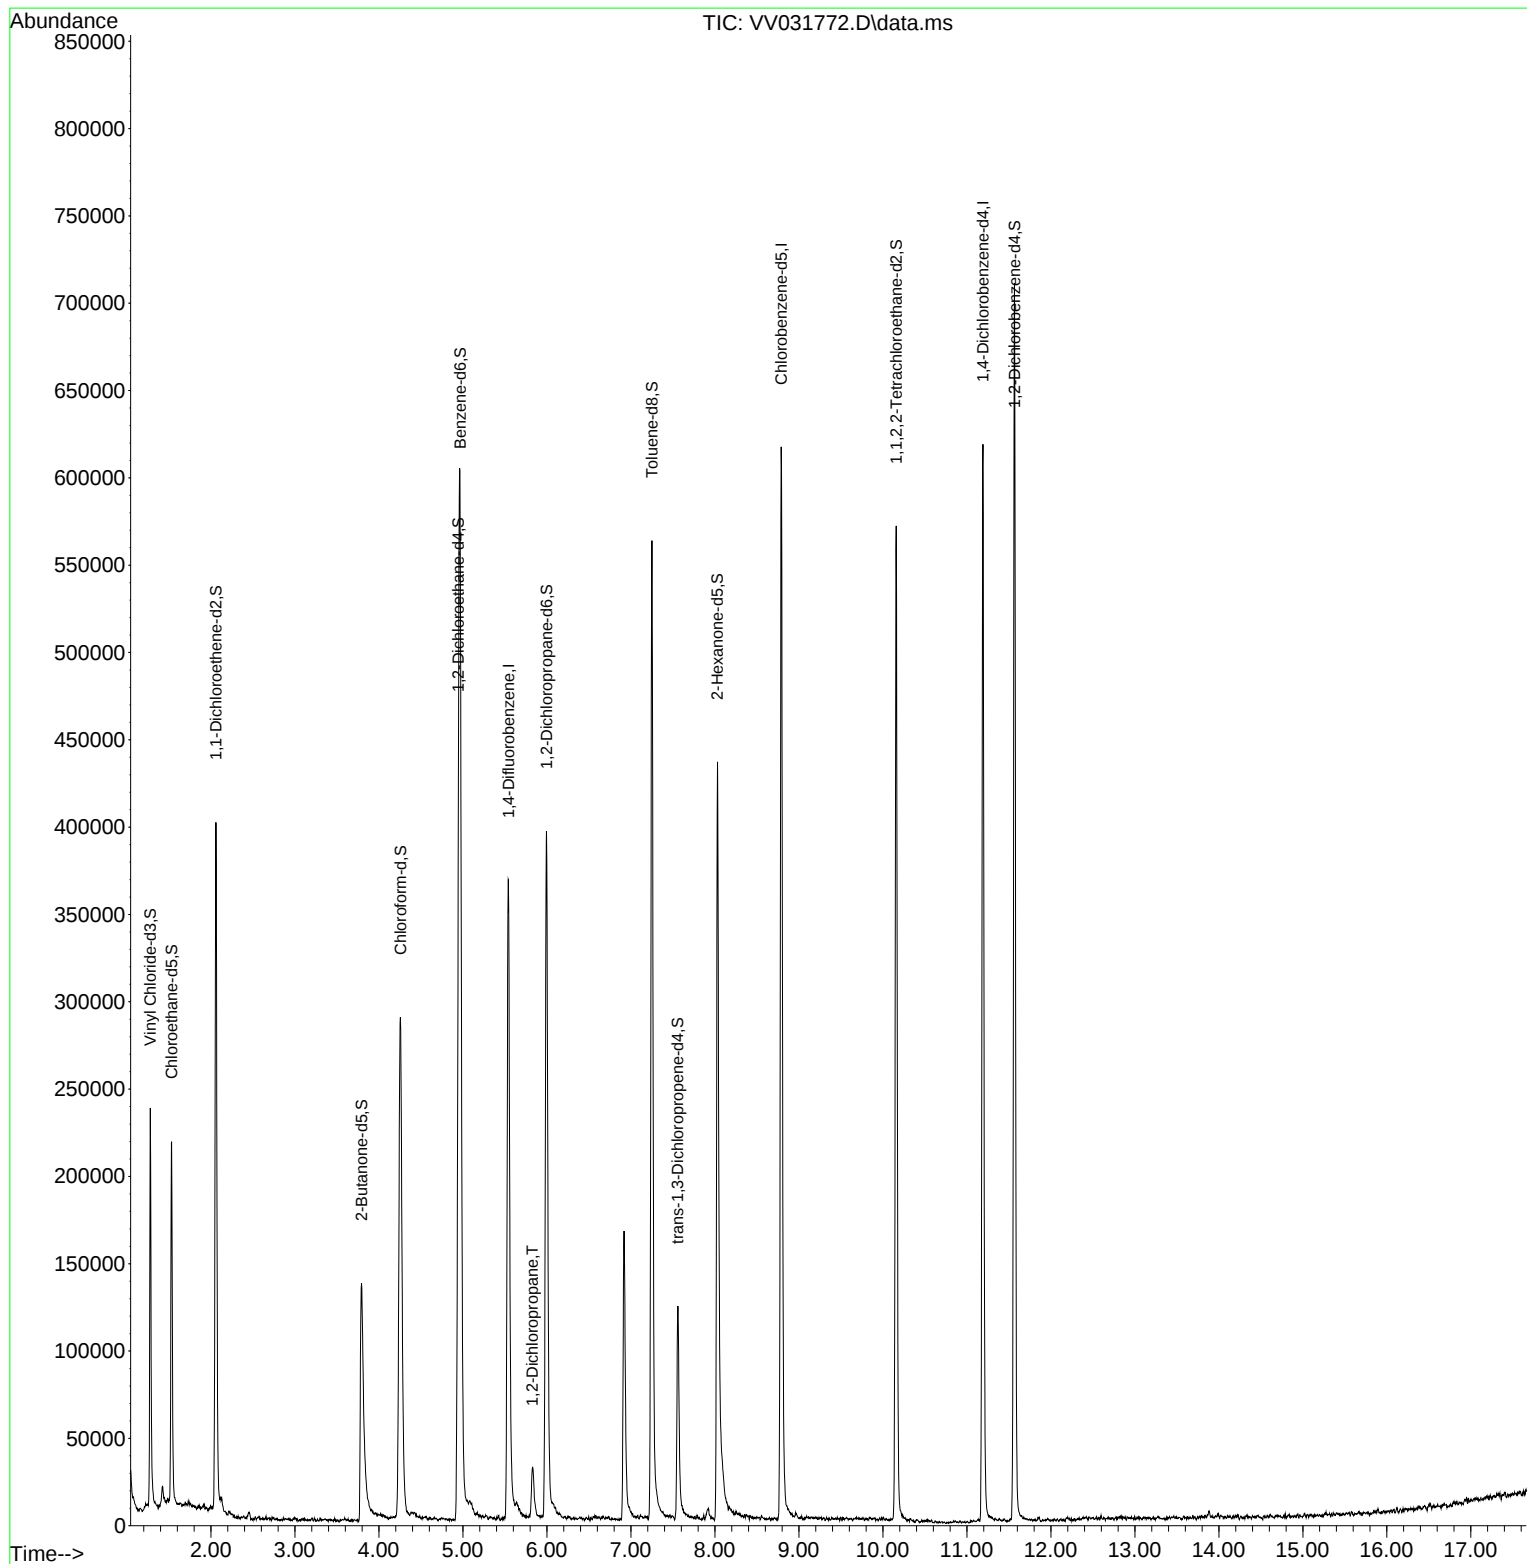

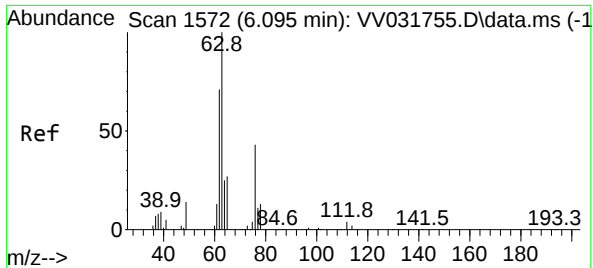

#37
 1,2-Dichloropropane
 Concen: 0.621 ug/L
 RT: 5.828 min Scan# 14
 Delta R.T. -0.267 min
 Lab File: VV031772.D
 Acq: 26 Jul 2023 16:23

Instrument :
 MSVOA_V
 ClientSampleId :

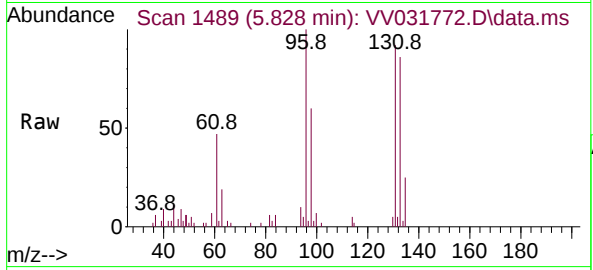

Tgt Ion:	63	Resp:	2176
Ion Ratio	Lower	Upper	
63	100		
112	4.3	3.7	5.5

