

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031761.D
 Acq On : 26 Jul 2023 12:05
 Operator : SY/MD
 Sample : 03754-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X5

Quant Time: Jul 27 05:40:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	245213	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	268656	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	120103	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	156101	62.446	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 124.900%		
7) Chloroethane-d5	1.532	69	142259	62.099	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 124.200%		
11) 1,1-Dichloroethene-d2	2.063	65	67096	57.986	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 115.980%		
21) 2-Butanone-d5	3.789	46	219184	126.714	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 126.710%		
24) Chloroform-d	4.256	84	325543	63.342	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 126.680%#		
26) 1,2-Dichloroethane-d4	4.947	65	212640	66.496	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 133.000%#		
32) Benzene-d6	4.966	84	522685	61.440	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 122.880%		
36) 1,2-Dichloropropane-d6	5.992	67	202852	63.478	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 126.960%#		
41) Toluene-d8	7.249	98	393839	55.231	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 110.460%		
43) trans-1,3-Dichloroprop...	7.558	79	82128	59.792	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 119.580%		
47) 2-Hexanone-d5	8.030	63	132960	110.952	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 110.950%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	287564	65.311	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 130.620%#		
66) 1,2-Dichlorobenzene-d4	11.567	152	180281	74.137	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 148.280%#		
Target Compounds						
13) Acetone	2.114	43	64229	38.793	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031761.D
Acq On : 26 Jul 2023 12:05
Operator : SY/MD
Sample : 03754-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X5

Quant Time: Jul 27 05:40:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

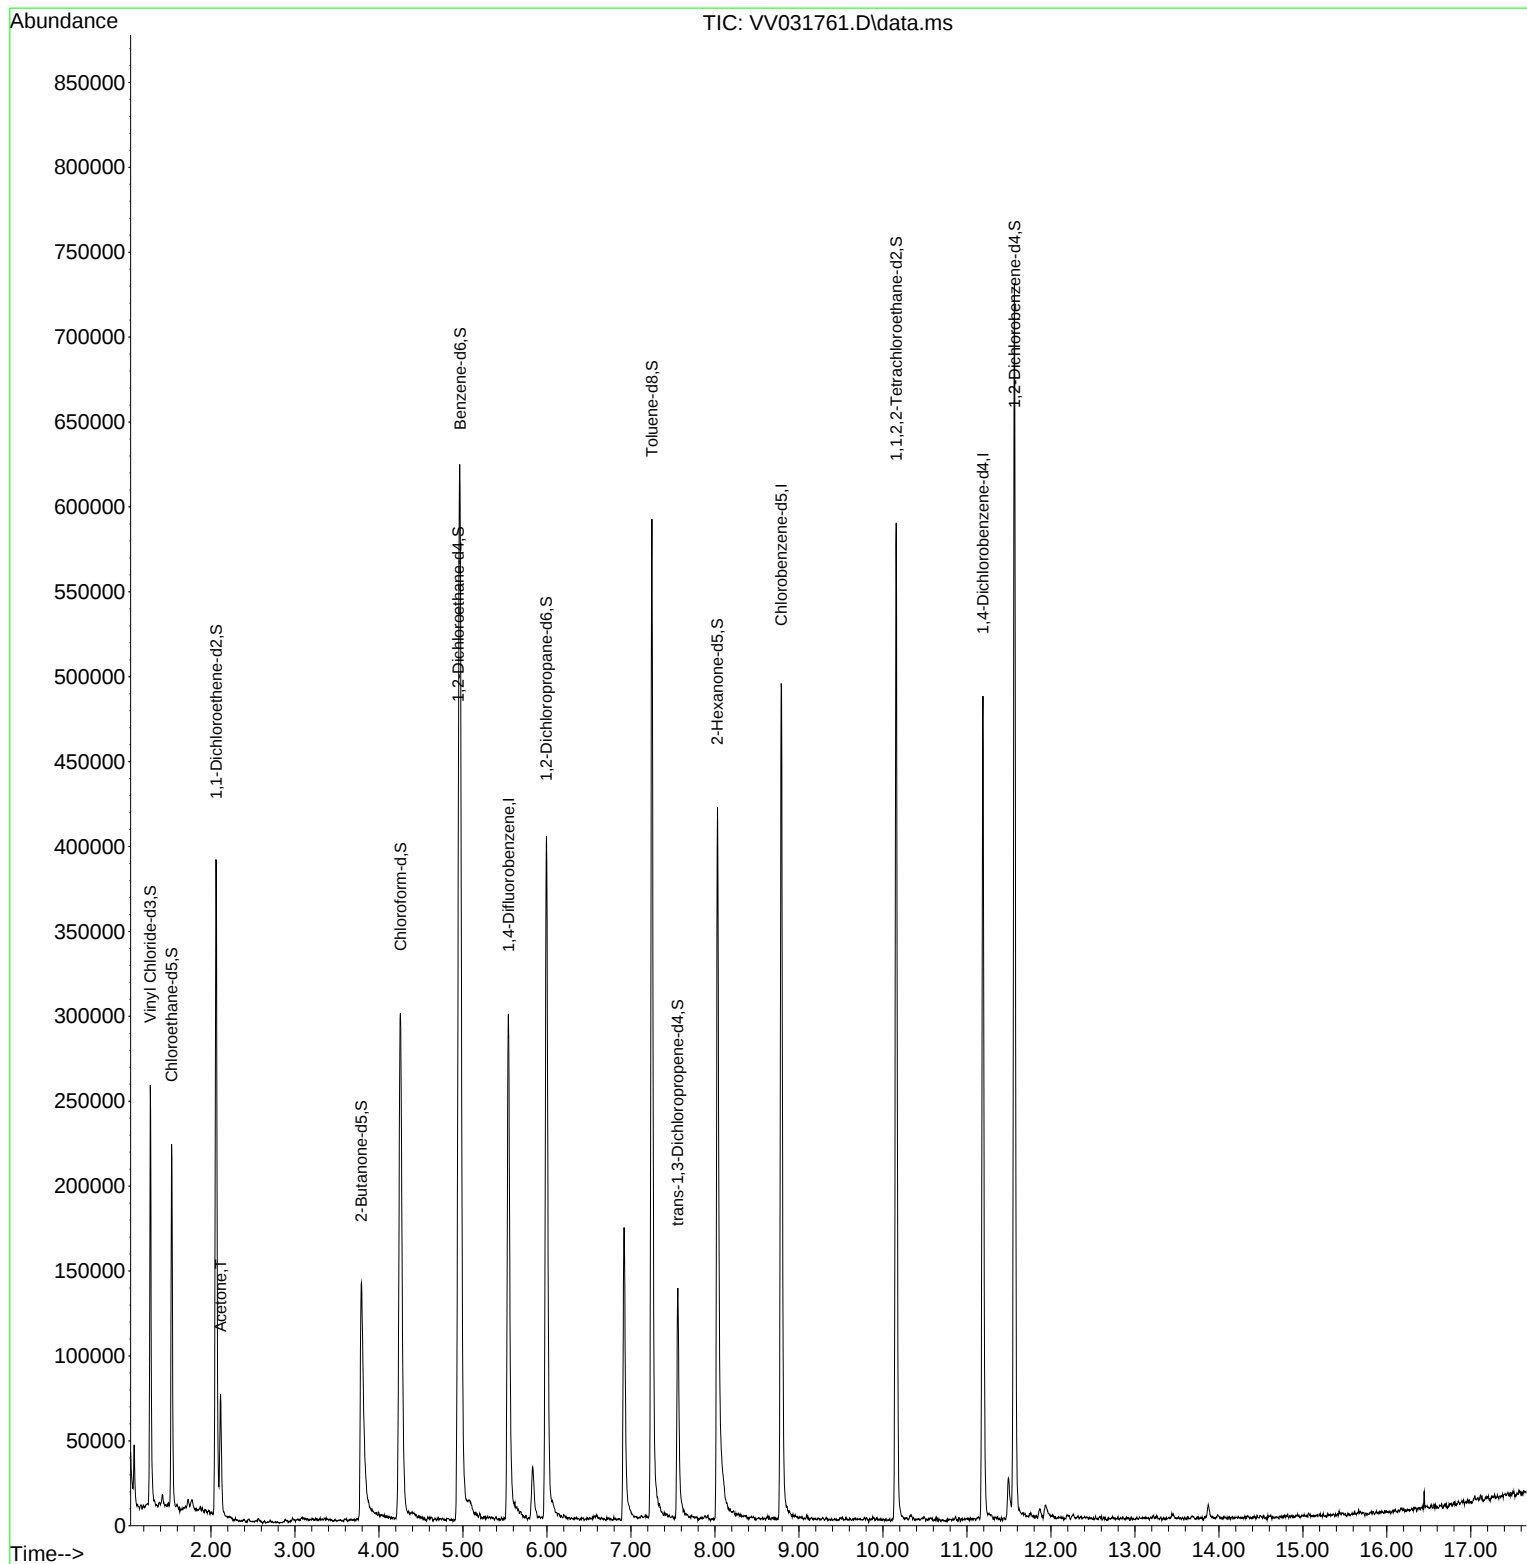

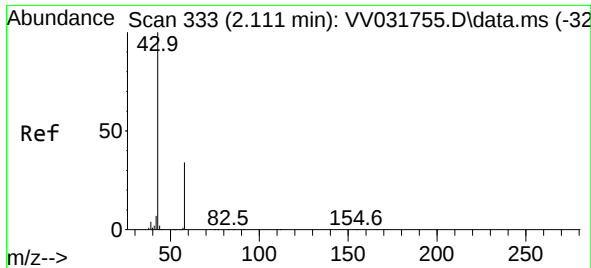

#13
Acetone
Concen: 38.793 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV031761.D
Acq: 26 Jul 2023 12:05

Instrument :
MSVOA_V
ClientSampleId :
BH2X5

Tgt Ion: 43 Resp: 64229
Ion Ratio Lower Upper
43 100
58 33.2 0.0 72.0

