

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031762.D
 Acq On : 26 Jul 2023 12:28
 Operator : SY/MD
 Sample : 03712-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2Y1

Quant Time: Jul 27 05:20:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	304982	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	330771	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	155858	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	136895	44.031	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.060%		
7) Chloroethane-d5	1.532	69	131284	46.077	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.160%		
11) 1,1-Dichloroethene-d2	2.060	65	61051	42.422	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.840%		
21) 2-Butanone-d5	3.793	46	179056	83.229	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.230%		
24) Chloroform-d	4.256	84	294472	46.068	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.140%		
26) 1,2-Dichloroethane-d4	4.947	65	184643	46.425	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.860%		
32) Benzene-d6	4.966	84	468466	44.726	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.460%		
36) 1,2-Dichloropropane-d6	5.995	67	182728	46.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.880%		
41) Toluene-d8	7.249	98	361641	41.192	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.380%		
43) trans-1,3-Dichloroprop...	7.558	79	69845	41.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.600%		
47) 2-Hexanone-d5	8.030	63	104301	70.692	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.690%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	231708	42.742	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.480%		
66) 1,2-Dichlorobenzene-d4	11.567	152	161921	51.311	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.620%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	52037	25.270	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031762.D
Acq On : 26 Jul 2023 12:28
Operator : SY/MD
Sample : 03712-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2Y1

Quant Time: Jul 27 05:20:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

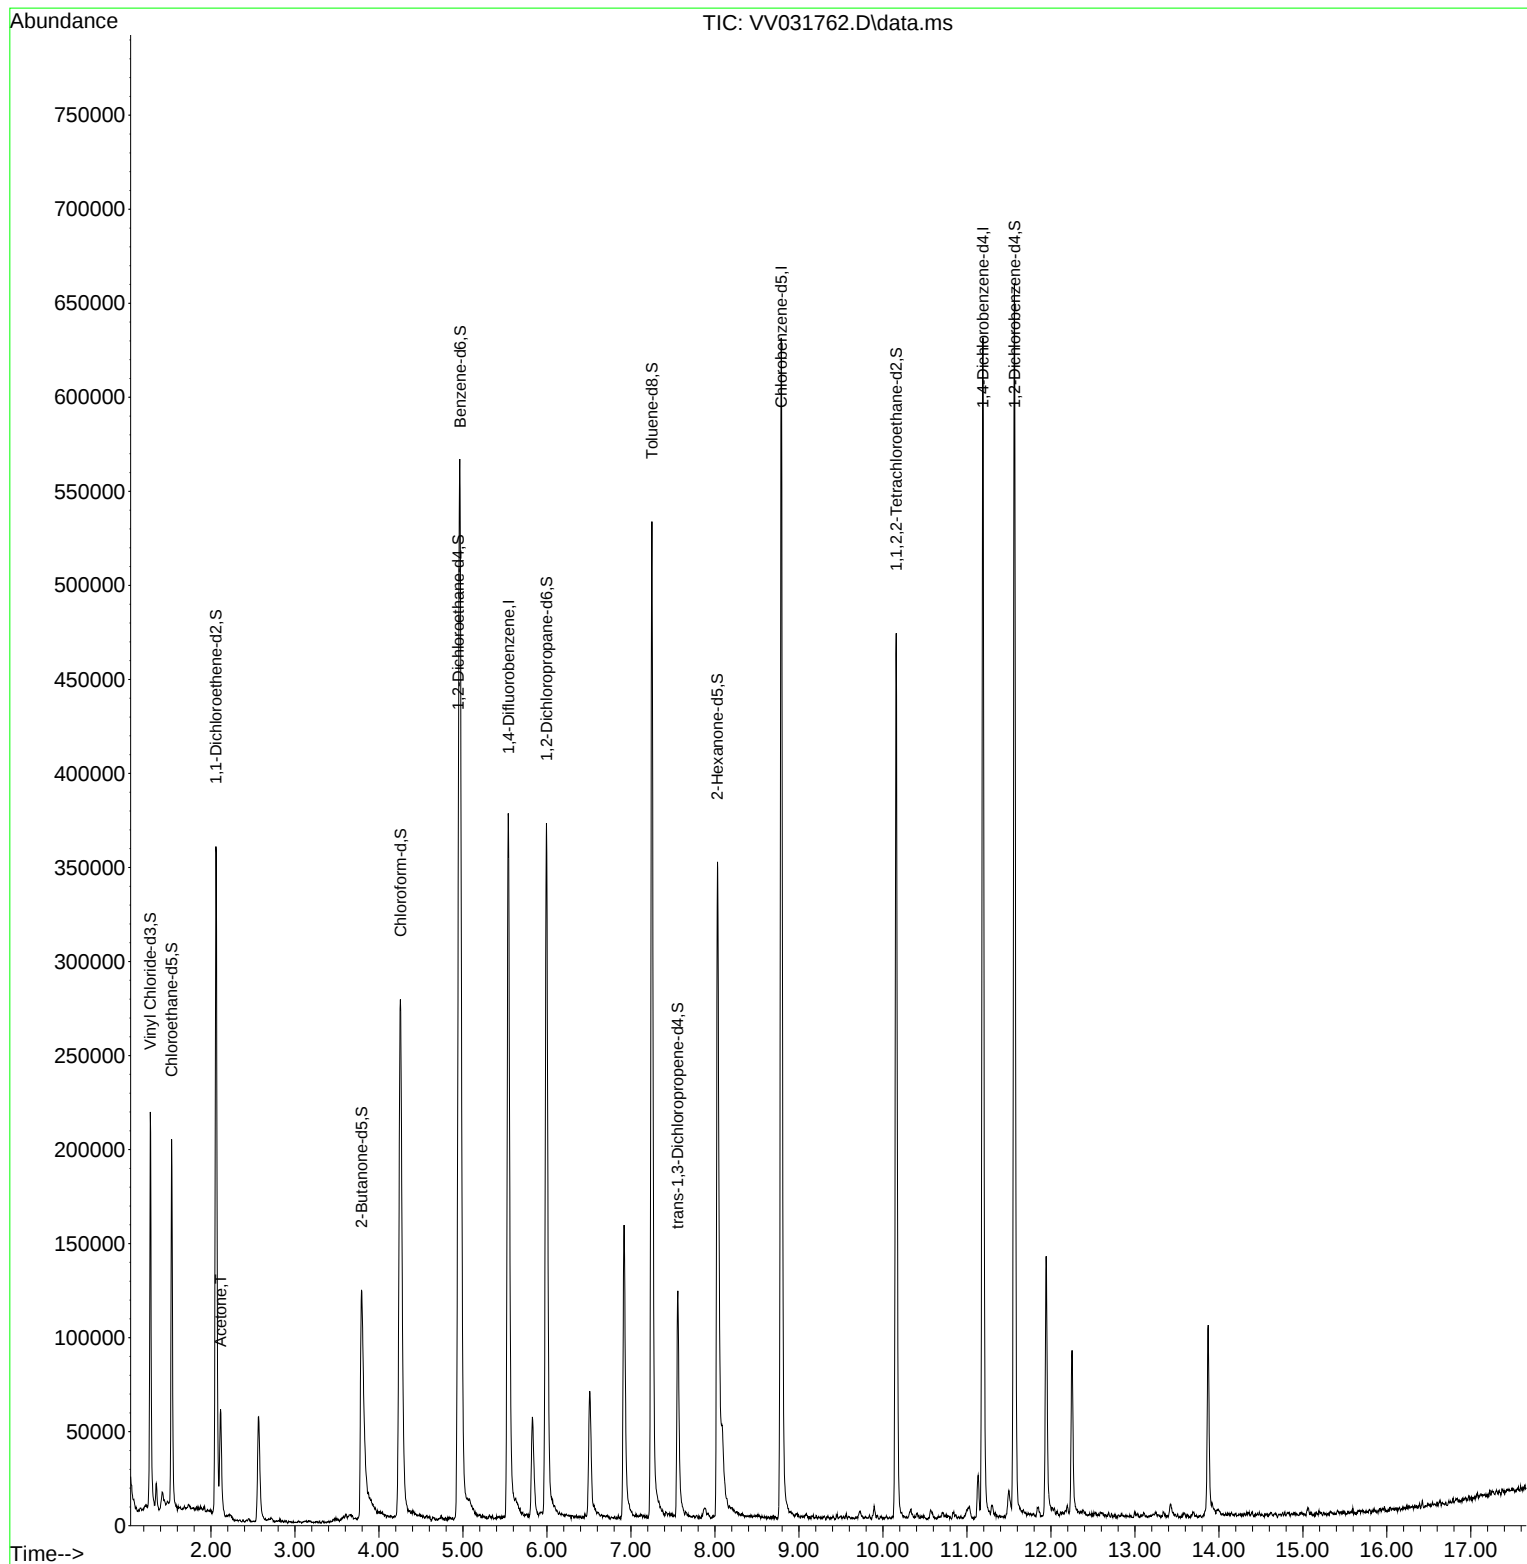

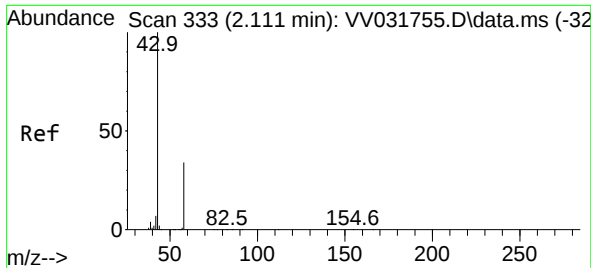

#13

Acetone

Concen: 25.270 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV031762.D


Acq: 26 Jul 2023 12:28

Instrument :

MSVOA_V

ClientSampleId :

BH2Y1

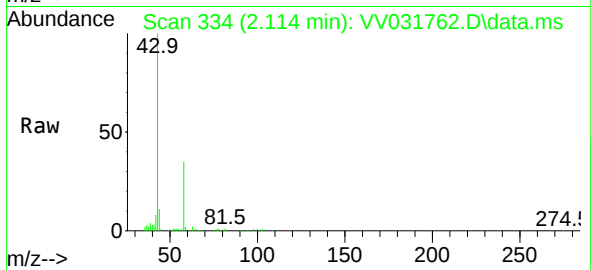

Tgt Ion: 43 Resp: 52037

Ion Ratio Lower Upper

43 100

58 35.0 0.0 72.0

