

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW072623\  
 Data File : VW031764.D  
 Acq On : 26 Jul 2023 13:15  
 Operator : SY/MD  
 Sample : 03712-08  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BH2Y5

Quant Time: Jul 27 05:20:32 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072523WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Jul 27 05:18:30 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	346289	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	356456	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	160882	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	141497	40.082	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	80.160%		
7) Chloroethane-d5	1.532	69	138250	42.734	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	85.460%		
11) 1,1-Dichloroethene-d2	2.060	65	66638	40.780	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	81.560%		
21) 2-Butanone-d5	3.790	46	214680	87.884	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	87.880%		
24) Chloroform-d	4.256	84	319156	43.974	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	87.940%		
26) 1,2-Dichloroethane-d4	4.947	65	206000	45.617	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	91.240%		
32) Benzene-d6	4.966	84	516390	45.749	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	91.500%		
36) 1,2-Dichloropropane-d6	5.992	67	199585	47.072	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	94.140%		
41) Toluene-d8	7.249	98	381439	40.316	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	80.640%		
43) trans-1,3-Dichloroprop...	7.558	79	74744	41.013	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	82.020%		
47) 2-Hexanone-d5	8.031	63	129630	81.529	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	81.530%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	241436	41.328	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	82.660%		
66) 1,2-Dichlorobenzene-d4	11.567	152	171159	52.545	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	105.080%		
-----						
Target Compounds						Qvalue
13) Acetone	2.114	43	44523	19.042	ug/L	99
-----						


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072623\  
 Data File : VV031764.D  
 Acq On : 26 Jul 2023 13:15  
 Operator : SY/MD  
 Sample : 03712-08  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BH2Y5

Quant Time: Jul 27 05:20:32 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072523WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Jul 27 05:18:30 2023  
 Response via : Initial Calibration

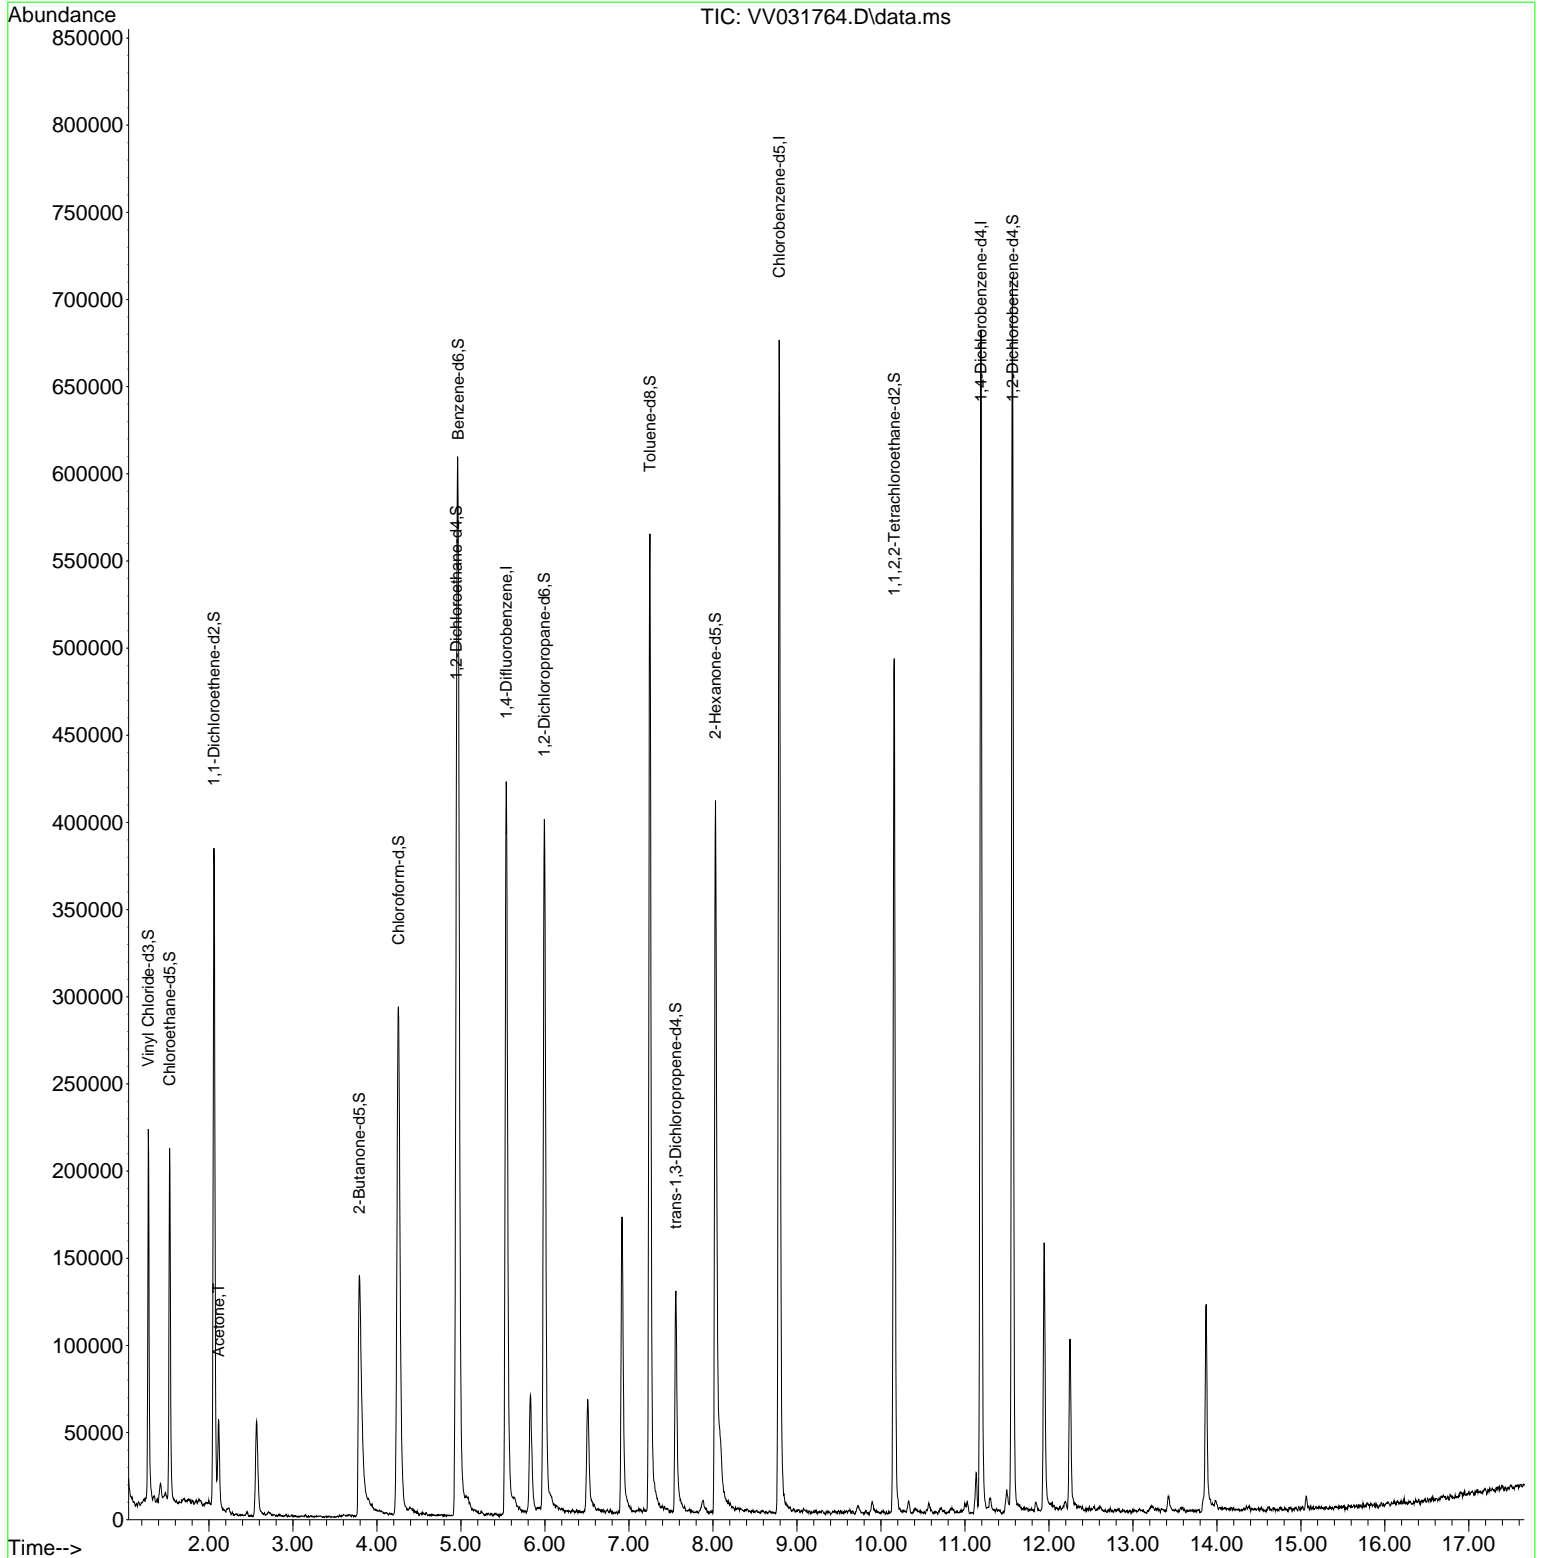

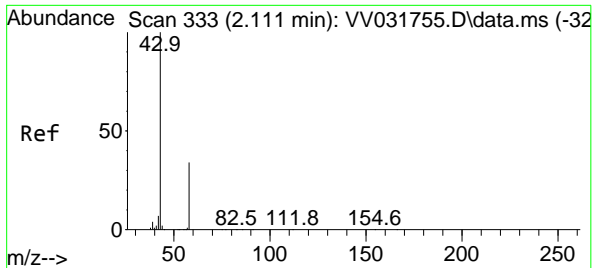

#13  
 Acetone  
 Concen: 19.042 ug/L  
 RT: 2.114 min Scan# 31  
 Delta R.T. 0.003 min  
 Lab File: VV031764.D  
 Acq: 26 Jul 2023 13:15

Instrument : MSVOA\_V  
 ClientSampleId : BH2Y5

Tgt Ion: 43 Resp: 44523  
 Ion Ratio Lower Upper  
 43 100  
 58 35.5 0.0 72.0

