

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031770.D
 Acq On : 26 Jul 2023 15:36
 Operator : SY/MD
 Sample : 03754-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2Z3

Quant Time: Jul 27 05:21:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 27 05:18:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	321843	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	342937	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	154730	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	142351	43.387	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.780%
7) Chloroethane-d5	1.532	69	137610	45.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.540%
11) 1,1-Dichloroethene-d2	2.063	65	64221	42.287	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.580%
21) 2-Butanone-d5	3.793	46	215684	95.002	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.000%
24) Chloroform-d	4.259	84	305792	45.332	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.660%
26) 1,2-Dichloroethane-d4	4.947	65	197617	47.084	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.160%
32) Benzene-d6	4.966	84	486763	44.824	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.640%
36) 1,2-Dichloropropane-d6	5.995	67	191639	46.980	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.960%
41) Toluene-d8	7.249	98	372021	40.871	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.740%
43) trans-1,3-Dichloroprop...	7.558	79	76386	43.566	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.140%
47) 2-Hexanone-d5	8.031	63	129185	84.452	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.450%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	245340	43.652	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.300%
66) 1,2-Dichlorobenzene-d4	11.567	152	168189	53.686	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.380%
Target Compounds						
13) Acetone	2.118	43	40312	18.551	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031770.D
Acq On : 26 Jul 2023 15:36
Operator : SY/MD
Sample : 03754-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2Z3

Quant Time: Jul 27 05:21:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 27 05:18:30 2023
Response via : Initial Calibration

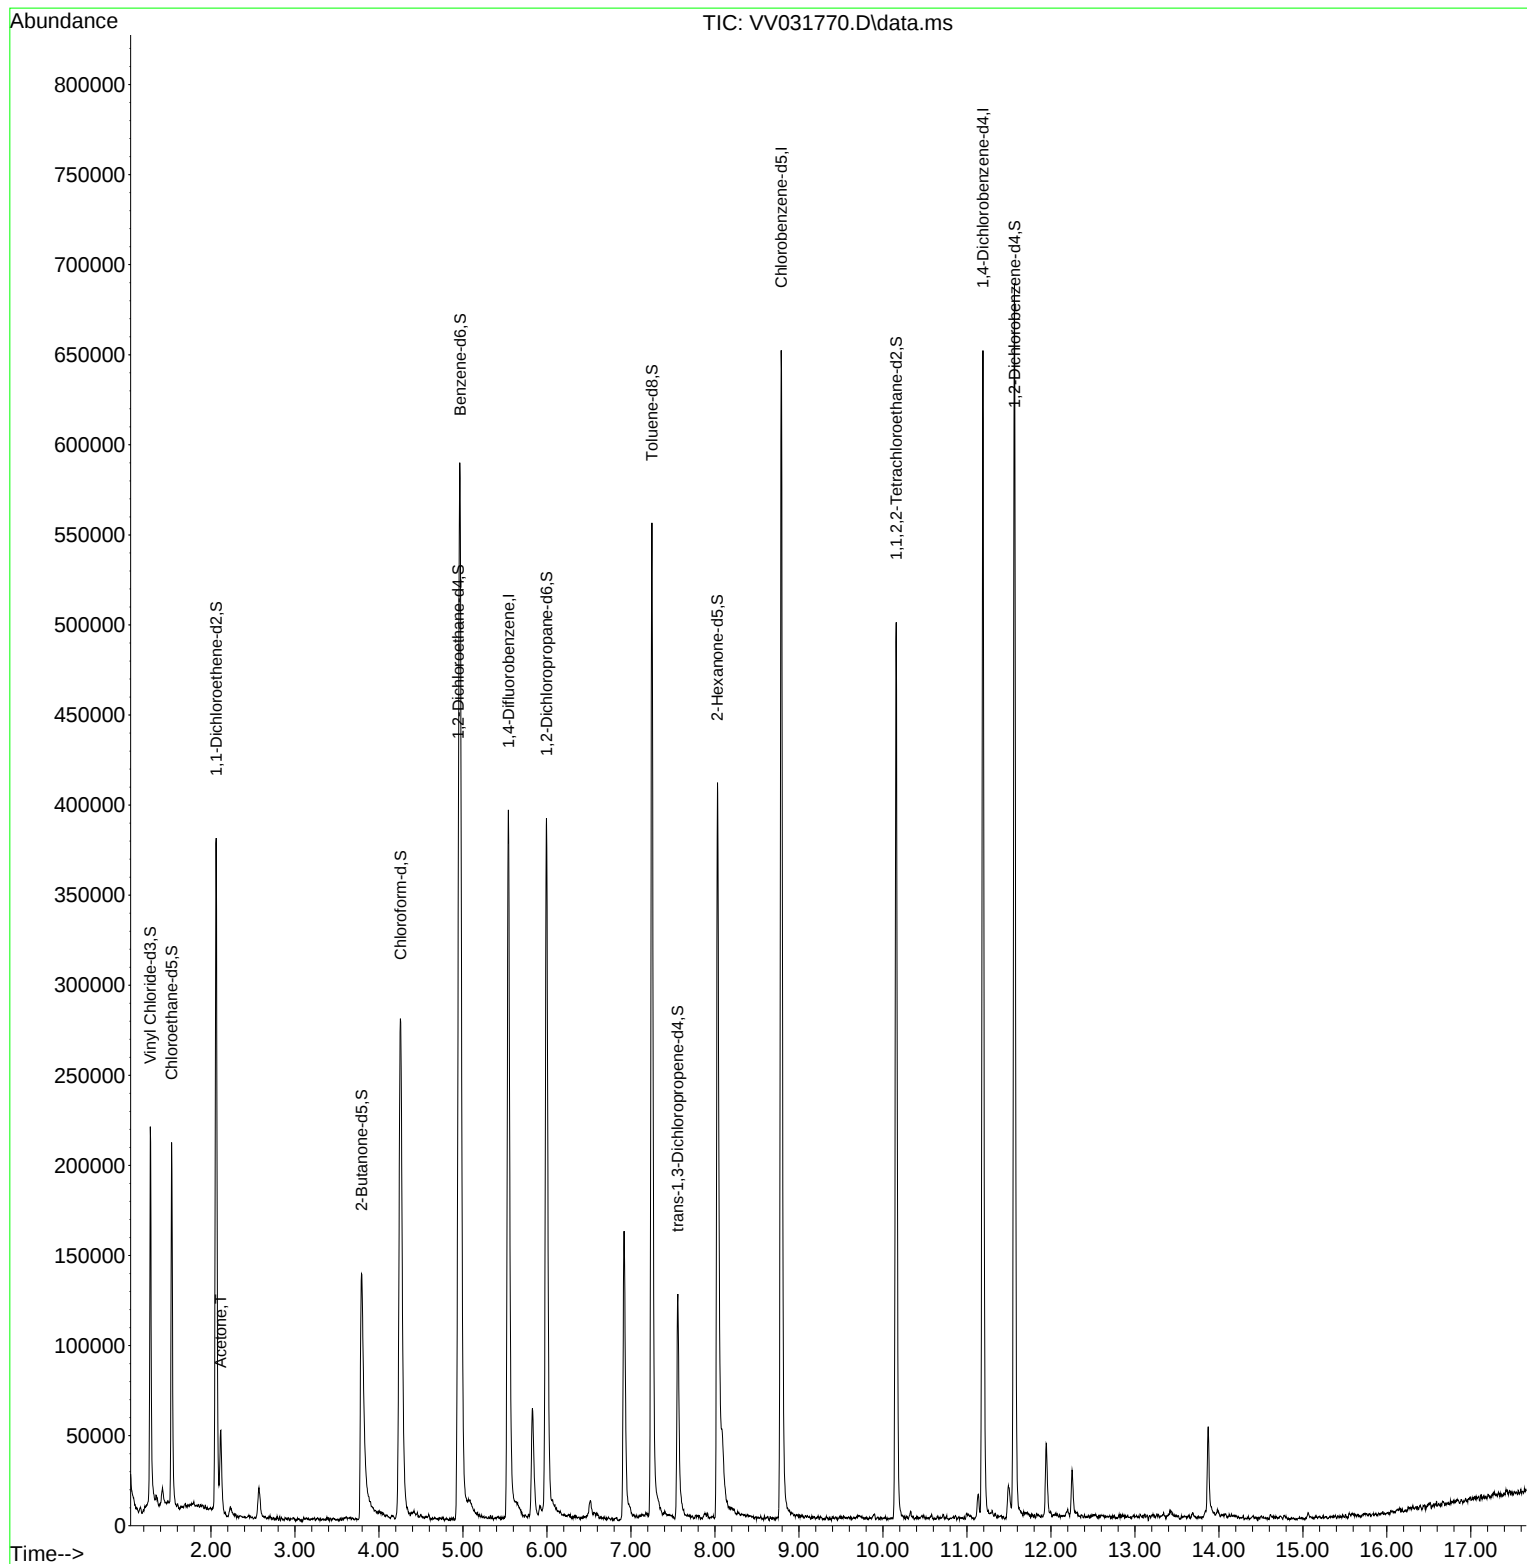

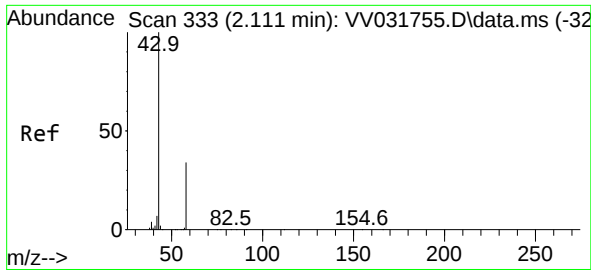

#13

Acetone

Concen: 18.551 ug/L

RT: 2.118 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV031770.D

Acq: 26 Jul 2023 15:36

Instrument :

MSVOA_V

ClientSampleId :

BH2Z3

Tgt Ion: 43 Resp: 40312

Ion Ratio Lower Upper

43 100

58 33.4 0.0 72.0

