

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031756.D
 Acq On : 26 Jul 2023 10:02
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

Signal : TIC: VV031756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	232305	248010	15.20%	2.046%
2	1.532	146	153	167	rVB	217750	259809	15.92%	2.143%
3	2.060	308	317	331	rBV	395848	573870	35.17%	4.734%
4	2.625	490	493	497	rBV5	1478	945	0.06%	0.008%
5	2.645	497	499	500	rBV2	1084	440	0.03%	0.004%
6	2.751	529	532	535	rVB4	1191	697	0.04%	0.006%
7	2.770	535	538	540	rBV4	1705	1125	0.07%	0.009%
8	2.841	557	560	562	rBV4	1684	1011	0.06%	0.008%
9	2.883	570	573	574	rBV3	1266	837	0.05%	0.007%
10	2.921	582	585	588	rBV5	1206	930	0.06%	0.008%
11	3.034	617	620	624	rBV5	1098	1151	0.07%	0.009%
12	3.072	630	632	634	rVB3	1410	528	0.03%	0.004%
13	3.092	634	638	639	rBV3	1484	879	0.05%	0.007%
14	3.124	647	648	651	rBV2	1043	402	0.02%	0.003%
15	3.182	663	666	668	rVB3	920	550	0.03%	0.005%
16	3.201	668	672	674	rBV5	1827	1472	0.09%	0.012%
17	3.262	688	691	692	rBV3	1057	478	0.03%	0.004%
18	3.304	701	704	707	rBV5	958	758	0.05%	0.006%
19	3.323	709	710	712	rVV3	1339	557	0.03%	0.005%
20	3.346	715	717	722	rVB5	1519	1003	0.06%	0.008%
21	3.404	733	735	738	rBV4	824	593	0.04%	0.005%
22	3.423	738	741	744	rVB4	1475	945	0.06%	0.008%
23	3.439	744	746	748	rVB4	940	410	0.03%	0.003%
24	3.535	774	776	780	rVB5	1266	792	0.05%	0.007%
25	3.577	788	789	791	rBV2	977	488	0.03%	0.004%
26	3.616	796	801	803	rBV4	1406	1113	0.07%	0.009%
27	3.693	821	825	826	rBV3	688	473	0.03%	0.004%
28	3.725	833	835	837	rVB3	1079	397	0.02%	0.003%
29	3.751	840	843	844	rBV3	1335	603	0.04%	0.005%
30	3.786	845	854	886	rBV	131105	365298	22.39%	3.014%
31	4.252	984	999	1022	rBV2	283997	730487	44.77%	6.027%
32	4.696	1133	1137	1140	rBV5	1820	1592	0.10%	0.013%
33	4.841	1180	1182	1183	rBV2	930	453	0.03%	0.004%
34	4.863	1186	1189	1191	rVB4	1314	774	0.05%	0.006%
35	4.876	1191	1193	1195	rBV3	1228	461	0.03%	0.004%
36	4.960	1201	1219	1245	rBV3	601780	1631520	100.00%	13.460%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031756.D
 Acq On : 26 Jul 2023 10:02
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	5.265	1312	1314	1316	rBV3	2134	818	0.05%	0.007%
38	5.539	1386	1399	1423	rBV	396444	839744	51.47%	6.928%
39	5.747	1462	1464	1466	rBV3	2130	1093	0.07%	0.009%
40	5.789	1475	1477	1478	rBV2	1853	895	0.05%	0.007%
41	5.828	1480	1489	1510	rVB2	42282	90895	5.57%	0.750%
42	5.992	1528	1540	1561	rBV	387235	800811	49.08%	6.607%
43	6.246	1617	1619	1624	rBV4	1787	1380	0.08%	0.011%
44	6.336	1645	1647	1650	rBV4	1035	718	0.04%	0.006%
45	6.436	1674	1678	1681	rBV6	1513	1222	0.07%	0.010%
46	6.555	1708	1715	1716	rBV5	1962	2258	0.14%	0.019%
47	6.654	1743	1746	1750	rVB6	1256	1043	0.06%	0.009%
48	6.674	1750	1752	1758	rBV7	1153	1179	0.07%	0.010%
49	6.747	1772	1775	1776	rBV2	1147	683	0.04%	0.006%
50	6.841	1801	1804	1806	rBV4	1631	978	0.06%	0.008%
51	6.918	1817	1828	1851	rBV	164354	324622	19.90%	2.678%
52	7.246	1919	1930	1958	rBV	559561	1029643	63.11%	8.495%
53	7.554	2018	2026	2048	rBV	126009	230536	14.13%	1.902%
54	7.763	2089	2091	2093	rBV2	1688	837	0.05%	0.007%
55	7.786	2093	2098	2103	rBV7	2864	3251	0.20%	0.027%
56	7.963	2149	2153	2155	rBV5	1300	966	0.06%	0.008%
57	8.030	2164	2174	2209	rBV	395751	809307	49.60%	6.677%
58	8.484	2311	2315	2316	rBV3	1874	1306	0.08%	0.011%
59	8.529	2327	2329	2331	rVB3	1739	647	0.04%	0.005%
60	8.789	2397	2410	2430	rBV	672467	1116770	68.45%	9.213%
61	9.448	2613	2615	2618	rBV3	830	617	0.04%	0.005%
62	9.519	2635	2637	2639	rBV2	1121	580	0.04%	0.005%
63	9.596	2659	2661	2664	rBV4	1281	870	0.05%	0.007%
64	9.657	2678	2680	2681	rBV2	1089	495	0.03%	0.004%
65	9.725	2697	2701	2703	rBV4	1706	1214	0.07%	0.010%
66	9.738	2703	2705	2707	rVV2	1297	604	0.04%	0.005%
67	9.796	2721	2723	2727	rBV5	1809	1120	0.07%	0.009%
68	9.915	2759	2760	2762	rBV2	1082	482	0.03%	0.004%
69	9.963	2772	2775	2777	rVB4	763	400	0.02%	0.003%
70	10.079	2809	2811	2815	rBV5	907	551	0.03%	0.005%
71	10.156	2824	2835	2859	rBV	529005	851777	52.21%	7.027%
72	10.442	2922	2924	2926	rBV3	1614	740	0.05%	0.006%
73	10.564	2960	2962	2964	rBV3	959	482	0.03%	0.004%
74	10.641	2983	2986	2990	rBV4	1290	1133	0.07%	0.009%
75	10.693	2998	3002	3005	rBV6	2531	1663	0.10%	0.014%
76	10.725	3010	3012	3014	rVB3	1027	381	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031756.D
 Acq On : 26 Jul 2023 10:02
 Operator : SY/MD
 Sample : VV0726WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	10.744	3016	3018	3021	rBV3	1835	988	0.06%	0.008%
78	10.760	3021	3023	3024	rBV	1184	540	0.03%	0.004%
79	10.924	3072	3074	3076	rBV3	1389	606	0.04%	0.005%
80	11.088	3123	3125	3127	rBV3	1120	530	0.03%	0.004%
81	11.130	3132	3138	3140	rBV5	2842	2989	0.18%	0.025%
82	11.191	3146	3157	3173	rBV	656547	1010882	61.96%	8.340%
83	11.445	3232	3236	3239	rBV6	2212	1551	0.10%	0.013%
84	11.496	3248	3252	3254	rBV6	1002	790	0.05%	0.007%
85	11.564	3260	3273	3294	rBV	697996	1121423	68.73%	9.252%
86	11.924	3381	3385	3386	rBV4	1365	908	0.06%	0.007%
87	12.435	3542	3544	3545	rBV2	1716	570	0.03%	0.005%
88	12.467	3551	3554	3555	rBV2	878	456	0.03%	0.004%
89	12.648	3607	3610	3613	rBV2	1444	979	0.06%	0.008%
90	12.664	3613	3615	3617	rBV3	1561	778	0.05%	0.006%
91	12.702	3625	3627	3631	rBV5	1241	819	0.05%	0.007%
92	12.959	3705	3707	3708	rBV2	1690	654	0.04%	0.005%
93	13.201	3778	3782	3783	rBV4	3744	2252	0.14%	0.019%
94	13.291	3808	3810	3811	rBV2	1405	600	0.04%	0.005%
95	13.361	3829	3832	3836	rBV4	2007	1810	0.11%	0.015%
96	13.686	3924	3933	3940	rBV4	5946	9444	0.58%	0.078%
97	14.094	4056	4060	4062	rBV3	1435	1313	0.08%	0.011%
98	14.210	4093	4096	4099	rBV5	2144	1584	0.10%	0.013%
99	14.342	4134	4137	4139	rBV4	2360	1322	0.08%	0.011%
100	14.512	4189	4190	4193	rBV3	1360	749	0.05%	0.006%




Sum of corrected areas: 12121099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031756.D
Acq On : 26 Jul 2023 10:02
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

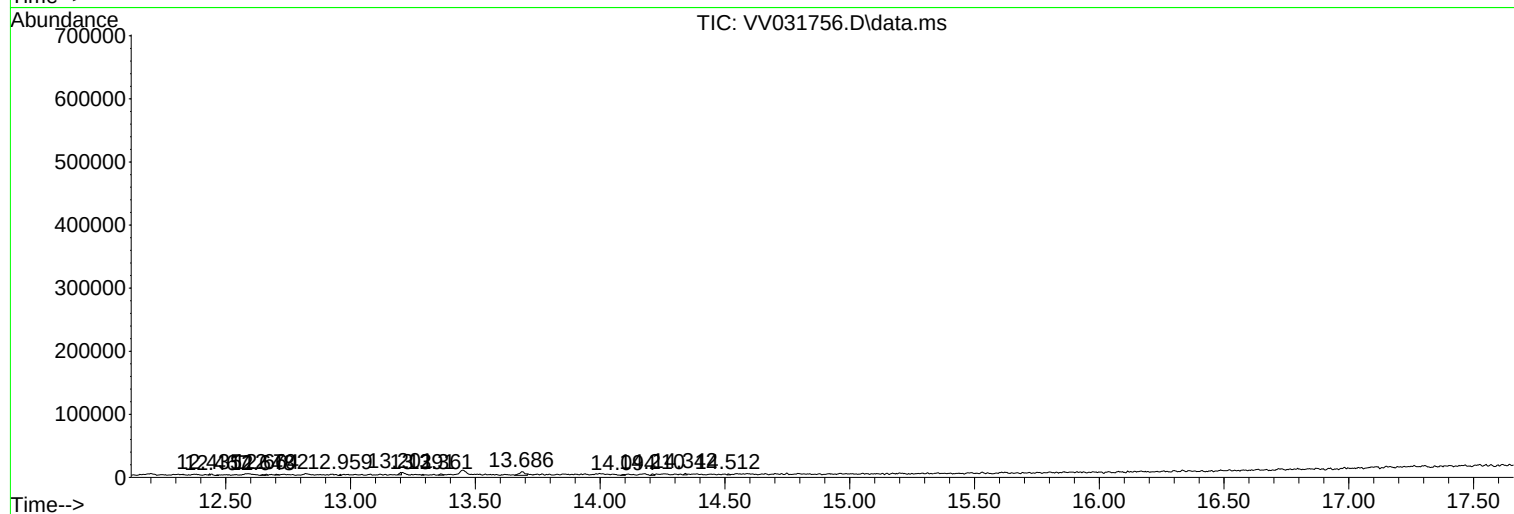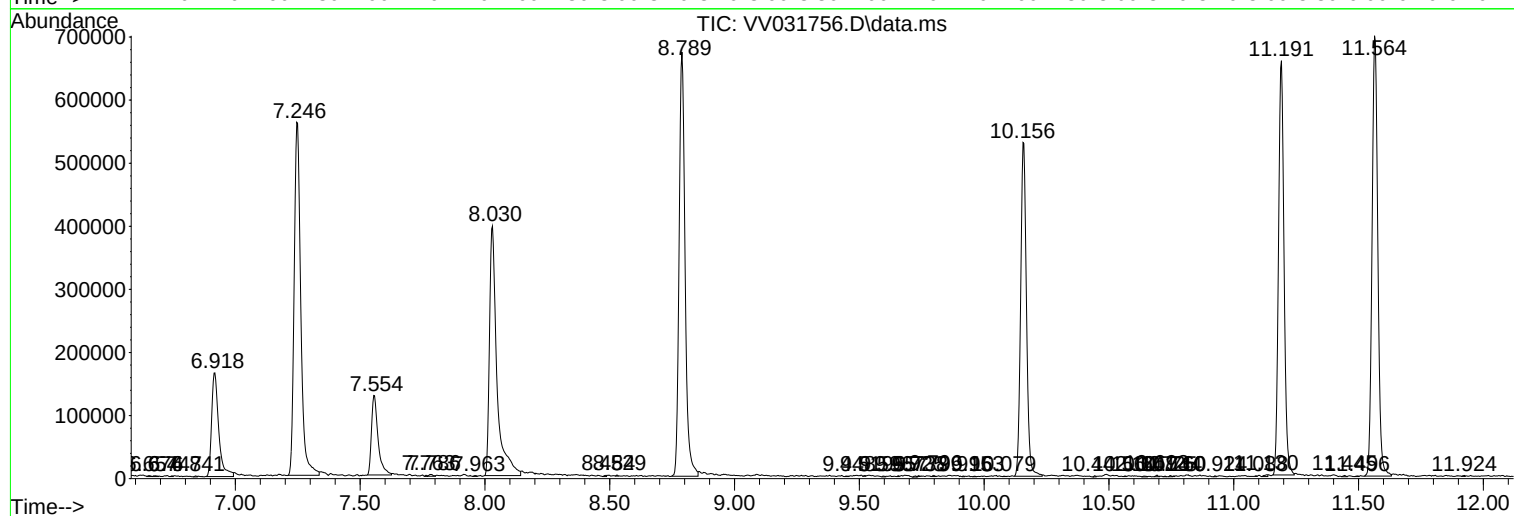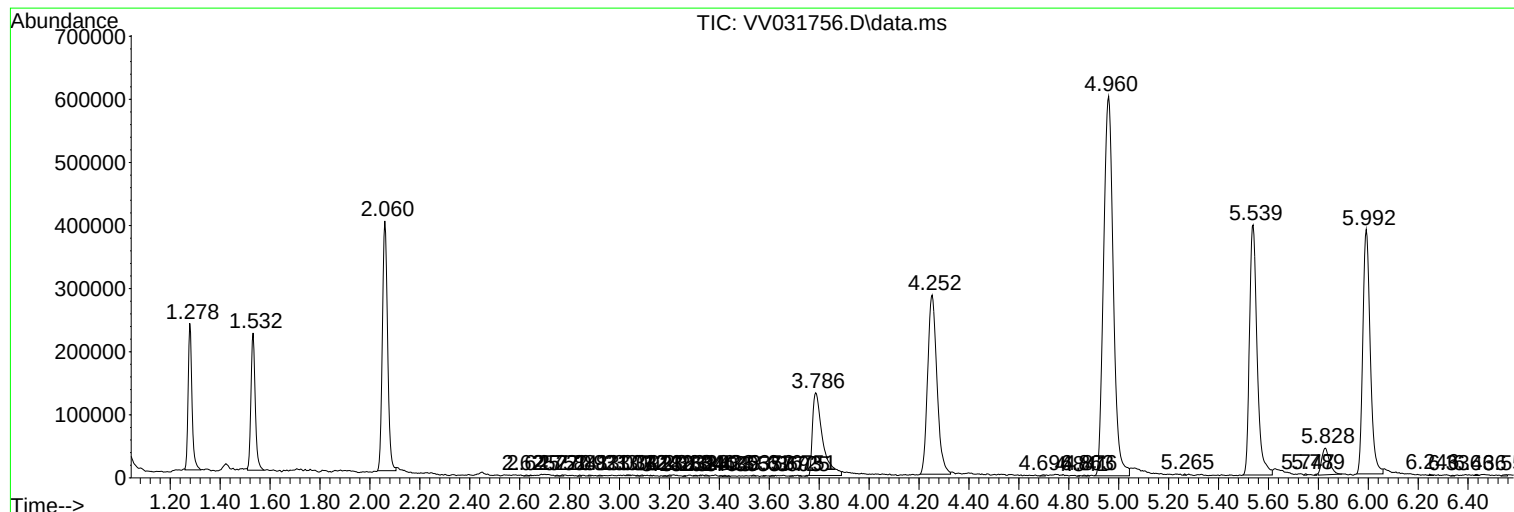

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031756.D
Acq On : 26 Jul 2023 10:02
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031756.D
Acq On : 26 Jul 2023 10:02
Operator : SY/MD
Sample : VV0726WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------